


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120618\
Data File : VV008853.D
Acq On : 06 Dec 2018 10:07
Operator : SY/MD
Sample : BFB56
Misc : 5.00g/10.0 mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM120618S.M
Title : VOC Analysis
Last Update : Wed Dec 12 04:31:38 2018

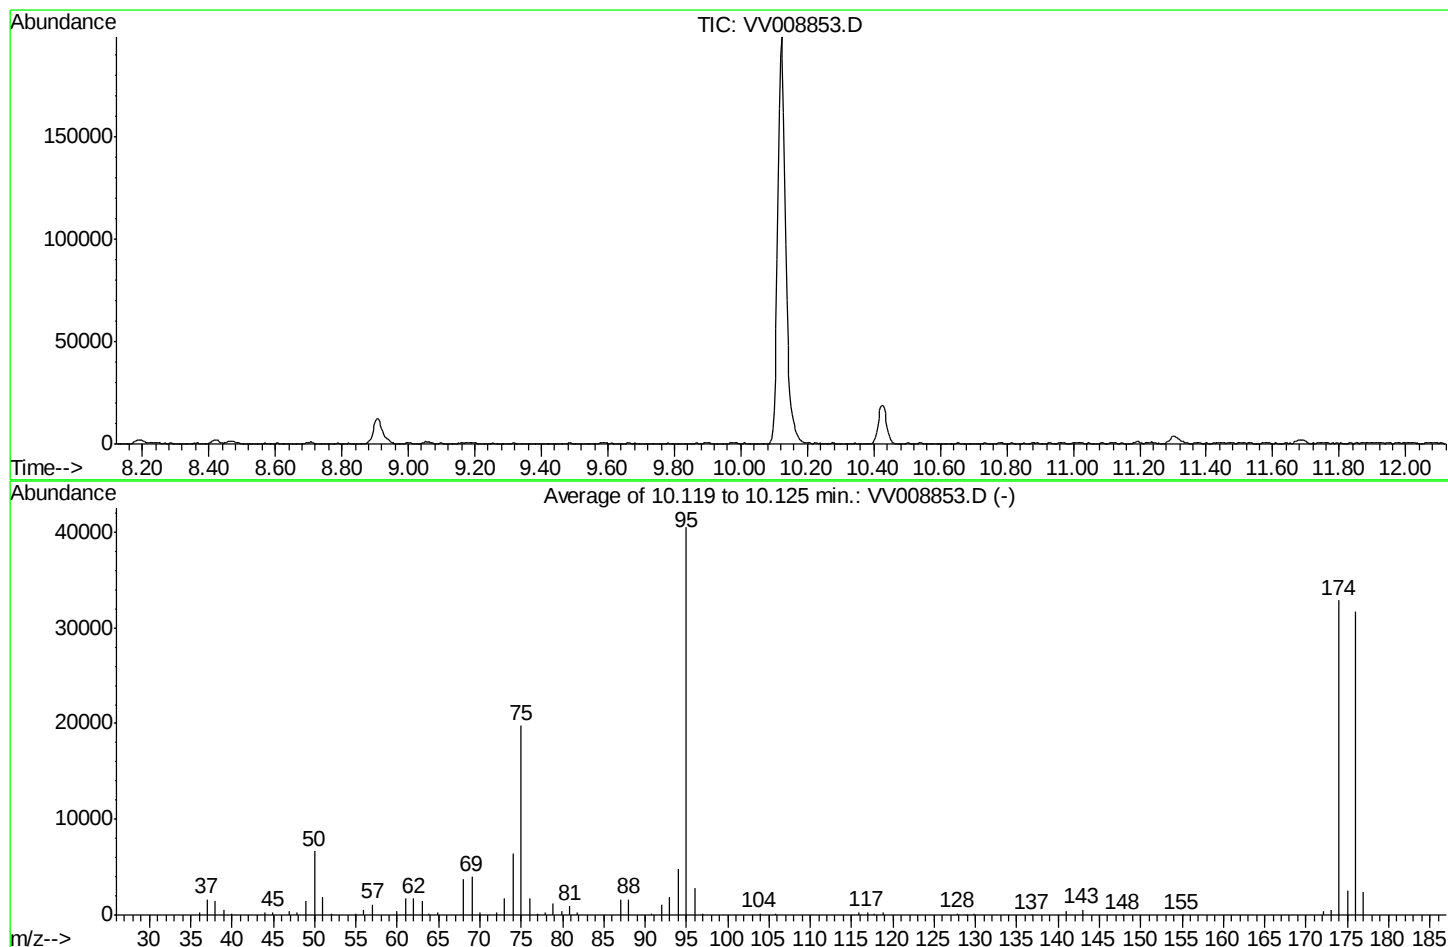

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	6672	PASS
75	95	30	80	48.8	19752	PASS
95	95	100	100	100.0	40504	PASS
96	95	5	9	7.0	2835	PASS
173	174	0.00	2	1.5	507	PASS
174	95	50	120	81.2	32885	PASS
175	174	5	9	7.8	2581	PASS
176	174	95	101	96.4	31698	PASS
177	176	5	9	7.6	2410	PASS

m/z	Abundance
36.00	250.0
37.00	1732.0
38.00	1501.0
39.00	521.0
39.90	188.0
43.90	431.0
45.00	264.0
46.90	418.0
47.90	286.0
49.00	1437.0
50.00	6779.0
51.00	1785.0
54.90	103.0
55.90	554.0
57.00	1098.0
59.90	353.0
61.00	1647.0
62.00	1796.0
63.00	1530.0
63.90	221.0
64.90	251.0
68.00	3789.0
69.00	4014.0
70.00	312.0
72.00	235.0
73.00	1742.0
74.00	6472.0
75.00	19776.0
76.00	1772.0
77.00	185.0
78.00	169.0
78.90	1185.0
79.90	325.0
80.90	930.0
81.80	286.0
87.00	1588.0
88.00	1565.0
90.80	129.0
92.00	1219.0
93.00	1849.0
94.00	4725.0
95.00	39832.0
96.00	3009.0
97.00	157.0
103.90	176.0
105.80	165.0
115.90	264.0
116.90	343.0
117.90	107.0
118.80	224.0
127.80	180.0
128.90	106.0
129.80	148.0
140.90	363.0
143.00	518.0
172.10	414.0
173.10	546.0
174.00	31976.0
175.00	2460.0
176.00	30792.0
177.00	2397.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
43.80	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	251.0
37.00	1439.0
38.00	1487.0
38.90	575.0
39.90	132.0
44.00	410.0
44.90	306.0
46.90	443.0
47.90	261.0
49.00	1490.0
50.00	6262.0
51.00	1877.0
52.10	122.0
54.90	140.0
56.00	499.0
57.00	1010.0
59.90	450.0
61.00	1709.0
62.00	1615.0
63.00	1441.0
63.80	144.0
64.90	221.0
68.00	3657.0
69.00	3733.0
70.00	293.0
72.10	217.0
73.00	1785.0
74.00	6039.0
75.00	19040.0
76.00	1698.0
76.90	214.0
77.90	237.0
78.90	1130.0
79.90	377.0
80.90	1003.0
81.90	259.0
87.00	1614.0
88.00	1555.0
90.80	145.0
92.00	998.0
93.00	1799.0
94.00	4687.0
95.00	39880.0
96.00	2600.0
103.90	175.0
105.80	138.0
115.80	171.0
116.90	298.0
117.80	152.0
118.90	202.0
127.90	148.0
129.80	104.0
136.80	107.0
141.00	430.0
142.90	542.0
147.80	110.0
172.00	370.0
173.10	454.0
174.00	32704.0
175.00	2604.0
176.00	31608.0
177.00	2304.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	245.0
37.00	1688.0
38.00	1620.0
39.00	554.0
39.90	153.0
44.00	449.0
44.90	299.0
46.90	427.0
47.90	297.0
49.00	1559.0
50.00	6975.0
51.00	1927.0
52.00	108.0
54.90	138.0
55.90	533.0
57.00	1127.0
59.90	432.0
61.00	1724.0
62.00	1799.0
63.00	1556.0
63.80	185.0
64.90	243.0
68.00	3885.0
69.00	4154.0
70.00	328.0
72.00	234.0
73.00	1898.0
74.00	6568.0
75.00	20440.0
76.00	1783.0
77.00	197.0
78.00	234.0
78.90	1216.0
79.90	381.0
80.90	974.0
81.80	305.0
87.00	1634.0
88.00	1726.0
90.80	132.0
92.00	1181.0
93.00	1957.0
94.00	4929.0
95.00	41800.0
96.00	2898.0
97.00	131.0
103.90	198.0
105.80	165.0
115.80	235.0
116.90	347.0
117.70	140.0
118.90	216.0
127.80	183.0
129.90	124.0
141.00	420.0
143.00	571.0
155.00	105.0
172.00	422.0
173.00	522.0
174.00	33976.0
175.00	2681.0
176.00	32696.0
177.00	2529.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56