
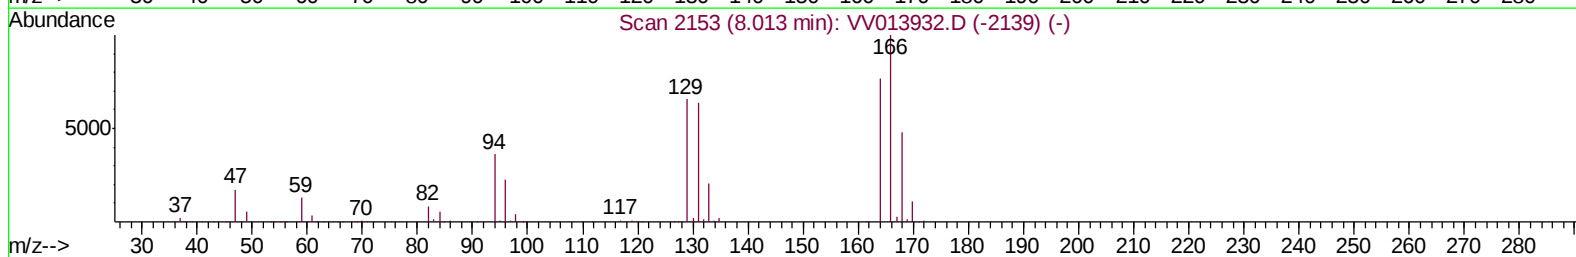
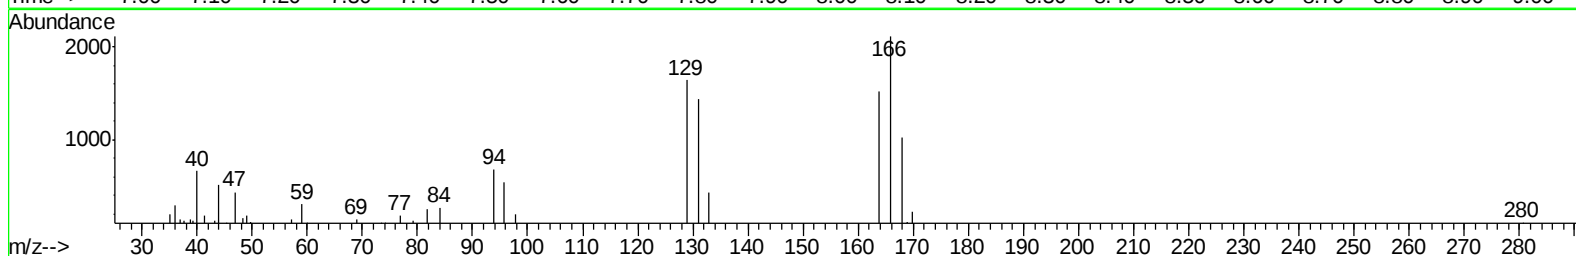


Data File : VV013936.D
Acq On : 06 Dec 2019 12:34
Operator : SY/MD
Sample : K6165-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Dec 07 01:41:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

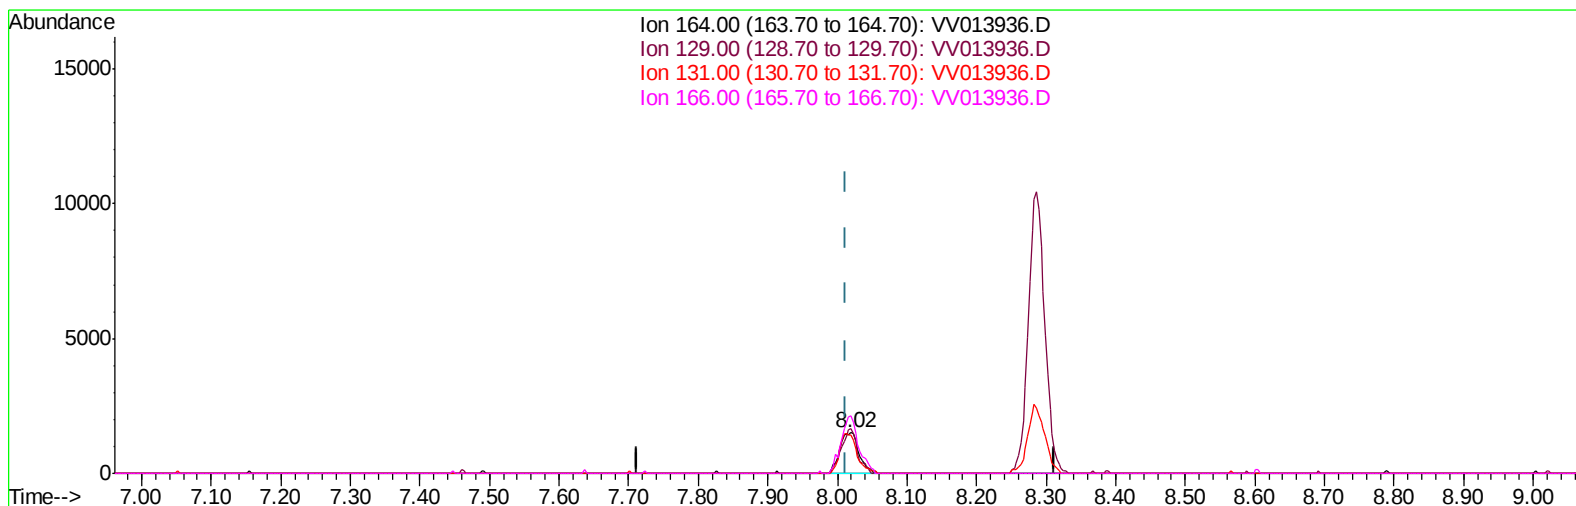

TIC: VV013936.D

(46) Tetrachloroethene (T)

8.019min (+0.006) 1.02ug/L m

response 2867

Ion	Exp%	Act%
164.00	100	100
129.00	88.20	108.30
131.00	83.50	94.86
166.00	133.50	139.26