
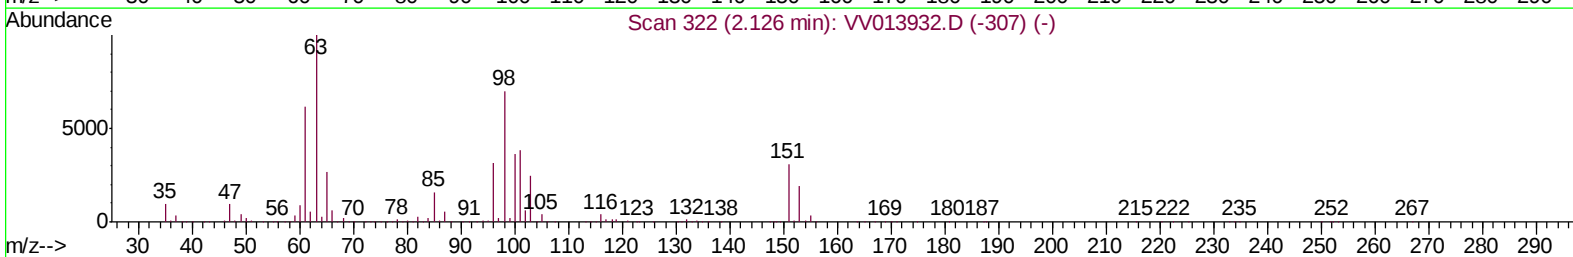
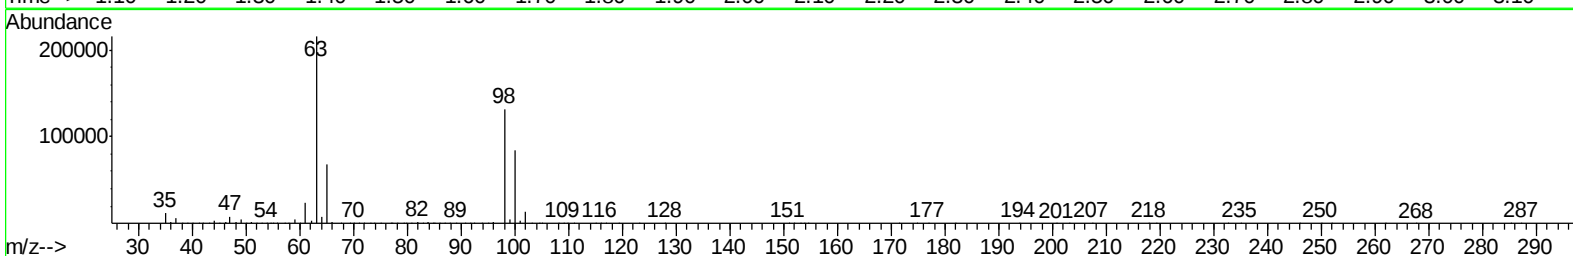


Data File : VV013941.D
Acq On : 06 Dec 2019 14:37
Operator : SY/MD
Sample : K6190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 07 01:42:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

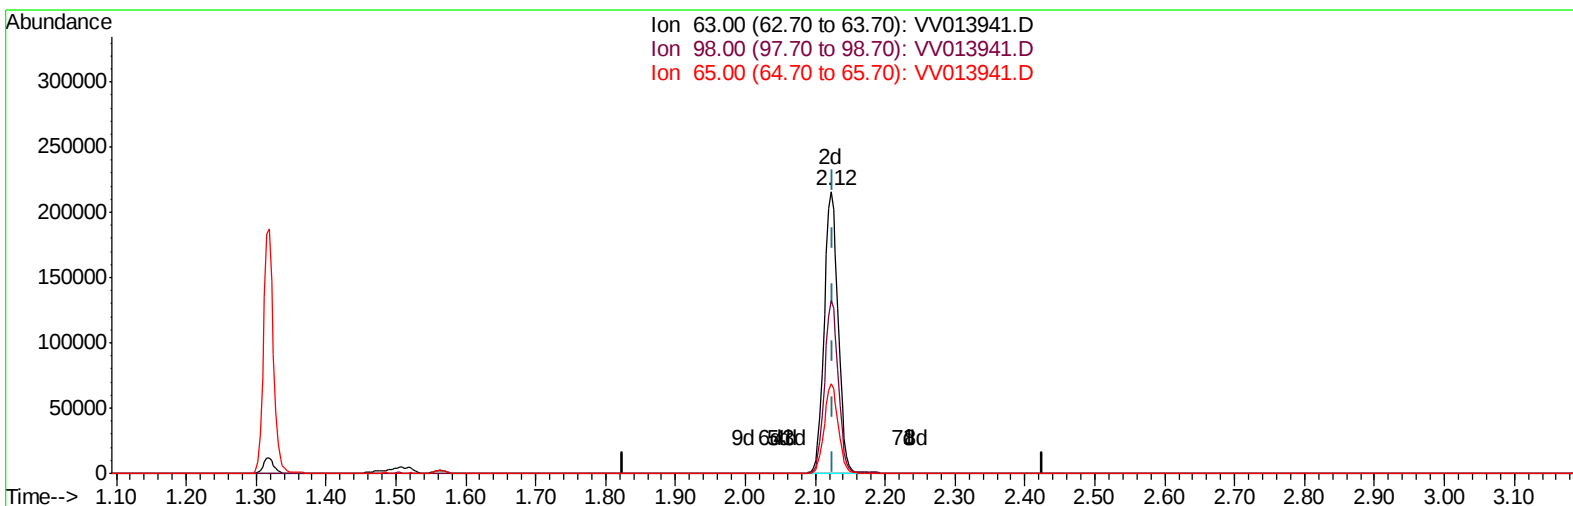

TIC: VV013941.D

(11) 1,1-Dichloroethene-d2 (S)

2.122min (-0.003) 43.56ug/L m

response 300451

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	0.02#
65.00	23.60	0.01#
0.00	0.00	0.00