
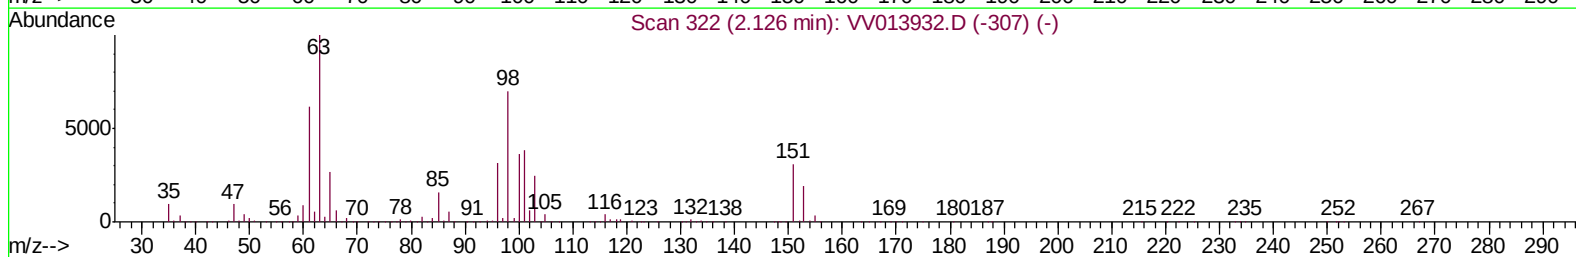
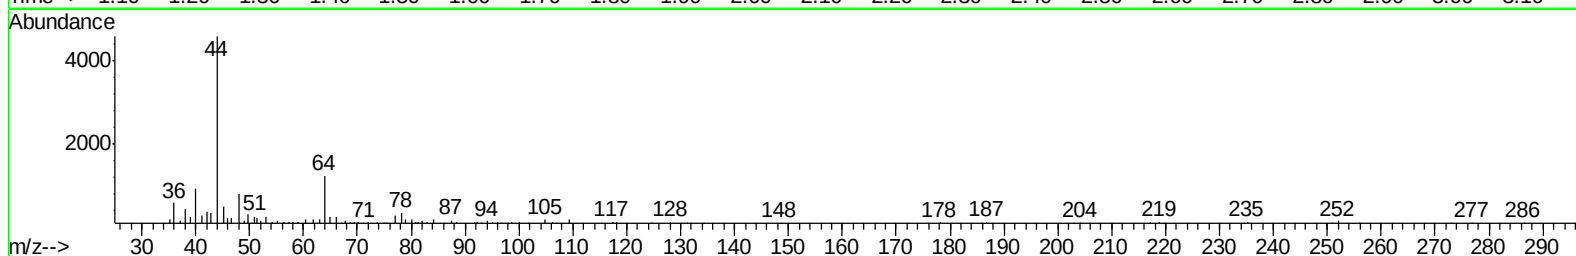


Data File : VV013947.D  
Acq On : 06 Dec 2019 18:45  
Operator : SY/MD  
Sample : K6170-14  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 07 01:43:32 2019  
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_V\METHOD\SOMVLM120219WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Dec 07 01:39:07 2019  
Response via : Initial Calibration

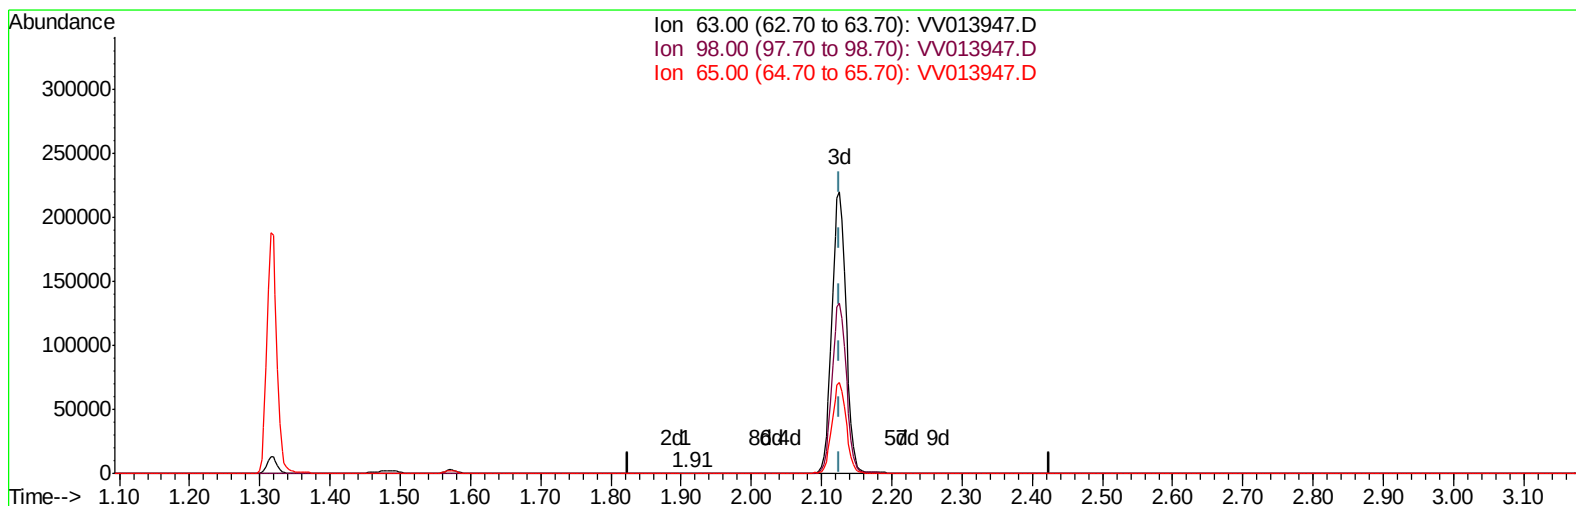

TIC: VV013947.D

(11) 1,1-Dichloroethene-d2 (S)

1.907min (-0.219) 0.03ug/L

response 225

| Ion   | Exp%  | Act%  |
|-------|-------|-------|
| 63.00 | 100   | 100   |
| 98.00 | 79.40 | 70.22 |
| 65.00 | 23.60 | 22.22 |
| 0.00  | 0.00  | 0.00  |