
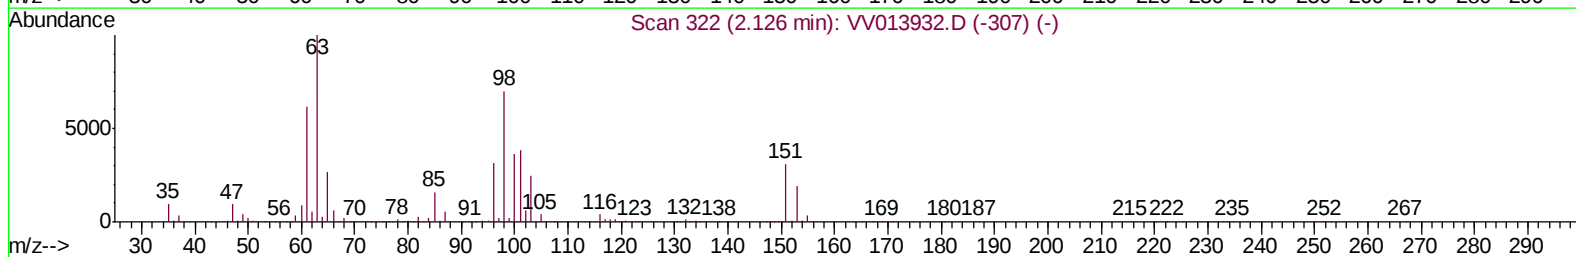
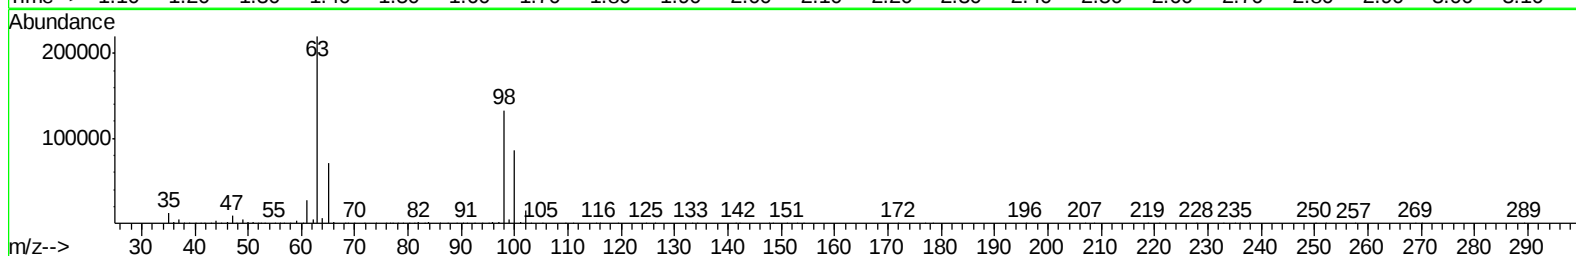


Data File : VV013947.D
Acq On : 06 Dec 2019 18:45
Operator : SY/MD
Sample : K6170-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 07 01:43:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

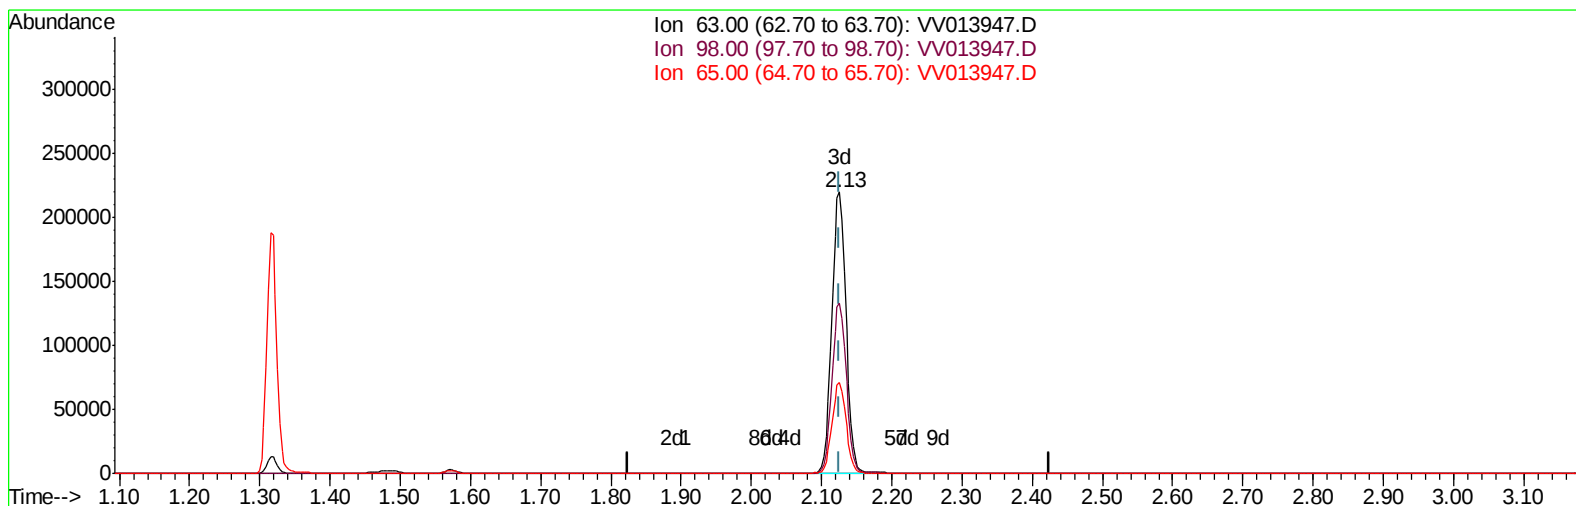

TIC: VV013947.D

(11) 1,1-Dichloroethene-d2 (S)

2.126min (+0.000) 37.84ug/L m

response 305712

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	0.05#
65.00	23.60	0.02#
0.00	0.00	0.00