
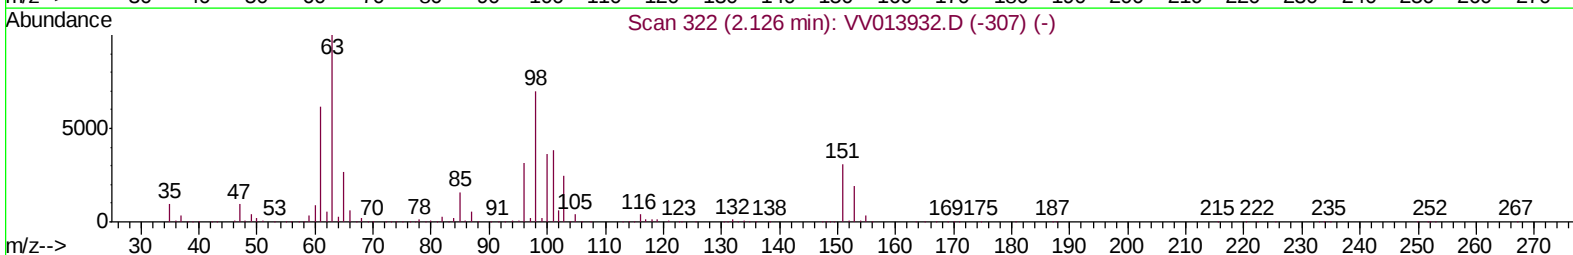
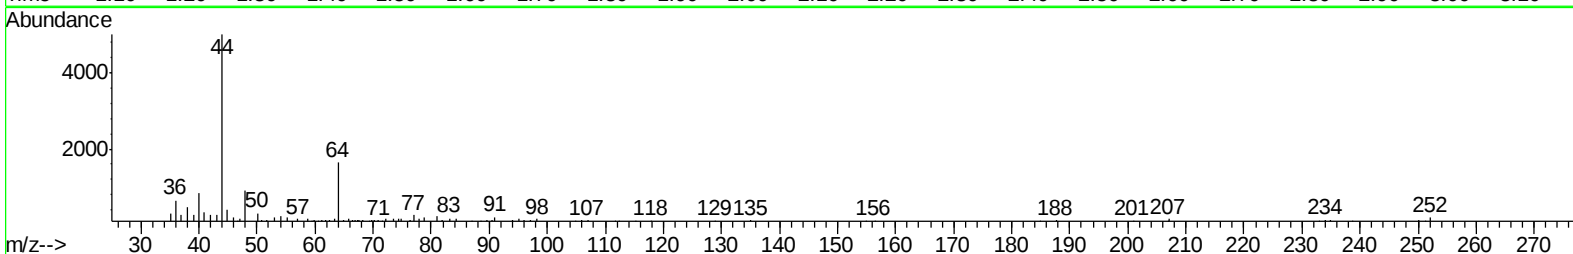


Data File : VV013948.D
Acq On : 06 Dec 2019 19:10
Operator : SY/MD
Sample : K6170-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Dec 07 01:43:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

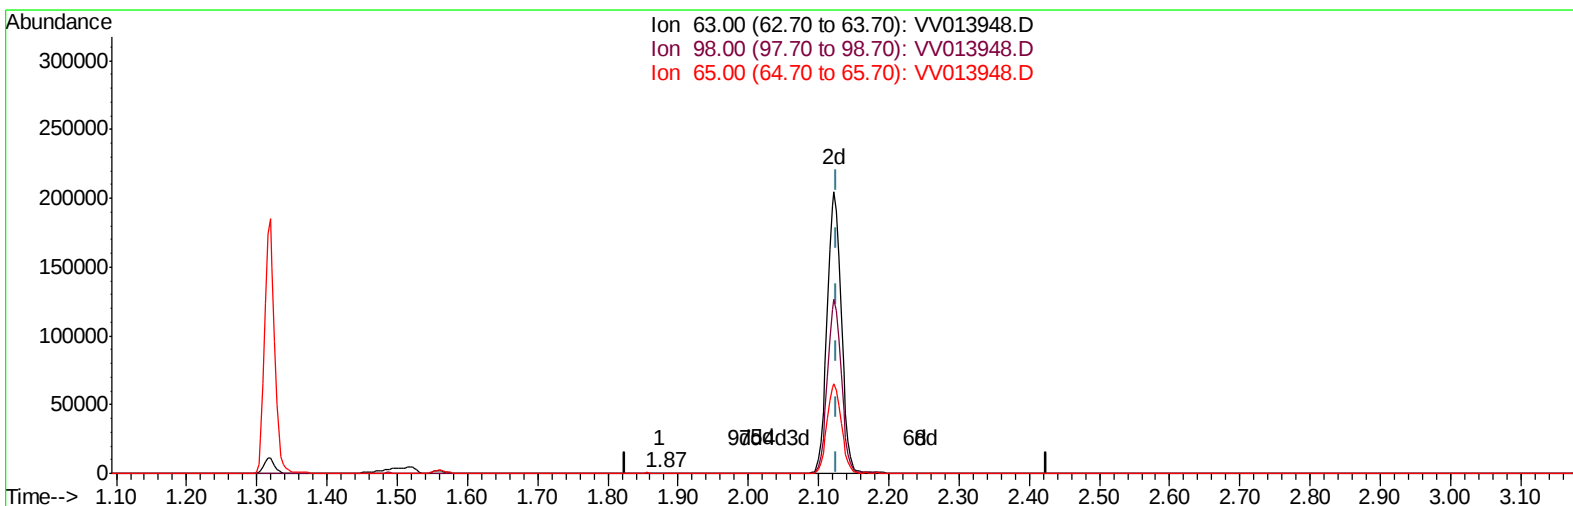

TIC: VV013948.D

(11) 1,1-Dichloroethene-d2 (S)

1.875min (-0.251) 0.02ug/L

response 157

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	71.34
65.00	23.60	17.20
0.00	0.00	0.00