

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Quantitation Report (QT Reviewed)


Data File : VV013937.D
Acq On : 06 Dec 2019 12:59
Operator : SY/MD
Sample : K6170-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR9

Manual Integrations
APPROVED

apatel
12/9/2019 2:05:47 PM

Quant Time: Dec 07 02:37:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

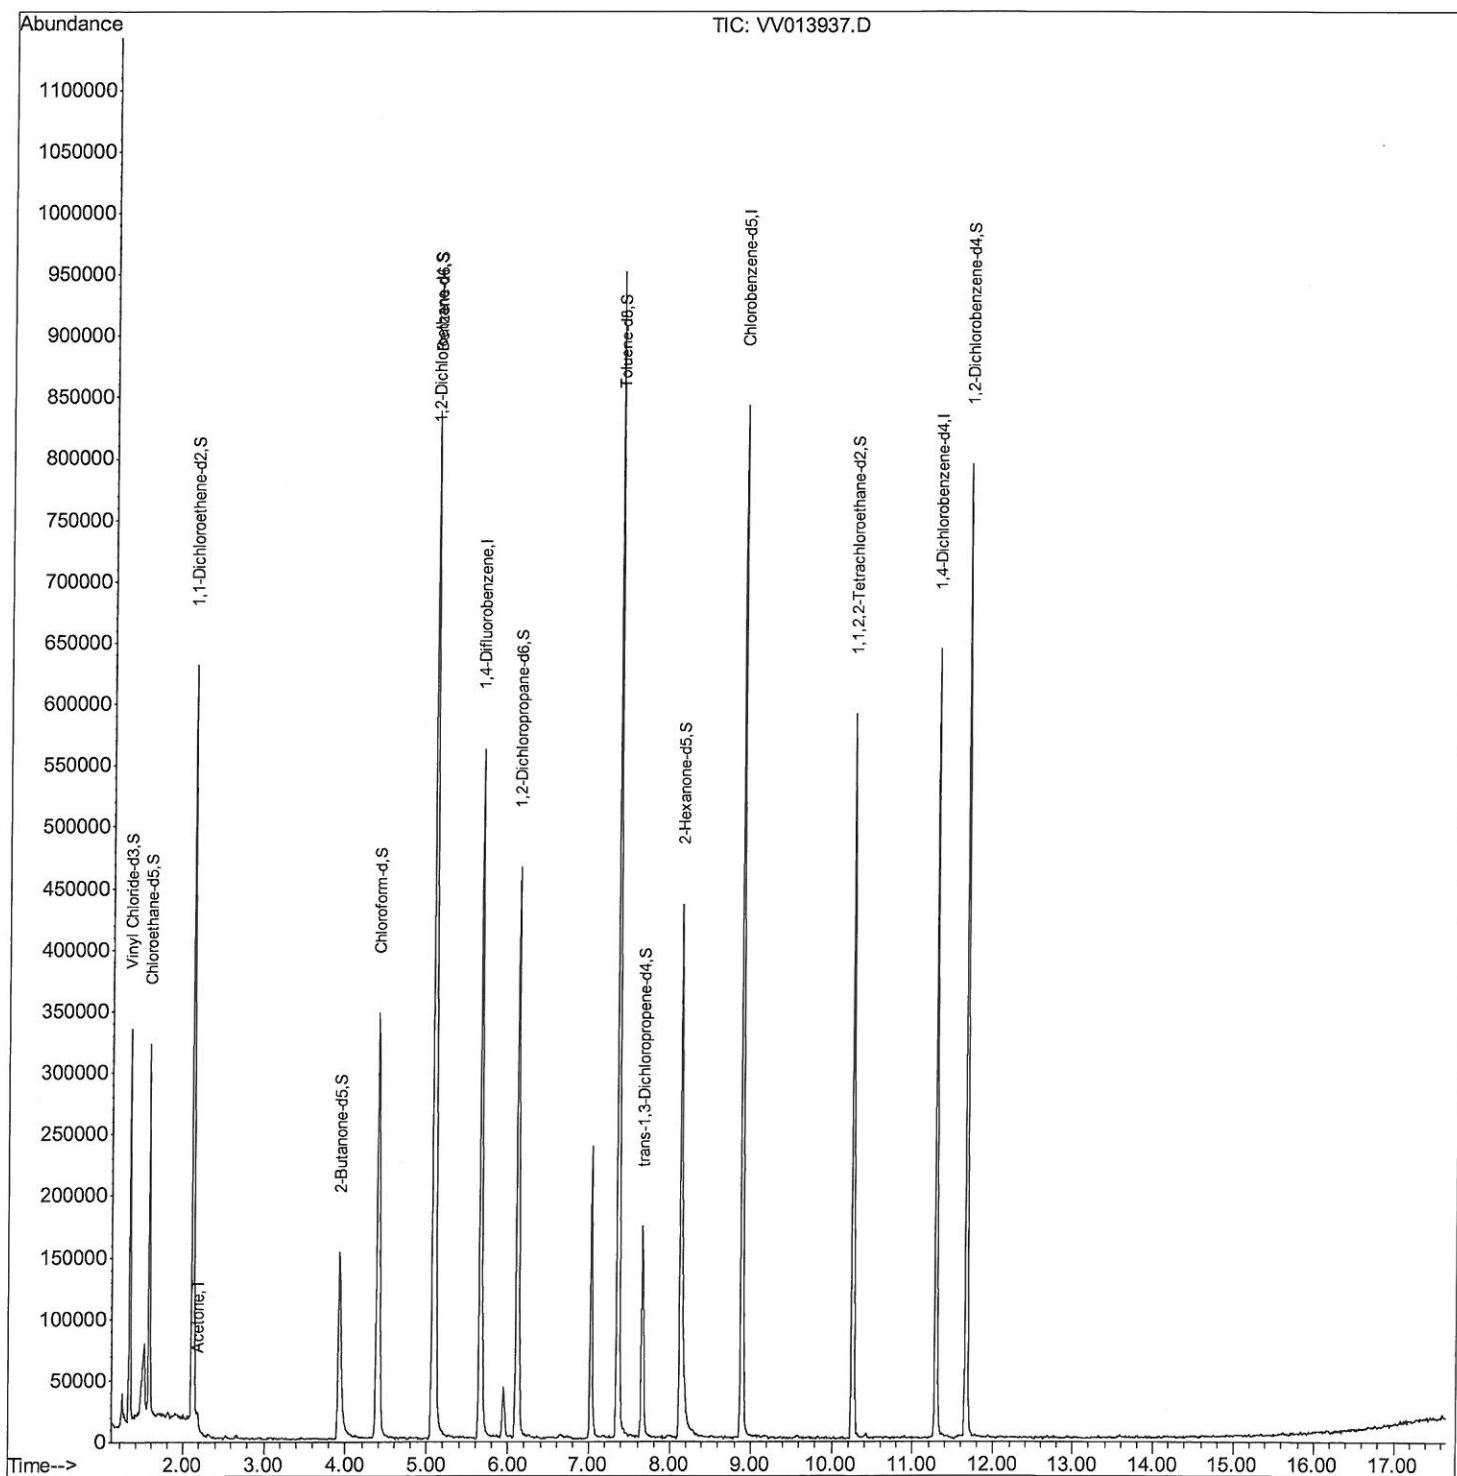

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Quantitation Report (Qedit)




Data File : VV013937.D
Acq On : 06 Dec 2019 12:59
Operator : SY/MD
Sample : K6170-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR9

Manual Integrations
APPROVED

apatel
12/9/2019 2:05:47 PM

Quant Time: Dec 07 01:42:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

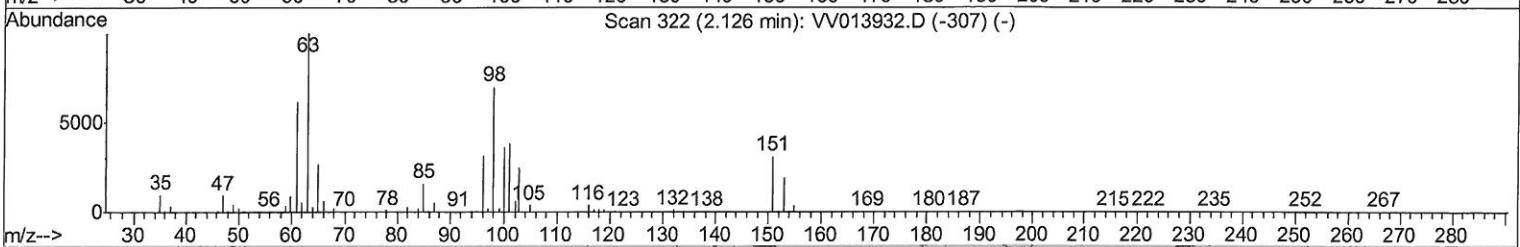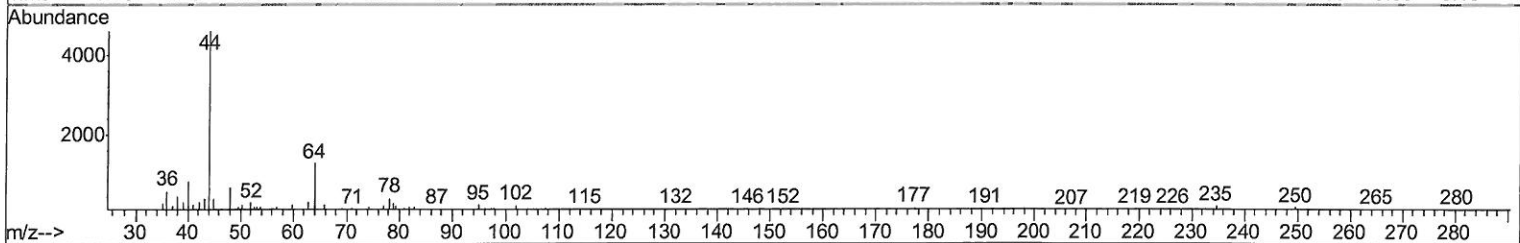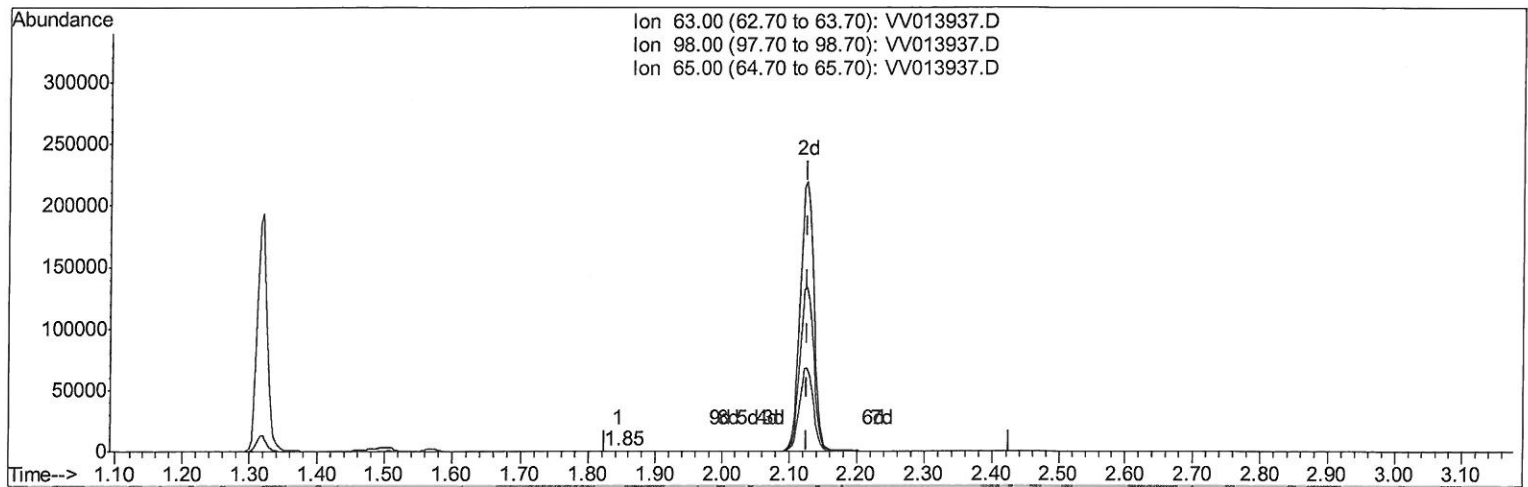

TIC: VV013937.D

(11) 1,1-Dichloroethene-d2 (S)

1.846min (-0.280) 0.04ug/L

response 261

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	77.39
65.00	23.60	27.20
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Quantitation Report (Qedit)




Data File : VV013937.D
Acq On : 06 Dec 2019 12:59
Operator : SY/MD
Sample : K6170-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BR9

Manual Integrations
APPROVED

apatel
12/9/2019 2:05:47 PM

Quant Time: Dec 07 01:42:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

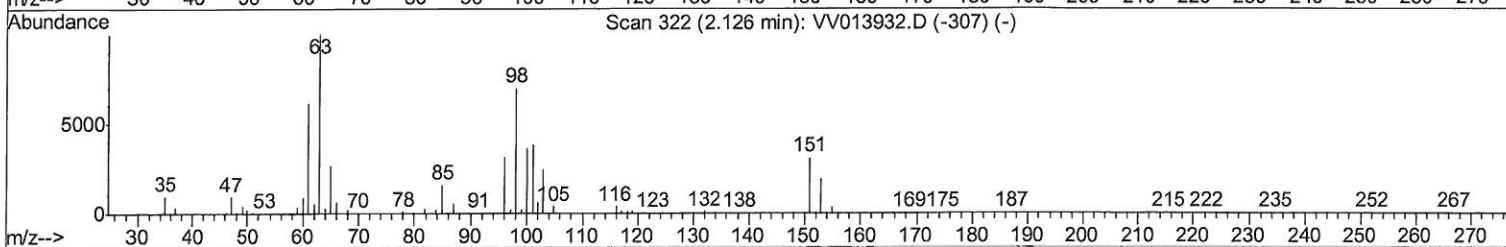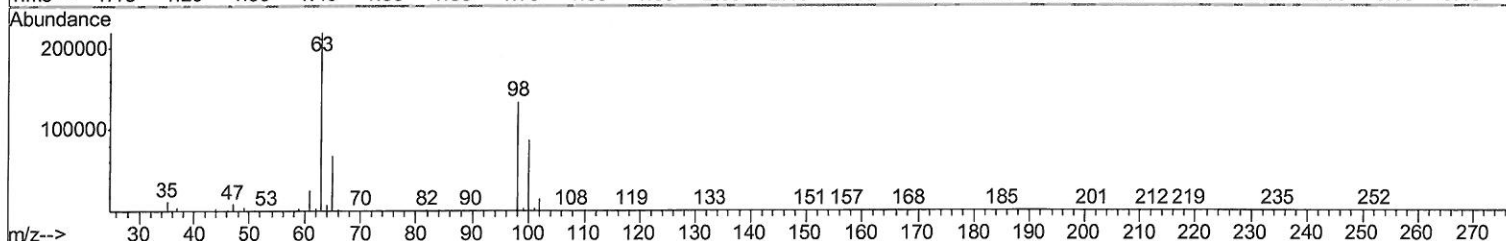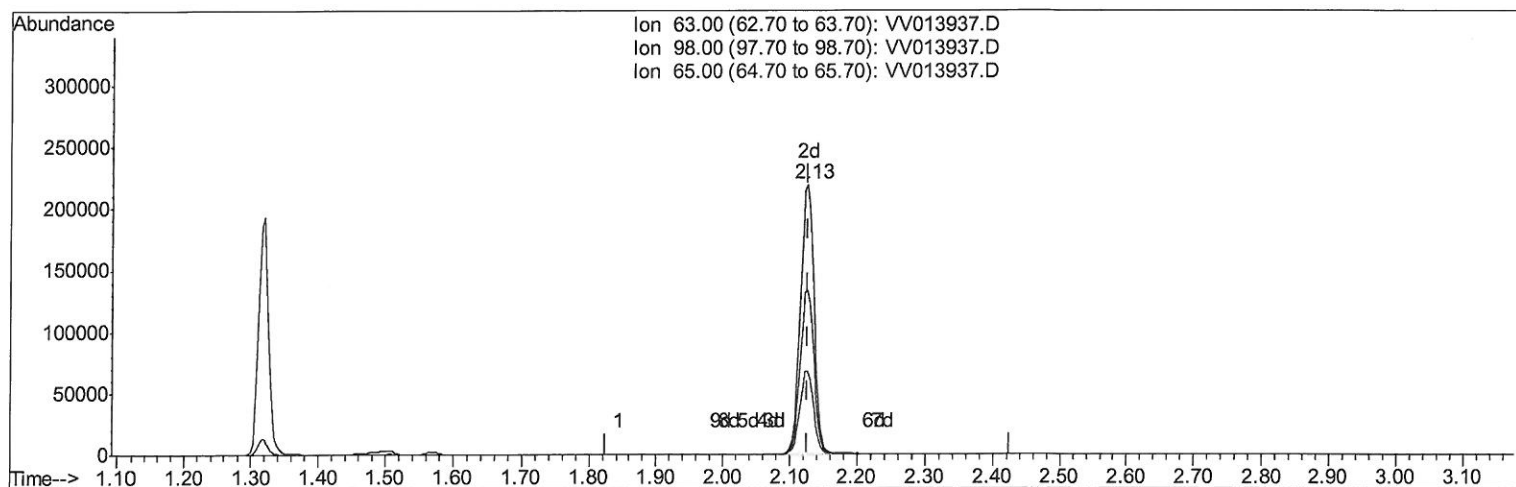

TIC: VV013937.D

(11) 1,1-Dichloroethene-d2 (S)

2.126min (+0.000) 48.58ug/L m

response 304648

Ion Exp% Act%

63.00 100 100

98.00 79.40 0.07#

65.00 23.60 0.02#

0.00 0.00 0.00

7mg
12/16/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Quantitation Report (QT Reviewed)

Data File : VV013937.D
Acq On : 06 Dec 2019 12:59
Operator : SY/MD
Sample : K6170-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0BR9

Manual Integrations
APPROVED

apatel
12/9/2019 2:05:47 PM

Quant Time: Dec 07 02:37:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	490337	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	473191	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	178685	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	191501	67.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	135.06%#
7) Chloroethane-d5	1.57	69	195950	66.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	132.40%#
11) 1,1-Dichloroethene-d2	2.13	63	304648m	48.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.16%
21) 2-Butanone-d5	3.92	46	235490	117.98	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	117.98%
24) Chloroform-d	4.39	84	352212	59.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	118.28%
26) 1,2-Dichloroethane-d4	5.07	65	226122	59.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.84%
32) Benzene-d6	5.09	84	734066	59.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	119.74%
36) 1,2-Dichloropropane-d6	6.11	67	221360	60.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	120.28%#
41) Toluene-d8	7.35	98	624343	55.85	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.70%
43) trans-1,3-Dichloropropene-	7.66	79	95257	53.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	106.38%
47) 2-Hexanone-d5	8.13	63	134662	97.98	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	267087	50.12	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.24%
64) 1,2-Dichlorobenzene-d4	11.67	152	223894	63.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	127.60%#

7MO
12/16/19

Target Compounds				Qvalue
13) Acetone	2.19	43	3000	1.026 ug/L 69

(#) = qualifier out of range (m) = manual integration (+) = signals summed