

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013934.D
 Acq On : 06 Dec 2019 11:45
 Operator : SY/MD
 Sample : K6170-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT5

Quant Time: Dec 07 01:54:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 01:39:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	1220459	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	1114408	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	477843	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	424302	60.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	120.22%
7) Chloroethane-d5	1.57	69	422515	57.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	114.70%
11) 1,1-Dichloroethene-d2	2.13	63	688846	44.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.26%
21) 2-Butanone-d5	3.91	46	591445	119.04	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	119.04%
24) Chloroform-d	4.39	84	826174	55.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.46%
26) 1,2-Dichloroethane-d4	5.07	65	481247	51.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.46%
32) Benzene-d6	5.09	84	1570452	54.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.76%
36) 1,2-Dichloropropane-d6	6.11	67	446380	51.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.00%
41) Toluene-d8	7.35	98	1354154	51.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.88%
43) trans-1,3-Dichloropropene-	7.66	79	203298	48.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.40%
47) 2-Hexanone-d5	8.12	63	281204	86.88	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.88%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	550026	43.82	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.64%
64) 1,2-Dichlorobenzene-d4	11.67	152	499783	53.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.50%


Target Compounds					Ovalue
13) Acetone	2.18	43	8657	1.189 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013934.D
Acq On : 06 Dec 2019 11:45
Operator : SY/MD
Sample : K6170-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT5

Quant Time: Dec 07 01:54:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

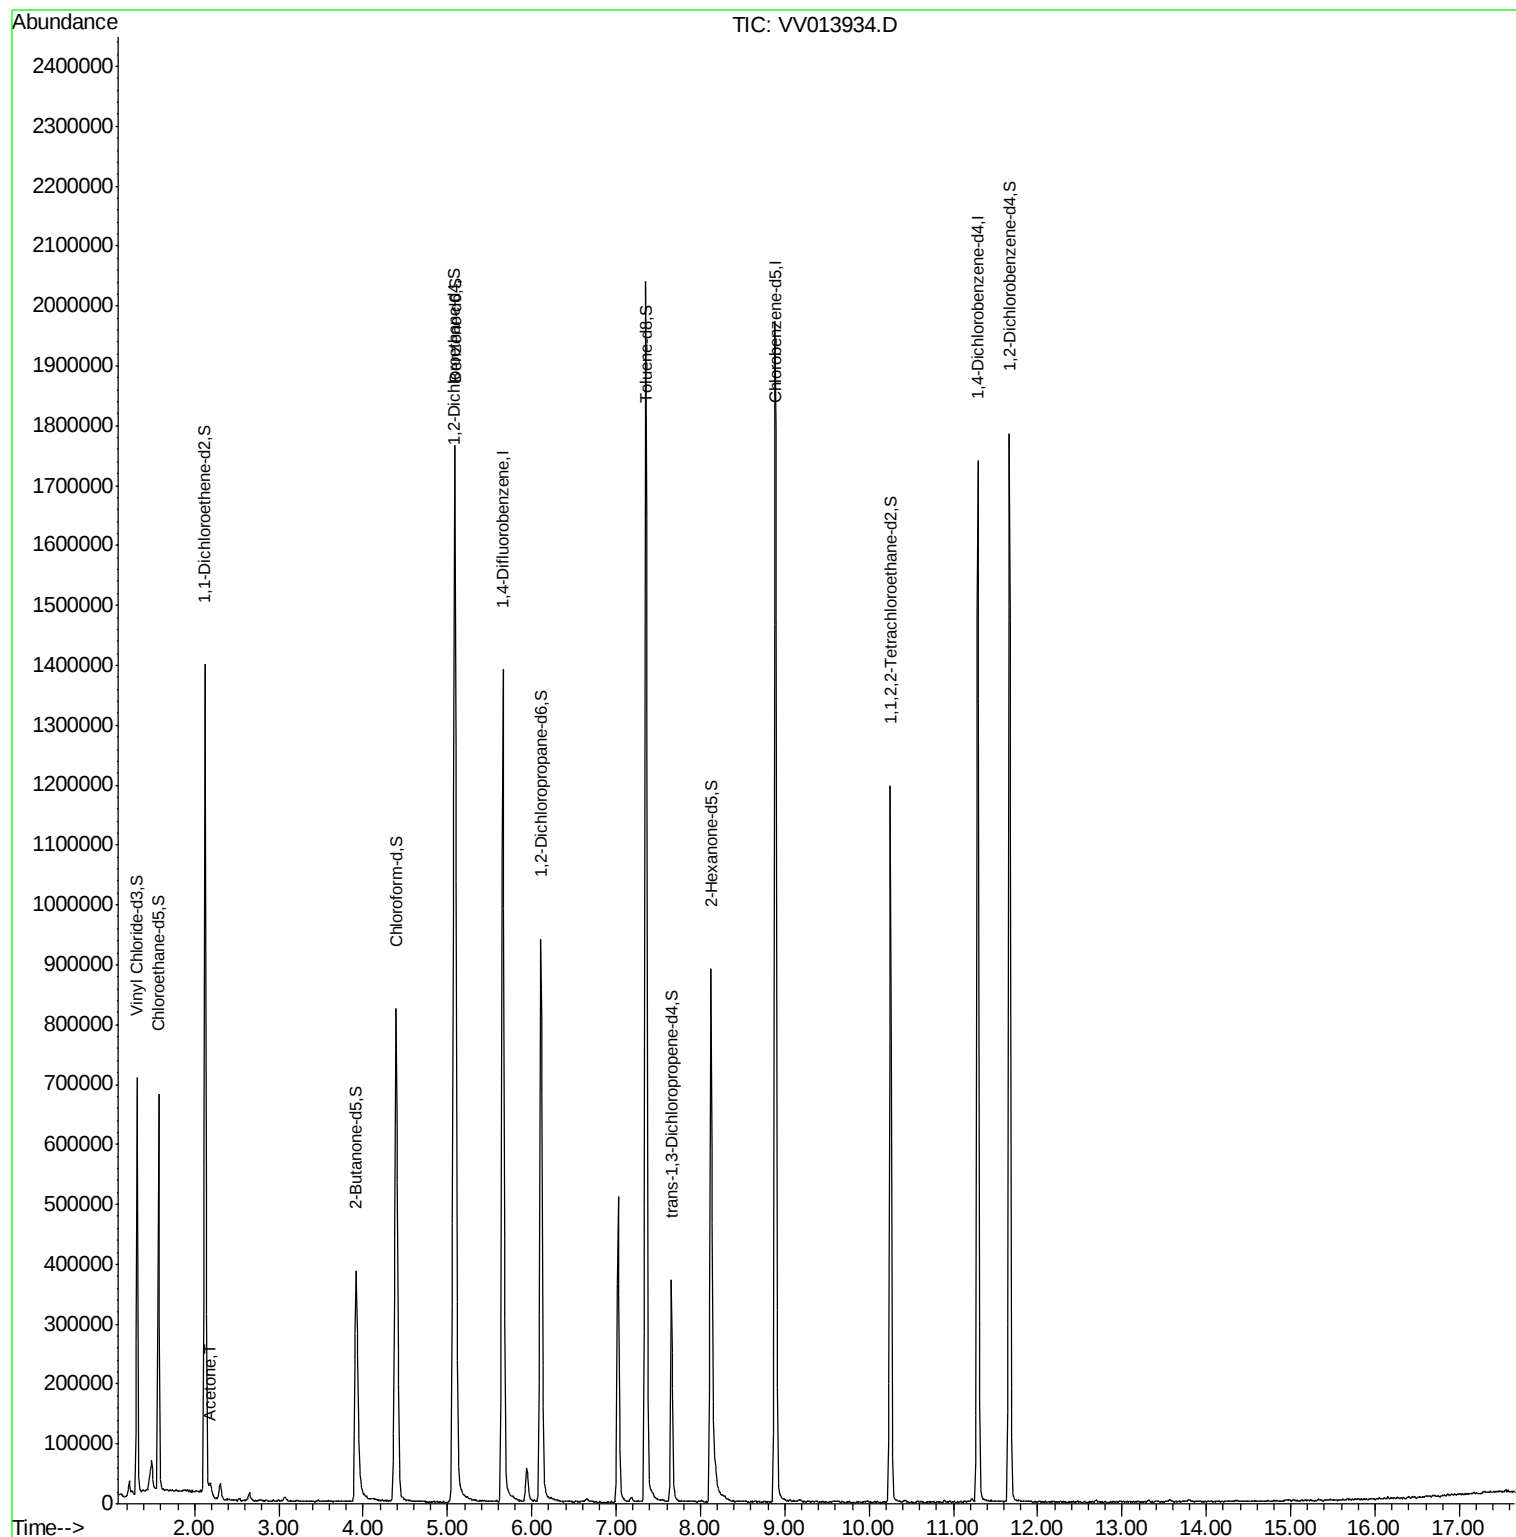

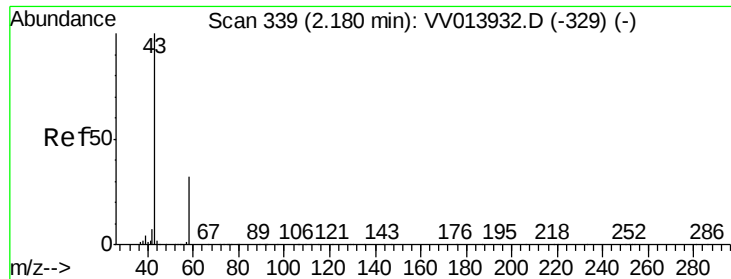

#13

Acetone

Concen: 1.189 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013934.D

Acq: 06 Dec 2019 11:45


Instrument :
MSVOA_V
ClientSampleId :
C0BT5

Tot Ion: 43 Resp: 8657

Ion Ratio Lower Upper

43 100

58 33.5 0.0 60.8

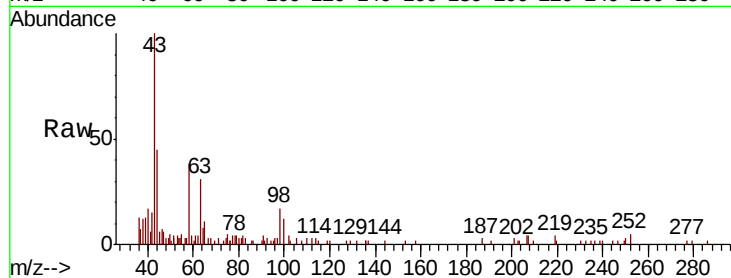

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

