

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013942.D
 Acq On : 06 Dec 2019 15:02
 Operator : SY/MD
 Sample : K6170-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT6

Quant Time: Dec 07 03:00:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 01:39:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	640253	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	579096	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	230330	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	197253	53.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	106.54%
7) Chloroethane-d5	1.57	69	197687	51.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.30%
11) 1,1-Dichloroethene-d2	2.13	63	306161	37.39	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.78%
21) 2-Butanone-d5	3.92	46	223030	85.57	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.57%
24) Chloroform-d	4.40	84	361354	46.47	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.94%
26) 1,2-Dichloroethane-d4	5.07	65	228809	46.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.86%
32) Benzene-d6	5.09	84	735256	49.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.11	67	229323	50.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.82%
41) Toluene-d8	7.35	98	616092	45.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.08%
43) trans-1,3-Dichloropropene-	7.66	79	92073	42.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.02%
47) 2-Hexanone-d5	8.13	63	112611	66.95	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	66.95%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	267779	41.06	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	82.12%
64) 1,2-Dichlorobenzene-d4	11.67	152	231862	51.25	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.50%


Target Compounds					Ovalue
13) Acetone	2.18	43	3935	1.030 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013942.D
Acq On : 06 Dec 2019 15:02
Operator : SY/MD
Sample : K6170-22
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT6

Quant Time: Dec 07 03:00:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

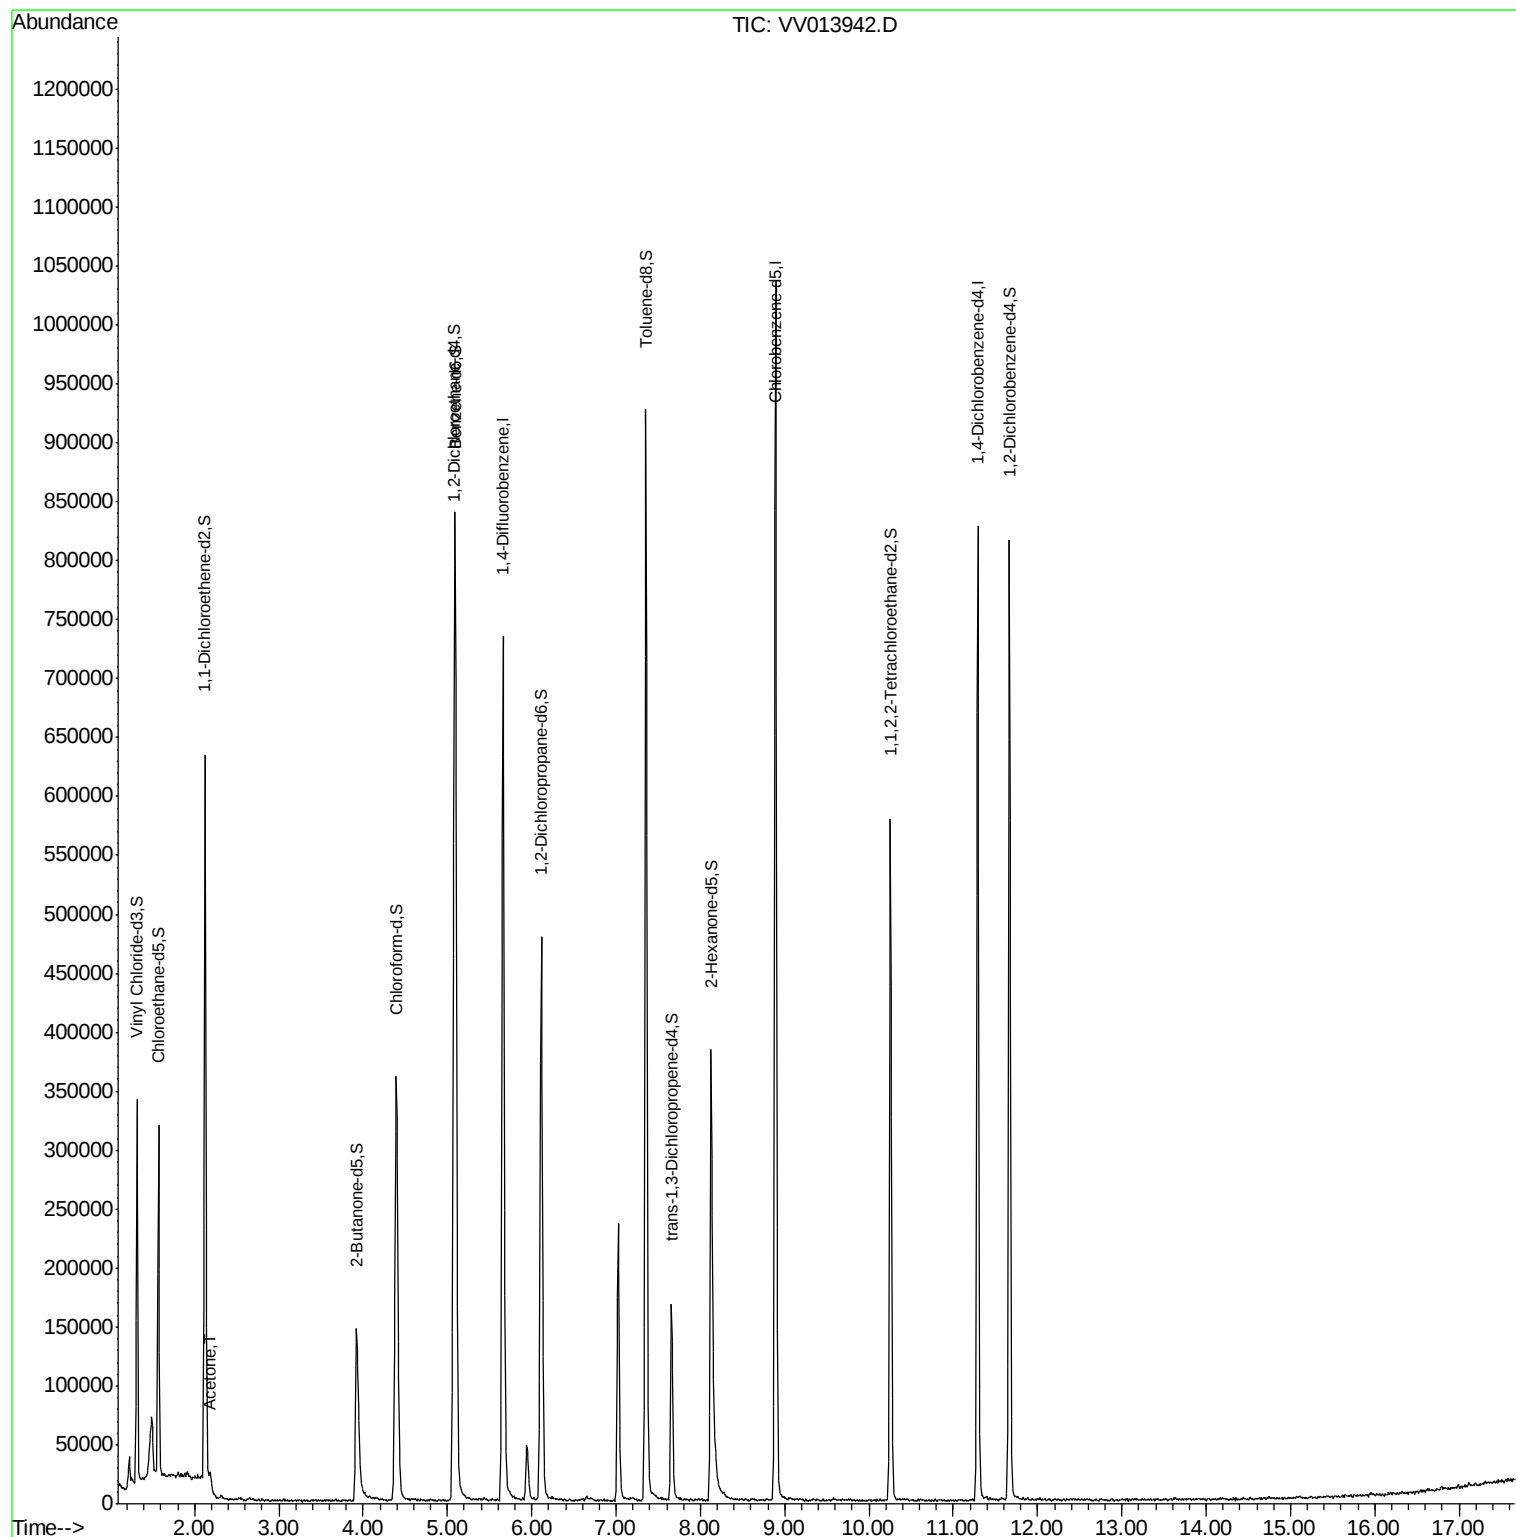

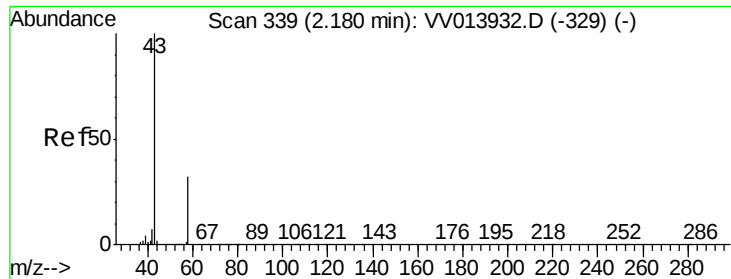

#13

Acetone

Concen: 1.030 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013942.D

Acq: 06 Dec 2019 15:02

Instrument :
MSVOA_V
ClientSampleId :
C0BT6

Tot Ion: 43 Resp: 3935

Ion Ratio Lower Upper

43 100

58 35.6 0.0 60.8

