

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013946.D
 Acq On : 06 Dec 2019 18:21
 Operator : SY/MD
 Sample : K6170-13
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BT9

Quant Time: Dec 07 03:20:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 07 01:39:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	623990	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	593519	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	213502	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	183251	50.78	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.56%
7) Chloroethane-d5	1.57	69	192537	51.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.22%
11) 1,1-Dichloroethene-d2	2.13	63	299926	37.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.16%
21) 2-Butanone-d5	3.92	46	233870	92.07	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	92.07%
24) Chloroform-d	4.40	84	345095	45.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.06%
26) 1,2-Dichloroethane-d4	5.07	65	219664	45.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.48%
32) Benzene-d6	5.09	84	702045	45.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.30%
36) 1,2-Dichloropropane-d6	6.11	67	208790	45.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.46%
41) Toluene-d8	7.36	98	576961	41.15	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.30%
43) trans-1,3-Dichloropropene-	7.66	79	85906	38.24	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.48%
47) 2-Hexanone-d5	8.13	63	121180	70.30	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.30%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	263141	39.36	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	78.72%
64) 1,2-Dichlorobenzene-d4	11.67	152	201723	48.11	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.22%


Target Compounds					Ovalue
13) Acetone	2.19	43	4139	1.112 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013946.D
Acq On : 06 Dec 2019 18:21
Operator : SY/MD
Sample : K6170-13
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BT9

Quant Time: Dec 07 03:20:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 01:39:07 2019
Response via : Initial Calibration

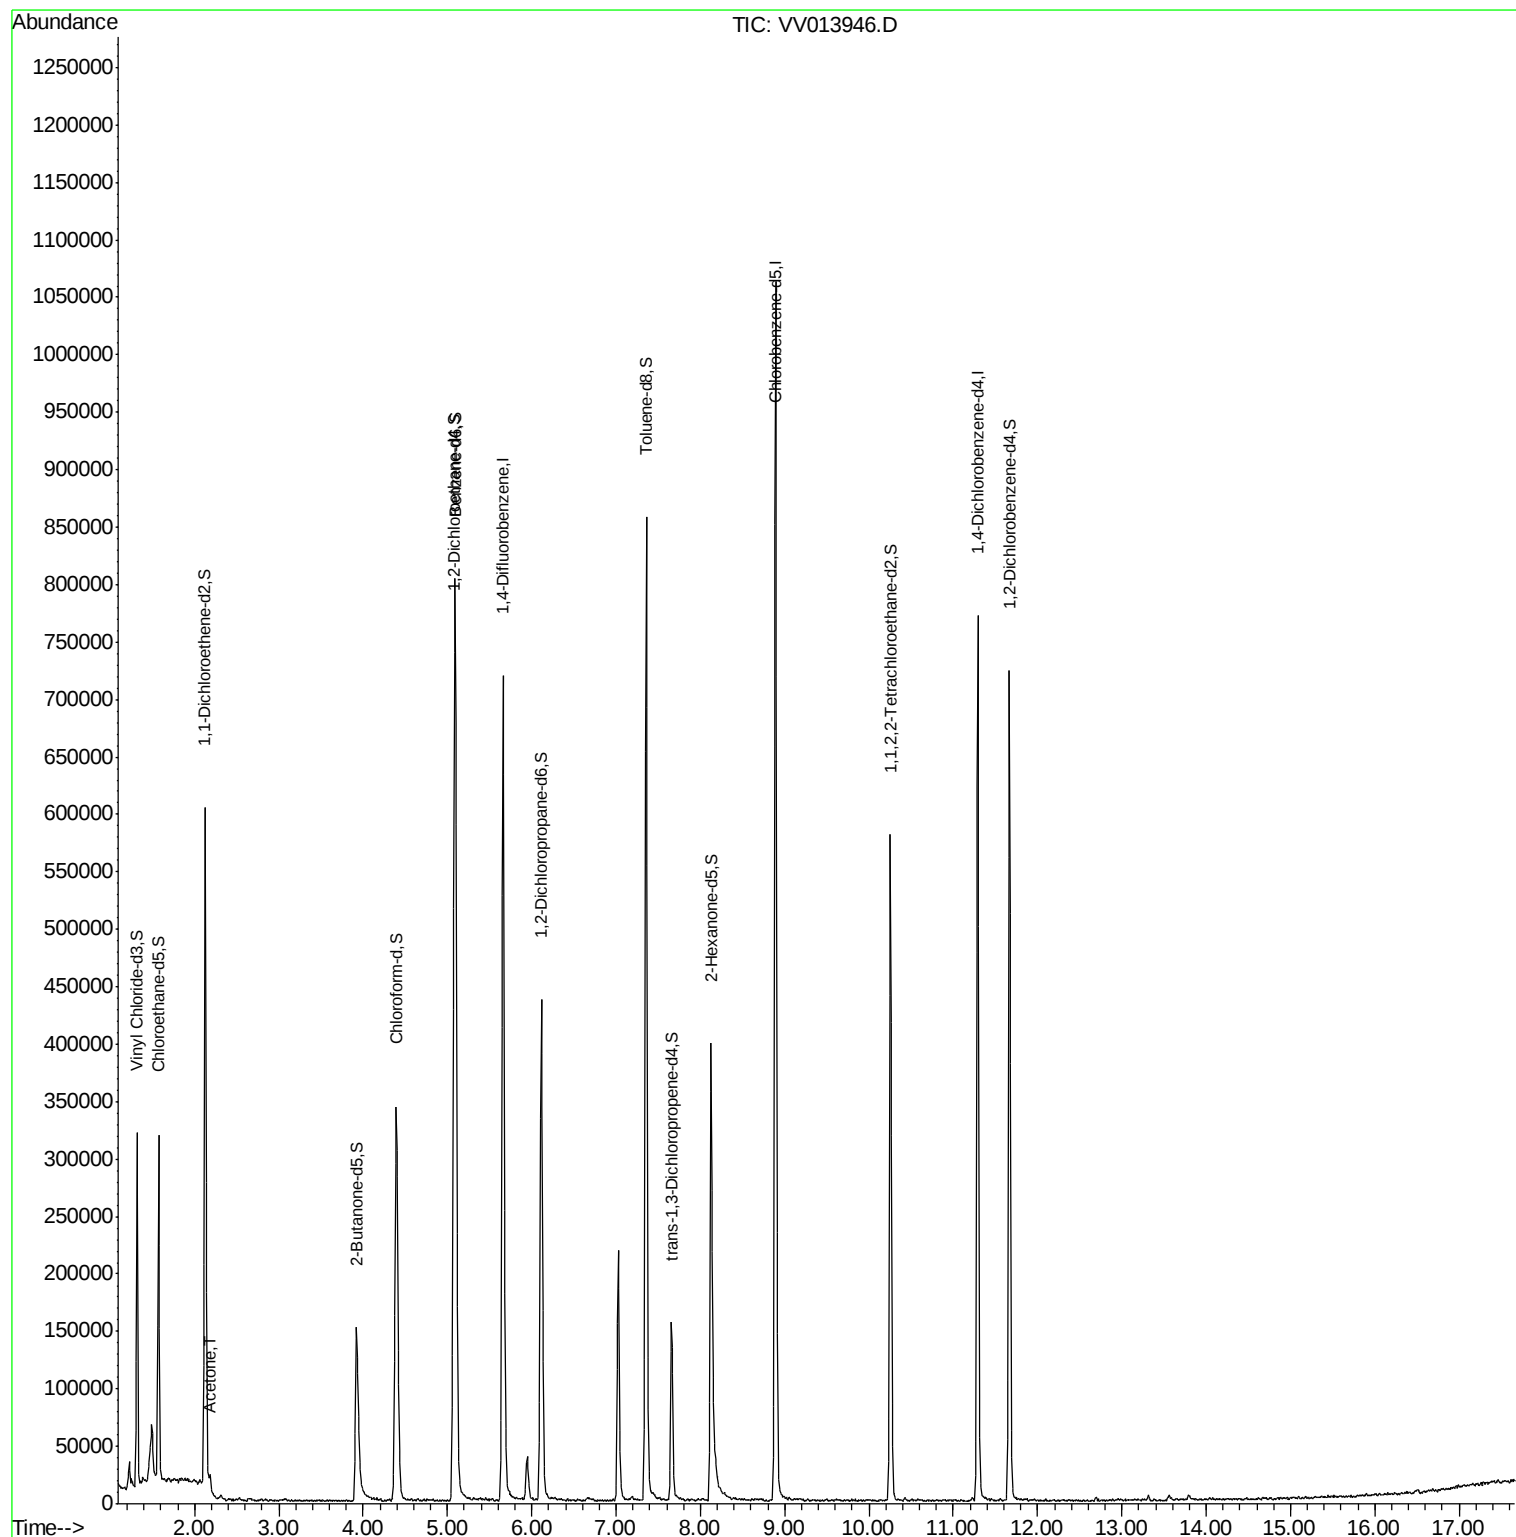

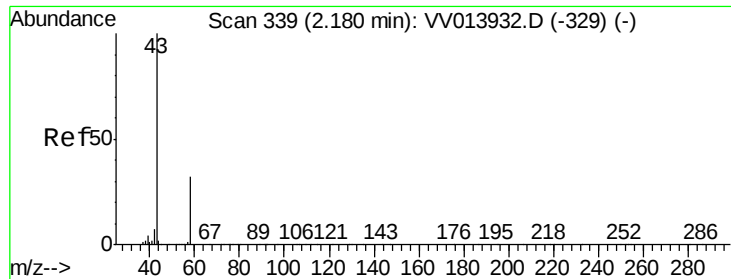

#13

Acetone

Concen: 1.112 ug/L

RT: 2.19 min Scan# 341

Delta R.T. 0.01 min

Lab File: VV013946.D

Acq: 06 Dec 2019 18:21

Instrument :
MSVOA_V
ClientSampleId :
C0BT9

Tot Ion: 43 Resp: 4139

Ion Ratio Lower Upper

43 100

58 33.1 0.0 60.8

