

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013939.D
 Acq On : 06 Dec 2019 13:48
 Operator : SY/MD
 Sample : K6190-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE896

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	337540	333029	15.33%	2.011%
2	1.566	142	148	160	rVB	317527	363453	16.73%	2.195%
3	2.123	313	321	334	rVB	591481	831362	38.27%	5.020%
4	2.518	441	444	446	rBV3	2135	1603	0.07%	0.010%
5	2.759	516	519	520	rBV3	1442	751	0.03%	0.005%
6	2.955	578	580	583	rBV2	975	419	0.02%	0.003%
7	2.975	583	586	588	rBV3	1286	1019	0.05%	0.006%
8	3.045	606	608	612	rBV5	1201	754	0.03%	0.005%
9	3.068	612	615	617	rBV2	1417	1056	0.05%	0.006%
10	3.135	630	636	638	rBV6	1115	1009	0.05%	0.006%
11	3.148	638	640	642	rVB2	1229	394	0.02%	0.002%
12	3.180	647	650	653	rVV4	1222	933	0.04%	0.006%
13	3.277	679	680	682	rVB2	926	232	0.01%	0.001%
14	3.293	682	685	688	rVB4	1405	979	0.05%	0.006%
15	3.319	688	693	696	rBV5	1500	1490	0.07%	0.009%
16	3.335	696	698	699	rBV	552	269	0.01%	0.002%
17	3.357	703	705	707	rBV3	512	158	0.01%	0.001%
18	3.370	707	709	711	rBV3	653	361	0.02%	0.002%
19	3.434	725	729	732	rBV3	1214	1250	0.06%	0.008%
20	3.479	741	743	745	rVB3	688	228	0.01%	0.001%
21	3.495	745	748	753	rBV6	1222	1188	0.05%	0.007%
22	3.560	765	768	772	rBV4	1119	1078	0.05%	0.007%
23	3.579	772	774	776	rVB3	1102	478	0.02%	0.003%
24	3.602	776	781	783	rBV3	954	824	0.04%	0.005%
25	3.637	791	792	793	rVB	628	121	0.01%	0.001%
26	3.647	793	795	799	rVB4	1377	823	0.04%	0.005%
27	3.666	799	801	803	rBV3	831	310	0.01%	0.002%
28	3.875	864	866	868	rBV2	1130	765	0.04%	0.005%
29	3.920	870	880	909	rVV	153299	432743	19.92%	2.613%
30	4.257	983	985	990	rBV5	1448	1233	0.06%	0.007%
31	4.331	1001	1008	1009	rBV6	1520	1311	0.06%	0.008%
32	4.396	1014	1028	1053	rVB	365486	902473	41.55%	5.449%
33	4.814	1157	1158	1161	rVB3	1377	464	0.02%	0.003%
34	4.875	1175	1177	1178	rBV2	1220	460	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013939.D
 Acq On : 06 Dec 2019 13:48
 Operator : SY/MD
 Sample : K6190-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE896

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.897	1181	1184	1186	rVB4	1166	586	0.03%	0.004%
36	4.929	1193	1194	1195	rBV	769	257	0.01%	0.002%
37	5.090	1226	1244	1272	rBV2	863249	2172207	100.00%	13.116%
38	5.659	1407	1421	1452	rBV	756793	1509662	69.50%	9.115%
39	5.884	1488	1491	1492	rBV3	1224	611	0.03%	0.004%
40	6.113	1549	1562	1578	rBV	482030	969415	44.63%	5.853%
41	6.299	1618	1620	1623	rBV3	2168	1307	0.06%	0.008%
42	6.826	1782	1784	1785	rBV2	980	364	0.02%	0.002%
43	6.868	1794	1797	1800	rVB3	1167	677	0.03%	0.004%
44	6.881	1800	1801	1803	rBV2	574	201	0.01%	0.001%
45	6.952	1821	1823	1824	rBV2	701	269	0.01%	0.002%
46	7.026	1835	1846	1864	rBV	249569	436555	20.10%	2.636%
47	7.354	1936	1948	1967	rBV	994351	1718873	79.13%	10.378%
48	7.659	2033	2043	2064	rVB	176439	299620	13.79%	1.809%
49	7.939	2128	2130	2132	rBV3	2669	1563	0.07%	0.009%
50	8.090	2172	2177	2178	rBV4	2233	1782	0.08%	0.011%
51	8.129	2178	2189	2223	rVV2	435514	925406	42.60%	5.588%
52	8.540	2315	2317	2320	rBV3	1723	1040	0.05%	0.006%
53	8.588	2330	2332	2335	rVB4	1309	642	0.03%	0.004%
54	8.891	2413	2426	2451	rBV	1136861	1809963	83.32%	10.928%
55	9.421	2588	2591	2593	rBV2	1418	840	0.04%	0.005%
56	9.479	2607	2609	2610	rBV2	1218	555	0.03%	0.003%
57	9.585	2634	2642	2654	rVB3	16294	28729	1.32%	0.173%
58	9.794	2705	2707	2710	rVB4	1433	959	0.04%	0.006%
59	9.813	2710	2713	2715	rBV3	2345	1414	0.07%	0.009%
60	9.849	2719	2724	2726	rBV5	4088	3712	0.17%	0.022%
61	10.055	2784	2788	2791	rBV5	1543	1291	0.06%	0.008%
62	10.087	2797	2798	2800	rBV2	963	466	0.02%	0.003%
63	10.167	2821	2823	2824	rBV2	1239	523	0.02%	0.003%
64	10.254	2838	2850	2872	rBV	620467	984385	45.32%	5.944%
65	10.469	2915	2917	2919	rBV3	1410	813	0.04%	0.005%
66	10.621	2962	2964	2968	rBV4	1466	841	0.04%	0.005%
67	10.704	2987	2990	2992	rBV3	1134	570	0.03%	0.003%
68	10.736	2998	3000	3003	rVB4	863	313	0.01%	0.002%
69	10.836	3029	3031	3033	rBV4	1104	617	0.03%	0.004%
70	11.013	3084	3086	3087	rBV2	1279	389	0.02%	0.002%
71	11.048	3095	3097	3102	rVB5	1823	1104	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013939.D
 Acq On : 06 Dec 2019 13:48
 Operator : SY/MD
 Sample : K6190-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BE896

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.071	3102	3104	3106	rBV2	931	477	0.02%	0.003%
73	11.112	3115	3117	3118	rBB3	270	134	0.01%	0.001%
74	11.203	3135	3145	3157	rBV3	5951	14511	0.67%	0.088%
75	11.289	3161	3172	3197	rVV	898044	1397416	64.33%	8.438%
76	11.666	3278	3289	3312	rVB	869480	1375570	63.33%	8.306%
77	11.858	3347	3349	3352	rBV3	1553	1309	0.06%	0.008%
78	12.174	3444	3447	3449	rBV4	1086	653	0.03%	0.004%
79	12.238	3465	3467	3468	rBV2	1189	547	0.03%	0.003%
80	12.293	3482	3484	3487	rVB4	1827	964	0.04%	0.006%
81	12.331	3494	3496	3497	rBV2	747	264	0.01%	0.002%
82	12.347	3497	3501	3503	rBV3	1612	1420	0.07%	0.009%
83	12.977	3695	3697	3700	rVB3	1772	1032	0.05%	0.006%
84	12.993	3700	3702	3703	rBV	970	333	0.02%	0.002%
85	13.090	3731	3732	3733	rBV	906	199	0.01%	0.001%
86	13.440	3838	3841	3842	rBV3	1121	661	0.03%	0.004%
87	13.813	3954	3957	3962	rBV7	2111	1587	0.07%	0.010%
88	13.984	4009	4010	4012	rBV2	1104	538	0.02%	0.003%
89	14.630	4209	4211	4212	rBV2	2037	768	0.04%	0.005%


Sum of corrected areas: 16561924

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013939.D
Acq On : 06 Dec 2019 13:48
Operator : SY/MD
Sample : K6190-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE896

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

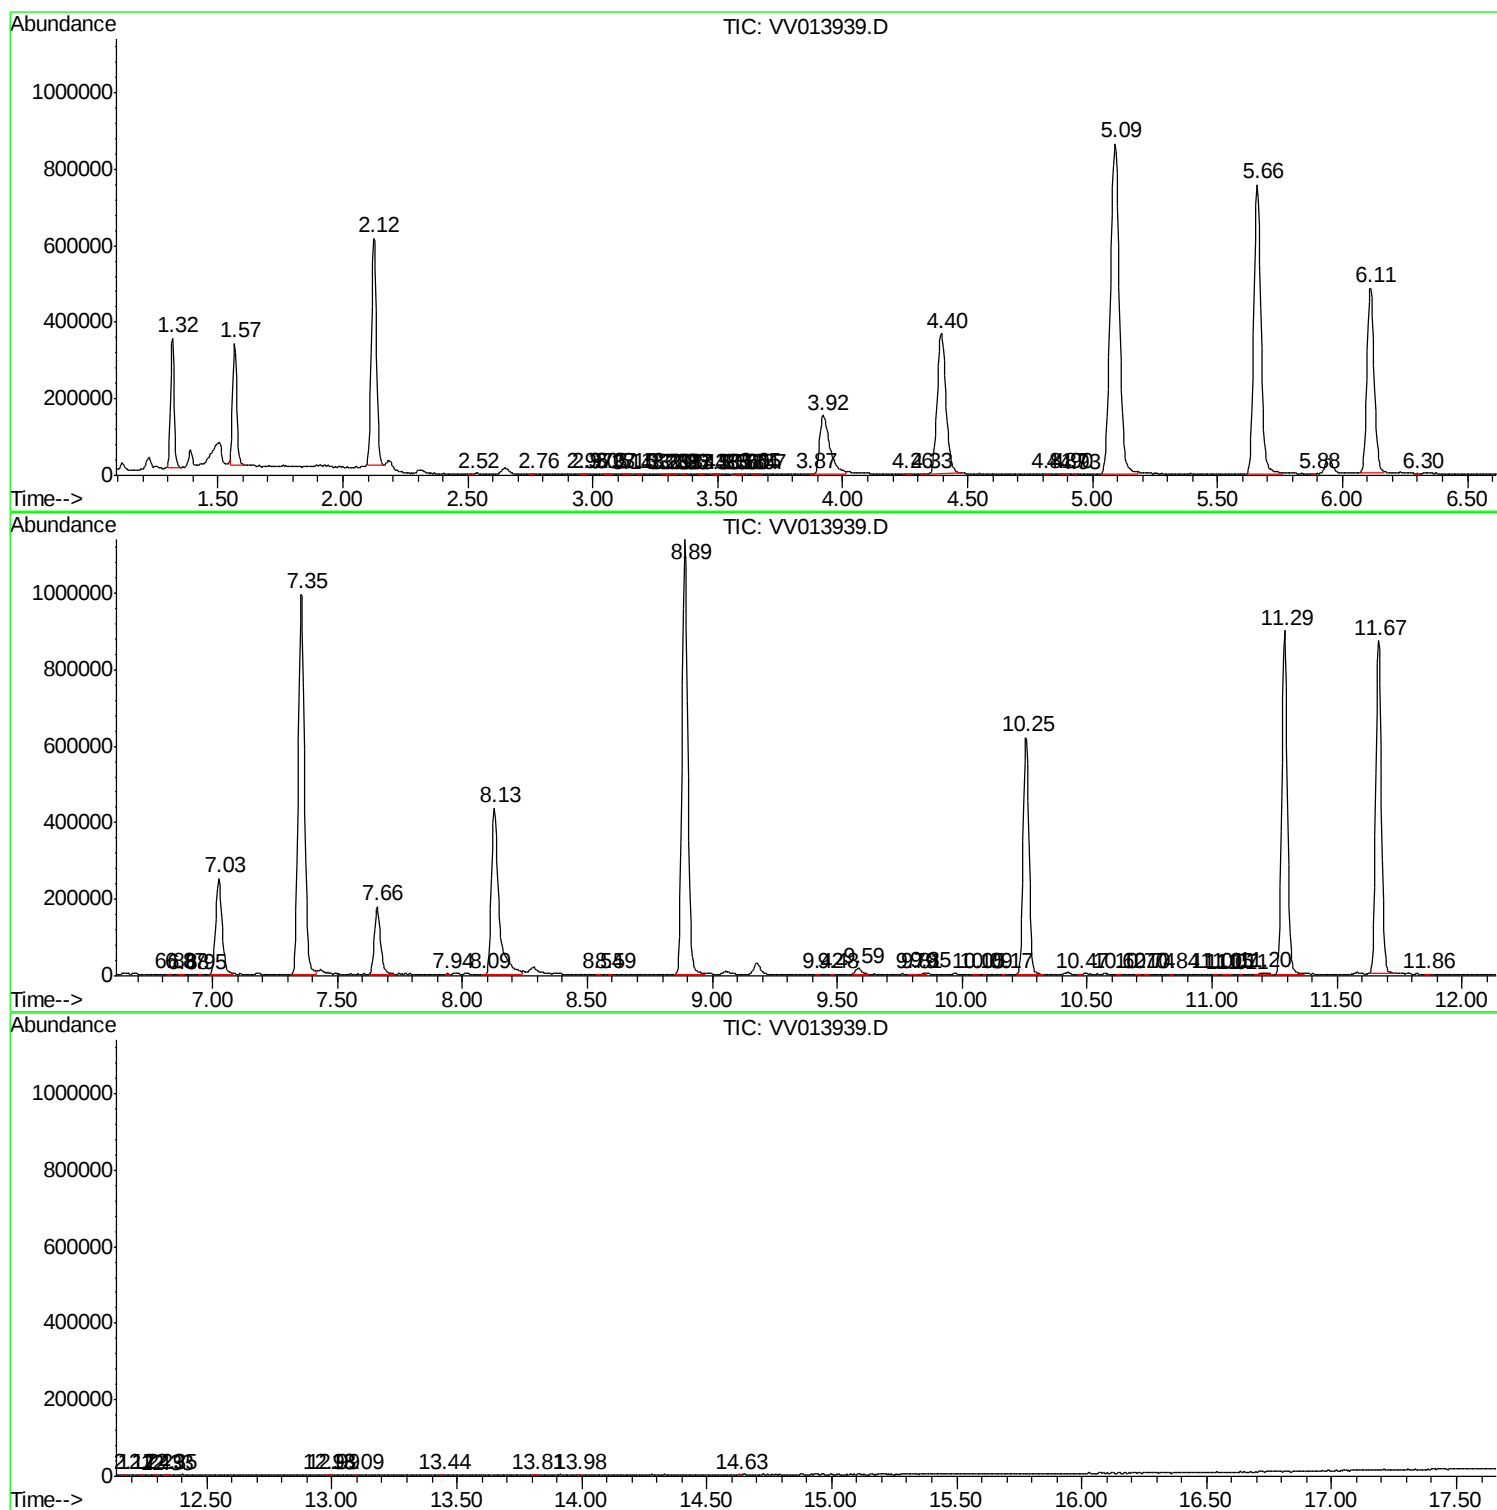

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013939.D
Acq On : 06 Dec 2019 13:48
Operator : SY/MD
Sample : K6190-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BE896

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120619\
Data File : VV013939.D
Acq On : 06 Dec 2019 13:48
Operator : SY/MD
Sample : K6190-02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BE896

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc