

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013941.D
 Acq On : 06 Dec 2019 14:37
 Operator : SY/MD
 Sample : K6190-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFR97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	299990	299715	15.03%	2.040%
2	1.563	141	147	162	rVB	288814	340892	17.09%	2.320%
3	2.122	313	321	334	rVB	598574	823482	41.29%	5.605%
4	2.753	515	517	519	rBV2	972	669	0.03%	0.005%
5	2.859	547	550	552	rBV3	1434	1008	0.05%	0.007%
6	2.965	581	583	585	rBV3	1294	553	0.03%	0.004%
7	3.302	686	688	690	rBV3	846	488	0.02%	0.003%
8	3.312	690	691	696	rVB3	1218	637	0.03%	0.004%
9	3.405	716	720	722	rBV2	1268	960	0.05%	0.007%
10	3.495	746	748	750	rVB2	1427	597	0.03%	0.004%
11	3.508	750	752	753	rBV2	1061	414	0.02%	0.003%
12	3.547	762	764	767	rBV3	898	481	0.02%	0.003%
13	3.727	819	820	822	rBV	726	370	0.02%	0.003%
14	3.839	853	855	858	rBV3	1170	781	0.04%	0.005%
15	3.852	858	859	861	rVB2	1152	373	0.02%	0.003%
16	3.923	869	881	907	rBV	154084	419822	21.05%	2.858%
17	4.392	1013	1027	1055	rVB	336968	799950	40.11%	5.445%
18	4.872	1173	1176	1184	rVB6	2501	2642	0.13%	0.018%
19	4.917	1184	1190	1194	rBV9	936	1374	0.07%	0.009%
20	4.962	1199	1204	1207	rBV6	1823	1818	0.09%	0.012%
21	5.029	1223	1225	1226	rBV2	1164	518	0.03%	0.004%
22	5.090	1227	1244	1267	rVV2	792210	1994259	100.00%	13.575%
23	5.492	1366	1369	1372	rBV3	1400	1238	0.06%	0.008%
24	5.572	1391	1394	1395	rBV2	1177	510	0.03%	0.003%
25	5.659	1407	1421	1444	rBV	619694	1231171	61.74%	8.381%
26	5.891	1491	1493	1497	rBV5	1040	939	0.05%	0.006%
27	6.113	1548	1562	1584	rBV	443820	900539	45.16%	6.130%
28	6.415	1654	1656	1658	rBV3	1287	373	0.02%	0.003%
29	6.547	1695	1697	1701	rVB3	1141	718	0.04%	0.005%
30	6.836	1783	1787	1790	rBV5	1460	1456	0.07%	0.010%
31	7.026	1833	1846	1864	rBV	224414	405045	20.31%	2.757%
32	7.148	1882	1884	1887	rBV2	1063	432	0.02%	0.003%
33	7.270	1918	1922	1925	rBV5	1828	1684	0.08%	0.011%
34	7.354	1935	1948	1969	rBV	894722	1552487	77.85%	10.568%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013941.D
 Acq On : 06 Dec 2019 14:37
 Operator : SY/MD
 Sample : K6190-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFR97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	7.659	2034	2043	2064	rVB	160648	273741	13.73%	1.863%
36	7.849	2098	2102	2105	rBV6	1375	1093	0.05%	0.007%
37	8.129	2178	2189	2223	rBV2	437073	910201	45.64%	6.196%
38	8.579	2326	2329	2335	rBV6	1220	1564	0.08%	0.011%
39	8.891	2412	2426	2449	rBV	884083	1432016	71.81%	9.748%
40	9.392	2580	2582	2584	rBV2	508	261	0.01%	0.002%
41	9.547	2627	2630	2632	rBV3	864	578	0.03%	0.004%
42	9.739	2688	2690	2697	rBV7	2171	2517	0.13%	0.017%
43	10.029	2778	2780	2782	rBV2	1231	702	0.04%	0.005%
44	10.067	2790	2792	2793	rBV2	644	247	0.01%	0.002%
45	10.151	2816	2818	2822	rBV3	1129	772	0.04%	0.005%
46	10.254	2839	2850	2869	rBV	583414	912922	45.78%	6.214%
47	10.569	2944	2948	2951	rBV5	1991	2176	0.11%	0.015%
48	10.711	2988	2992	2995	rVB4	1435	1071	0.05%	0.007%
49	10.727	2995	2997	3001	rBV3	1518	1279	0.06%	0.009%
50	10.749	3002	3004	3006	rBV3	1197	609	0.03%	0.004%
51	10.788	3015	3016	3020	rVB4	1213	709	0.04%	0.005%
52	10.842	3030	3033	3034	rBV2	935	630	0.03%	0.004%
53	11.106	3110	3115	3116	rBV2	1006	855	0.04%	0.006%
54	11.289	3160	3172	3193	rBV	704201	1105139	55.42%	7.523%
55	11.456	3222	3224	3226	rBV3	1218	555	0.03%	0.004%
56	11.527	3243	3246	3247	rBV2	851	435	0.02%	0.003%
57	11.665	3278	3289	3307	rBV	798013	1239168	62.14%	8.435%
58	11.874	3353	3354	3356	rBV	974	459	0.02%	0.003%
59	11.891	3356	3359	3363	rVV5	1479	1398	0.07%	0.010%
60	12.145	3434	3438	3441	rBV5	1491	1170	0.06%	0.008%
61	12.309	3487	3489	3490	rBV	1271	573	0.03%	0.004%
62	12.559	3565	3567	3570	rBV4	1381	690	0.03%	0.005%
63	12.845	3651	3656	3658	rBV4	1100	706	0.04%	0.005%
64	12.862	3658	3661	3663	rBV4	881	473	0.02%	0.003%
65	12.945	3685	3687	3693	rBV6	1463	1185	0.06%	0.008%
66	13.138	3745	3747	3751	rVB2	1396	648	0.03%	0.004%
67	13.347	3810	3812	3814	rBV2	1093	568	0.03%	0.004%
68	13.855	3968	3970	3971	rBV2	1446	558	0.03%	0.004%
69	14.366	4126	4129	4131	rBV3	1853	1236	0.06%	0.008%
70	14.427	4145	4148	4149	rBV3	1492	816	0.04%	0.006%
71	14.797	4259	4263	4268	rBV8	2335	2770	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013941.D
Acq On : 06 Dec 2019 14:37
Operator : SY/MD
Sample : K6190-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFR97

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis


Sum of corrected areas: 14690885

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013941.D
Acq On : 06 Dec 2019 14:37
Operator : SY/MD
Sample : K6190-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFR97

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

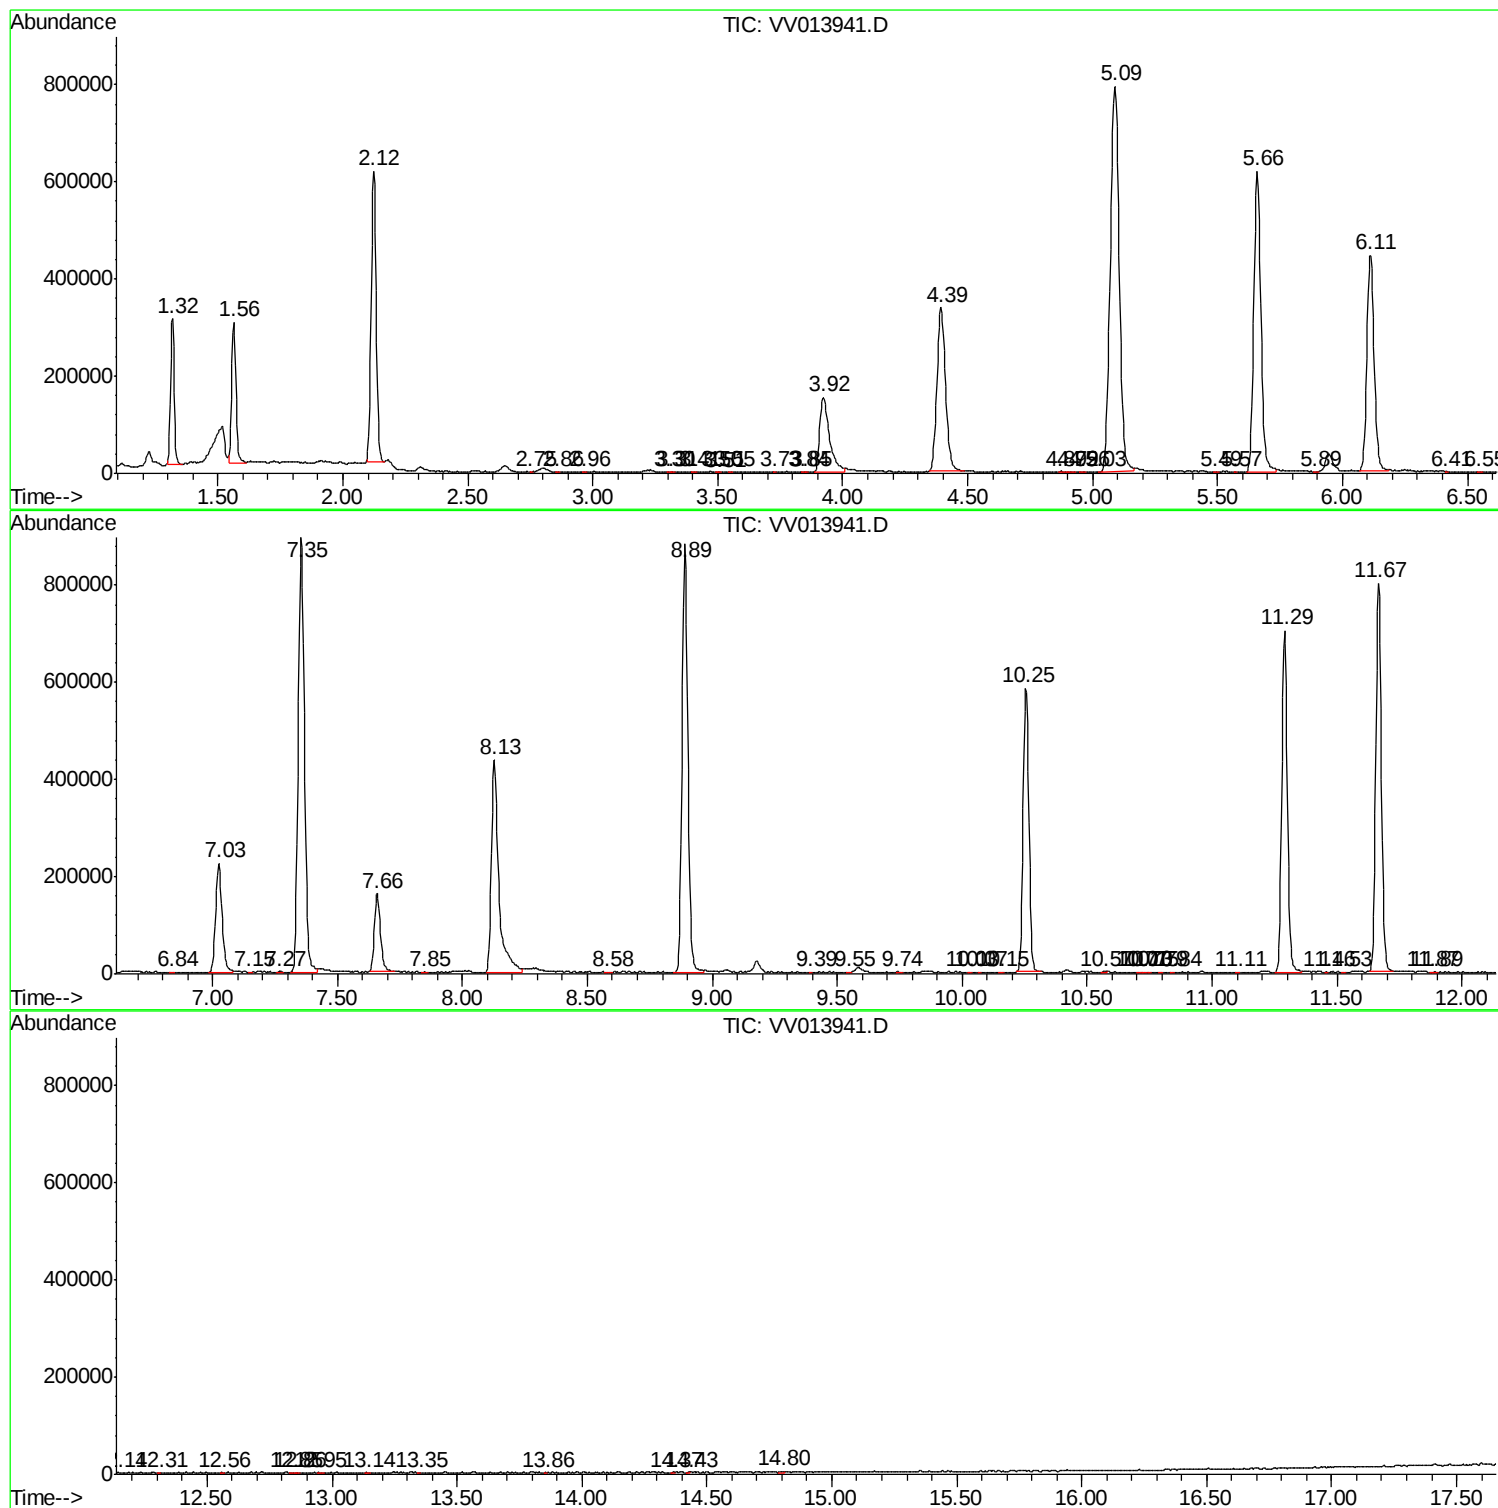

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013941.D
Acq On : 06 Dec 2019 14:37
Operator : SY/MD
Sample : K6190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFR97

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013941.D
Acq On : 06 Dec 2019 14:37
Operator : SY/MD
Sample : K6190-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFR97

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc