

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013944.D
 Acq On : 06 Dec 2019 15:49
 Operator : SY/MD
 Sample : K6165-10RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBW5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	83	rVB	320447	314018	8.63%	1.355%
2	1.570	142	149	160	rVB	334114	383964	10.55%	1.657%
3	2.126	313	322	334	rBV	676319	937519	25.76%	4.046%
4	2.309	372	379	391	rVB3	14196	24660	0.68%	0.106%
5	2.537	446	450	457	rVB7	3308	3598	0.10%	0.016%
6	2.569	457	460	463	rBV4	1509	873	0.02%	0.004%
7	2.653	475	486	499	rBV2	9180	19364	0.53%	0.084%
8	2.795	522	530	533	rBV9	2827	4105	0.11%	0.018%
9	2.978	581	587	588	rBV4	1671	1514	0.04%	0.007%
10	3.142	635	638	641	rVB5	1445	1080	0.03%	0.005%
11	3.174	646	648	652	rVB2	1677	881	0.02%	0.004%
12	3.209	656	659	661	rBV3	1544	951	0.03%	0.004%
13	3.251	669	672	674	rBV4	1275	923	0.03%	0.004%
14	3.679	803	805	813	rVB7	1142	1085	0.03%	0.005%
15	3.772	830	834	837	rVV5	1427	1034	0.03%	0.004%
16	3.852	853	859	865	rVB8	1924	2884	0.08%	0.012%
17	3.885	865	869	870	rBV3	1749	1255	0.03%	0.005%
18	3.923	870	881	907	rBV	175970	480440	13.20%	2.073%
19	4.399	1011	1029	1056	rBV2	433829	1272865	34.97%	5.493%
20	4.663	1110	1111	1116	rVB4	2127	1259	0.03%	0.005%
21	4.688	1116	1119	1122	rBV5	1871	1295	0.04%	0.006%
22	4.788	1147	1150	1155	rVB7	1588	1181	0.03%	0.005%
23	4.856	1168	1171	1173	rBV4	1301	939	0.03%	0.004%
24	5.026	1220	1224	1226	rBV3	1532	1127	0.03%	0.005%
25	5.090	1226	1244	1267	rBV2	937456	2343182	64.38%	10.112%
26	5.518	1374	1377	1380	rBV6	1416	1150	0.03%	0.005%
27	5.659	1407	1421	1448	rVV	1588902	3069564	84.33%	13.247%
28	5.946	1499	1510	1524	rVB3	41101	81688	2.24%	0.353%
29	6.113	1548	1562	1582	rBV	521625	1057454	29.05%	4.563%
30	6.364	1637	1640	1647	rVB6	1599	1911	0.05%	0.008%
31	6.396	1647	1650	1653	rBV5	1677	1060	0.03%	0.005%
32	6.489	1675	1679	1684	rVB6	2246	2554	0.07%	0.011%
33	6.553	1684	1699	1716	rBV	85258	168375	4.63%	0.727%
34	6.637	1721	1725	1726	rBV3	3428	1717	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013944.D
 Acq On : 06 Dec 2019 15:49
 Operator : SY/MD
 Sample : K6165-10RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBW5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.785	1766	1771	1773	rBV6	1550	1084	0.03%	0.005%
36	6.865	1792	1796	1799	rVB4	2045	1565	0.04%	0.007%
37	6.891	1799	1804	1806	rBV5	1431	1403	0.04%	0.006%
38	6.933	1811	1817	1821	rVB9	2422	2371	0.07%	0.010%
39	7.026	1834	1846	1870	rBV	274725	492386	13.53%	2.125%
40	7.235	1909	1911	1915	rVB4	1859	946	0.03%	0.004%
41	7.273	1915	1923	1935	rBV5	8213	15710	0.43%	0.068%
42	7.357	1936	1949	1967	rBV	1068524	1851285	50.86%	7.989%
43	7.659	2032	2043	2066	rBV	194085	354878	9.75%	1.531%
44	7.810	2086	2090	2093	rBV5	1028	928	0.03%	0.004%
45	7.839	2097	2099	2102	rBV3	1404	940	0.03%	0.004%
46	7.949	2128	2133	2135	rVV4	1829	1374	0.04%	0.006%
47	7.974	2135	2141	2145	rVV8	3081	4208	0.12%	0.018%
48	8.016	2145	2154	2164	rVV3	14206	24789	0.68%	0.107%
49	8.126	2177	2188	2218	rBV2	486234	1019813	28.02%	4.401%
50	8.286	2230	2238	2252	rVB3	39386	73197	2.01%	0.316%
51	8.582	2326	2330	2332	rBV5	2069	1523	0.04%	0.007%
52	8.653	2348	2352	2354	rVB5	1626	1312	0.04%	0.006%
53	8.675	2354	2359	2362	rBV7	1541	1533	0.04%	0.007%
54	8.891	2412	2426	2446	rBV	2272379	3639869	100.00%	15.708%
55	9.277	2544	2546	2548	rBV3	1797	1103	0.03%	0.005%
56	9.441	2590	2597	2599	rBV6	1458	1331	0.04%	0.006%
57	9.492	2610	2613	2617	rBV5	1367	1155	0.03%	0.005%
58	9.585	2637	2642	2644	rBV5	2057	1838	0.05%	0.008%
59	9.855	2719	2726	2727	rBV7	3246	2887	0.08%	0.012%
60	9.971	2758	2762	2764	rBV4	2307	1833	0.05%	0.008%
61	10.154	2815	2819	2825	rBV7	1141	1207	0.03%	0.005%
62	10.254	2837	2850	2872	rBV	678253	1080108	29.67%	4.661%
63	10.376	2885	2888	2891	rBV5	1325	900	0.02%	0.004%
64	10.412	2891	2899	2909	rVV5	14191	22345	0.61%	0.096%
65	10.531	2931	2936	2938	rBV5	4006	3937	0.11%	0.017%
66	10.743	2999	3002	3005	rBV4	1706	1272	0.03%	0.005%
67	10.823	3021	3027	3029	rVV7	1531	1333	0.04%	0.006%
68	10.897	3045	3050	3055	rBV6	2033	2072	0.06%	0.009%
69	10.977	3071	3075	3078	rBV4	1482	1603	0.04%	0.007%
70	11.090	3107	3110	3112	rBV3	1369	897	0.02%	0.004%
71	11.116	3112	3118	3119	rBV4	1196	968	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013944.D
 Acq On : 06 Dec 2019 15:49
 Operator : SY/MD
 Sample : K6165-10RE
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBW5RE

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.151	3127	3129	3134	rVB5	1080	903	0.02%	0.004%
73	11.199	3139	3144	3145	rBV4	1206	1085	0.03%	0.005%
74	11.289	3158	3172	3192	rBV	1854605	2842099	78.08%	12.265%
75	11.569	3257	3259	3262	rVB4	1620	872	0.02%	0.004%
76	11.666	3276	3289	3306	rBV	951152	1490506	40.95%	6.432%
77	12.022	3395	3400	3402	rBV5	1158	1035	0.03%	0.004%
78	12.067	3412	3414	3417	rVB3	1702	896	0.02%	0.004%
79	12.212	3456	3459	3463	rVB5	1581	1218	0.03%	0.005%
80	12.276	3476	3479	3481	rBV2	1404	968	0.03%	0.004%
81	12.505	3546	3550	3552	rBV3	1361	1104	0.03%	0.005%
82	12.691	3600	3608	3611	rBV8	2266	2987	0.08%	0.013%
83	13.042	3713	3717	3720	rBV5	1490	1286	0.04%	0.006%
84	13.174	3756	3758	3764	rVB6	1379	988	0.03%	0.004%
85	13.219	3769	3772	3776	rBV3	1893	1507	0.04%	0.007%
86	13.302	3796	3798	3800	rBV3	2059	1214	0.03%	0.005%
87	13.334	3806	3808	3812	rVB3	1639	1141	0.03%	0.005%
88	13.633	3897	3901	3903	rVB5	1383	1036	0.03%	0.004%
89	13.887	3976	3980	3982	rBV4	1681	1313	0.04%	0.006%
90	13.913	3986	3988	3995	rVB7	1939	1773	0.05%	0.008%
91	13.948	3995	3999	4001	rBV3	1449	1111	0.03%	0.005%
92	13.993	4009	4013	4015	rBV5	1154	1036	0.03%	0.004%
93	14.080	4036	4040	4042	rBV3	1957	1388	0.04%	0.006%
94	14.283	4099	4103	4104	rBV3	1866	1227	0.03%	0.005%
95	14.418	4140	4145	4146	rBV3	1712	1222	0.03%	0.005%
96	14.559	4184	4189	4193	rVV8	1514	1629	0.04%	0.007%
97	14.672	4221	4224	4225	rBV3	1493	898	0.02%	0.004%
98	15.051	4337	4342	4345	rBV7	1622	1887	0.05%	0.008%
99	15.392	4445	4448	4450	rBV3	2182	1374	0.04%	0.006%
100	15.582	4506	4507	4511	rBV4	1847	1214	0.03%	0.005%


Sum of corrected areas: 23172289

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013944.D
Acq On : 06 Dec 2019 15:49
Operator : SY/MD
Sample : K6165-10RE
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW5RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

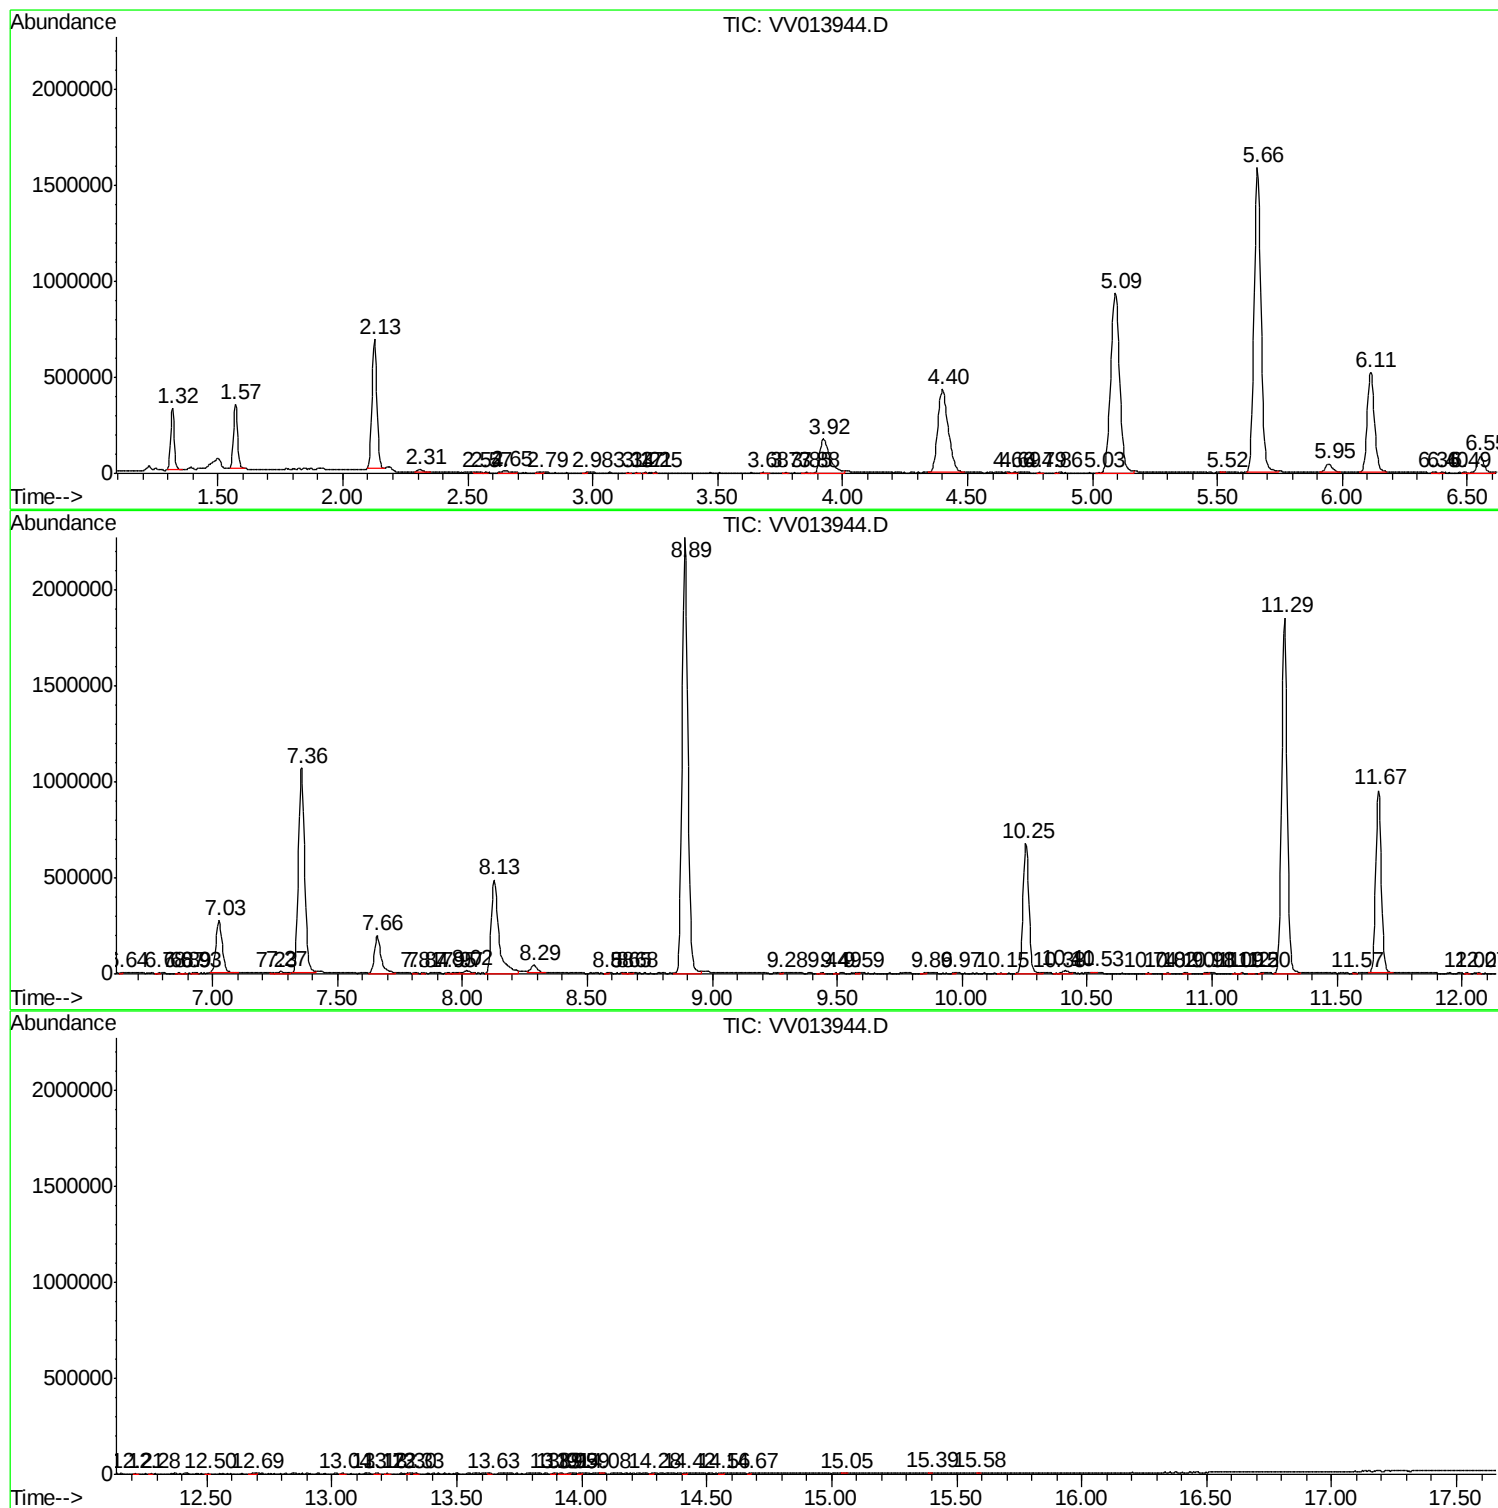

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013944.D
Acq On : 06 Dec 2019 15:49
Operator : SY/MD
Sample : K6165-10RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW5RE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013944.D
Acq On : 06 Dec 2019 15:49
Operator : SY/MD
Sample : K6165-10RE
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW5RE

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc