

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013949.D
 Acq On : 06 Dec 2019 19:34
 Operator : SY/MD
 Sample : K6170-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	84	rVB	297516	290221	15.03%	1.917%
2	1.560	141	146	162	rVB	274400	328809	17.03%	2.172%
3	2.123	313	321	333	rVB	581789	798420	41.35%	5.274%
4	2.615	472	474	476	rBV3	1296	418	0.02%	0.003%
5	2.637	476	481	483	rBV6	4968	4556	0.24%	0.030%
6	2.878	552	556	559	rBV5	1505	1367	0.07%	0.009%
7	2.901	559	563	565	rVV4	1260	957	0.05%	0.006%
8	3.148	638	640	644	rVB4	1622	1032	0.05%	0.007%
9	3.193	652	654	655	rVB2	739	183	0.01%	0.001%
10	3.241	666	669	670	rBV3	1672	952	0.05%	0.006%
11	3.264	670	676	679	rVV6	1944	2381	0.12%	0.016%
12	3.360	703	706	708	rBV3	792	568	0.03%	0.004%
13	3.396	715	717	719	rBV2	1000	626	0.03%	0.004%
14	3.512	750	753	754	rBV2	968	446	0.02%	0.003%
15	3.547	760	764	766	rBV4	1319	794	0.04%	0.005%
16	3.589	774	777	780	rBV4	1080	992	0.05%	0.007%
17	3.663	797	800	801	rBV2	924	649	0.03%	0.004%
18	3.685	805	807	811	rVB3	1734	1005	0.05%	0.007%
19	3.704	811	813	816	rBV3	1240	757	0.04%	0.005%
20	3.721	816	818	819	rBV2	894	405	0.02%	0.003%
21	3.772	832	834	836	rBV4	896	297	0.02%	0.002%
22	3.852	857	859	862	rBV3	1191	599	0.03%	0.004%
23	3.923	870	881	911	rBV	142582	388515	20.12%	2.566%
24	4.393	1013	1027	1052	rBV	327671	781203	40.46%	5.160%
25	4.807	1154	1156	1157	rBV2	588	148	0.01%	0.001%
26	4.856	1169	1171	1173	rBV3	852	310	0.02%	0.002%
27	4.875	1175	1177	1178	rBV2	943	386	0.02%	0.003%
28	4.910	1185	1188	1191	rBV4	840	729	0.04%	0.005%
29	4.984	1209	1211	1212	rBV	1126	419	0.02%	0.003%
30	5.090	1226	1244	1265	rBV2	767372	1930812	100.00%	12.754%
31	5.659	1407	1421	1446	rBV	688401	1385468	71.76%	9.152%
32	5.942	1501	1509	1525	rVB3	34113	66794	3.46%	0.441%
33	6.113	1548	1562	1595	rBV	438566	889054	46.05%	5.873%
34	6.431	1659	1661	1664	rBV4	1932	1358	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
 Data File : VV013949.D
 Acq On : 06 Dec 2019 19:34
 Operator : SY/MD
 Sample : K6170-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BW6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	6.489	1677	1679	1682	rBV3	1073	725	0.04%	0.005%
36	6.646	1724	1728	1729	rBV4	2460	1869	0.10%	0.012%
37	6.772	1765	1767	1774	rVB4	2044	2075	0.11%	0.014%
38	6.798	1774	1775	1776	rBV	1178	324	0.02%	0.002%
39	6.849	1789	1791	1792	rBV3	570	127	0.01%	0.001%
40	6.859	1792	1794	1797	rBV3	1569	915	0.05%	0.006%
41	7.023	1832	1845	1865	rBV	222117	402604	20.85%	2.659%
42	7.354	1936	1948	1967	rBV	889710	1519627	78.70%	10.038%
43	7.659	2033	2043	2062	rBV2	156614	266038	13.78%	1.757%
44	7.846	2099	2101	2102	rBV2	2155	802	0.04%	0.005%
45	8.129	2178	2189	2226	rBV3	420923	907465	47.00%	5.994%
46	8.566	2321	2325	2332	rBV10	2622	2700	0.14%	0.018%
47	8.843	2409	2411	2412	rBV2	1057	343	0.02%	0.002%
48	8.891	2414	2426	2450	rVV	1023553	1663398	86.15%	10.988%
49	9.338	2561	2565	2567	rBV4	1302	995	0.05%	0.007%
50	9.370	2571	2575	2576	rBV3	1151	882	0.05%	0.006%
51	9.402	2583	2585	2589	rBV4	1208	797	0.04%	0.005%
52	9.421	2589	2591	2593	rBV3	1082	411	0.02%	0.003%
53	9.508	2616	2618	2622	rBV5	1390	1037	0.05%	0.007%
54	9.540	2626	2628	2631	rBV3	916	625	0.03%	0.004%
55	9.634	2655	2657	2663	rVB5	1069	813	0.04%	0.005%
56	9.775	2699	2701	2703	rBV3	1044	445	0.02%	0.003%
57	10.026	2777	2779	2781	rBV4	687	373	0.02%	0.002%
58	10.064	2790	2791	2795	rBV3	720	504	0.03%	0.003%
59	10.151	2816	2818	2820	rBV3	886	487	0.03%	0.003%
60	10.254	2838	2850	2867	rBV	598695	927704	48.05%	6.128%
61	10.502	2925	2927	2932	rVB4	1194	616	0.03%	0.004%
62	10.531	2934	2936	2941	rBV4	1261	967	0.05%	0.006%
63	10.932	3057	3061	3063	rBV4	1088	726	0.04%	0.005%
64	11.183	3137	3139	3140	rBV2	869	275	0.01%	0.002%
65	11.289	3160	3172	3190	rBV	841449	1296336	67.14%	8.563%
66	11.666	3278	3289	3307	rBV	802372	1246157	64.54%	8.232%
67	12.235	3464	3466	3470	rBV4	1494	1322	0.07%	0.009%
68	12.672	3598	3602	3603	rBV3	1136	830	0.04%	0.005%
69	13.132	3743	3745	3746	rBV	1155	362	0.02%	0.002%
70	13.203	3764	3767	3773	rBV5	1690	1430	0.07%	0.009%
71	13.547	3869	3874	3875	rBV5	2195	1784	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013949.D
Acq On : 06 Dec 2019 19:34
Operator : SY/MD
Sample : K6170-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	13.852	3967	3969	3971	rBV2	1273	599	0.03%	0.004%
73	14.109	4047	4049	4050	rBV	1571	678	0.04%	0.004%
74	14.598	4200	4201	4203	rBV2	1208	613	0.03%	0.004%


Sum of corrected areas: 15138410

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120619\
Data File : VV013949.D
Acq On : 06 Dec 2019 19:34
Operator : SY/MD
Sample : K6170-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0BW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

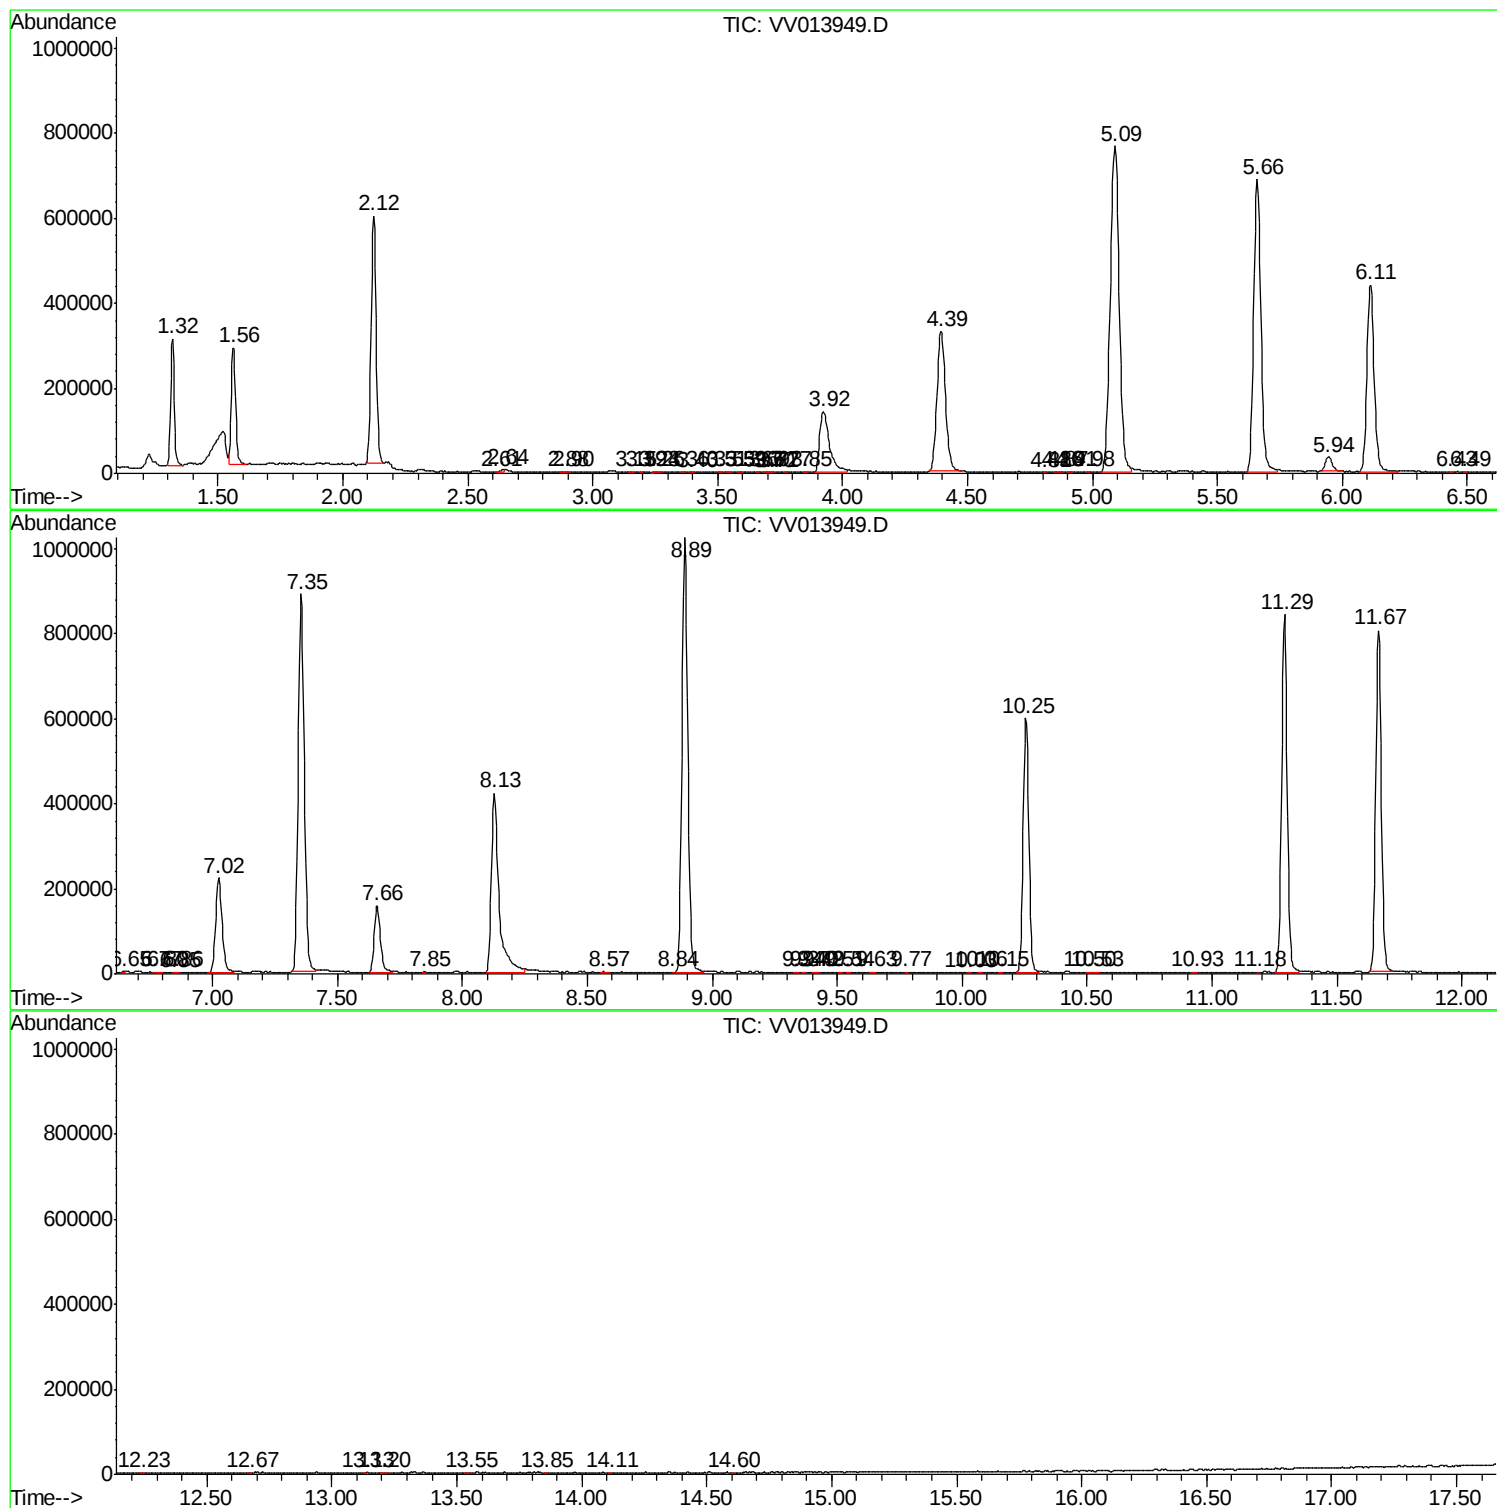

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013949.D
Acq On : 06 Dec 2019 19:34
Operator : SY/MD
Sample : K6170-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120619\
Data File : VV013949.D
Acq On : 06 Dec 2019 19:34
Operator : SY/MD
Sample : K6170-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BW6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc