


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120619\
Data File : VV013931.D
Acq On : 06 Dec 2019 09:06
Operator : SY/MD
Sample : BFB77
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis
Last Update : Sat Dec 07 01:39:07 2019

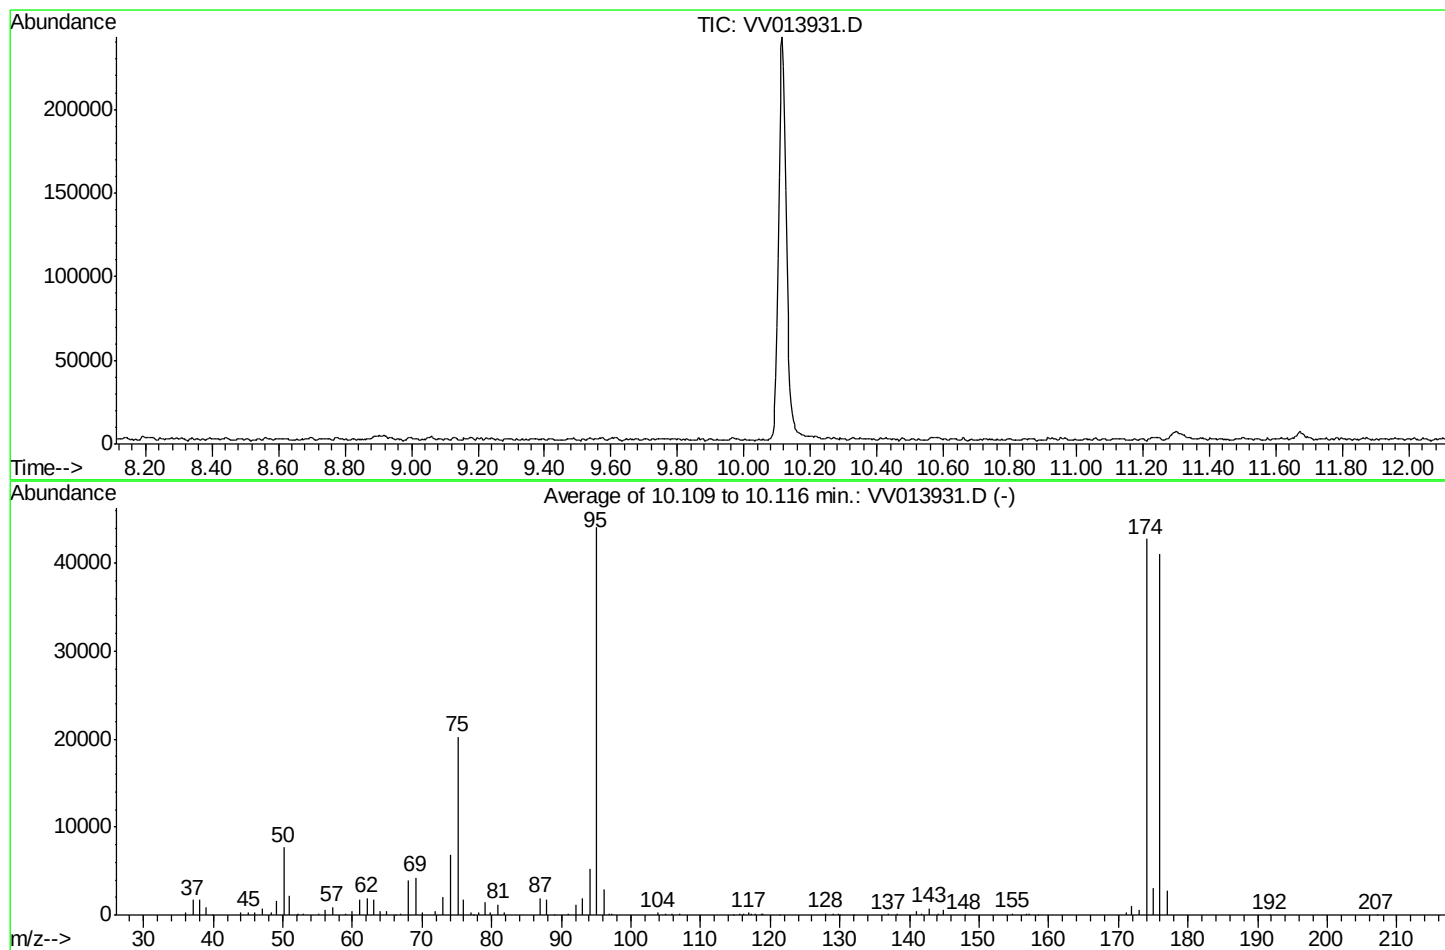

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	7712	PASS
75	95	30	80	45.9	20237	PASS
95	95	100	100	100.0	44090	PASS
96	95	5	9	6.7	2933	PASS
173	174	0.00	2	1.4	613	PASS
174	95	50	120	96.9	42741	PASS
175	174	5	9	7.2	3067	PASS
176	174	95	101	95.9	41005	PASS
177	176	5	9	6.9	2824	PASS

m/z	Abundance
36.20	414.0
37.10	1644.0
38.10	1646.0
39.10	931.0
39.90	639.0
43.90	554.0
45.00	327.0
46.00	249.0
47.00	613.0
48.30	193.0
49.00	1443.0
50.10	7182.0
51.00	2093.0
52.00	209.0
53.00	134.0
55.00	142.0
56.10	505.0
57.10	806.0
59.90	469.0
61.00	1646.0
62.10	1886.0
63.10	1657.0
64.00	439.0
64.90	383.0
66.90	197.0
68.00	3551.0
69.10	4019.0
70.00	209.0
72.00	396.0
72.90	1848.0
74.10	5809.0
75.10	18104.0
76.00	1531.0
76.90	224.0
77.30	215.0
78.10	256.0
79.00	1337.0
79.80	275.0
80.90	1266.0
81.90	388.0
87.00	1598.0
87.90	1514.0
91.10	221.0
92.00	1144.0
93.00	1737.0
94.10	4673.0
95.00	40544.0
96.10	2592.0
96.90	156.0
103.90	223.0
104.90	144.0
105.80	182.0
106.90	128.0
115.60	130.0
116.90	361.0
117.80	158.0
118.80	304.0
128.00	219.0
129.00	103.0
129.70	144.0
129.90	143.0
137.00	108.0
141.00	352.0
142.90	711.0
144.10	135.0
145.00	394.0
147.90	119.0
155.00	168.0
156.70	111.0
157.10	124.0
171.10	280.0
172.00	844.0
174.00	37792.0
175.00	2727.0
176.00	36280.0
177.00	2513.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.10	408.0
37.10	1760.0
38.10	1738.0
39.00	986.0
39.90	568.0
44.00	488.0
45.10	354.0
45.90	228.0
47.00	792.0
48.20	227.0
49.00	1678.0
50.10	7913.0
51.00	2330.0
52.20	161.0
53.00	175.0
55.10	184.0
56.10	584.0
57.10	926.0
59.00	144.0
60.00	448.0
61.00	1970.0
62.00	1957.0
63.10	1809.0
64.00	459.0
64.90	457.0
66.10	112.0
66.90	232.0
68.10	3985.0
69.10	4384.0
70.00	291.0
71.90	423.0
72.90	2051.0
74.10	7064.0
75.10	21088.0
76.00	1817.0
77.00	348.0
78.00	217.0
79.00	1482.0
79.80	329.0
80.90	1246.0
81.90	344.0
87.00	1967.0
87.90	1876.0
91.10	226.0
92.00	1131.0
93.00	2019.0
94.10	5487.0
95.00	45928.0
96.00	3084.0
96.90	140.0
97.30	114.0
103.90	266.0
104.90	165.0
105.80	227.0
106.90	149.0
115.70	151.0
116.20	142.0
117.00	440.0
117.80	228.0
118.80	268.0
128.00	244.0
129.00	132.0
129.70	223.0
136.90	134.0
138.20	109.0
141.00	428.0
141.80	151.0
142.90	851.0
144.00	122.0
144.90	537.0
154.80	169.0
156.80	147.0
157.10	166.0
171.00	321.0
172.00	1128.0
173.00	950.0
174.00	44248.0
175.00	3156.0
175.90	42560.0
176.90	2905.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

m/z	Abundance
36.10	396.0
37.00	1799.0
38.10	1662.0
39.00	913.0
39.90	490.0
44.20	508.0
45.20	379.0
45.90	291.0
47.00	835.0
48.20	278.0
49.00	1671.0
50.10	8041.0
51.00	2349.0
52.30	149.0
53.00	172.0
55.10	218.0
56.10	689.0
57.10	942.0
59.10	169.0
60.00	454.0
61.00	2156.0
62.10	1949.0
63.10	1735.0
64.00	429.0
64.90	446.0
67.00	202.0
68.00	4094.0
69.00	4311.0
70.00	431.0
71.90	312.0
73.00	2056.0
74.00	7545.0
75.10	21520.0
76.00	2023.0
77.00	378.0
78.00	221.0
79.00	1496.0
79.90	417.0
80.90	1200.0
81.80	268.0
87.00	2182.0
87.90	2030.0
88.90	108.0
91.00	191.0
92.00	1045.0
93.00	2040.0
94.10	5679.0
95.00	45800.0
96.00	3124.0
97.20	144.0
103.90	268.0
104.90	118.0
105.80	244.0
106.90	129.0
114.70	132.0
116.20	202.0
117.20	465.0
117.80	239.0
119.00	251.0
121.40	118.0
128.00	184.0
129.00	137.0
129.70	231.0
132.00	103.0
136.90	153.0
138.20	130.0
141.00	566.0
141.80	160.0
142.90	837.0
144.00	121.0
144.80	661.0
154.80	166.0
156.70	132.0
157.10	136.0
158.50	102.0
171.00	331.0
171.90	1169.0
173.00	891.0
174.00	46184.0
175.00	3320.0
175.90	44176.0
176.90	3054.0
191.80	114.0
207.10	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77

Scan 2794 (10.074 min): VV013931.D
BFB77

m/z	Abundance
35.40	123.0
36.00	148.0
36.40	136.0
37.50	143.0
40.00	530.0
42.50	128.0
43.40	143.0
44.10	384.0
47.60	210.0
51.10	125.0
60.80	110.0
63.60	119.0
114.10	123.0
146.00	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB77