

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120621\
 Data File : VW023792.D
 Acq On : 06 Dec 2021 12:51
 Operator : SY/MD
 Sample : VW1206WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Quant Time: Dec 07 05:29:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	131259	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	124967	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61037	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	53982	5.010	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.564	69	39036	4.609	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	92.200%	
11) 1,1-Dichloroethene-d2	2.105	63	73999	3.897	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.000%	
20) 2-Butanone-d5	3.899	46	52874	40.818	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	81.640%	
24) Chloroform-d	4.342	84	89106	4.749	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.000%	
26) 1,2-Dichloroethane-d4	5.027	65	42524	4.851	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.000%	
32) Benzene-d6	5.047	84	179035	5.259	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.200%	
36) 1,2-Dichloropropane-d6	6.066	67	49874	5.226	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.600%	
41) Toluene-d8	7.313	98	164919	5.185	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.600%	
43) trans-1,3-Dichloroprop...	7.619	79	18648	4.848	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.000%	
46) 2-Hexanone-d5	8.088	63	71751	56.138	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	112.280%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	32013	4.662	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	61323	5.683	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	8130	0.648	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
Data File : VV023792.D
Acq On : 06 Dec 2021 12:51
Operator : SY/MD
Sample : VV1206WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Time: Dec 07 05:29:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration

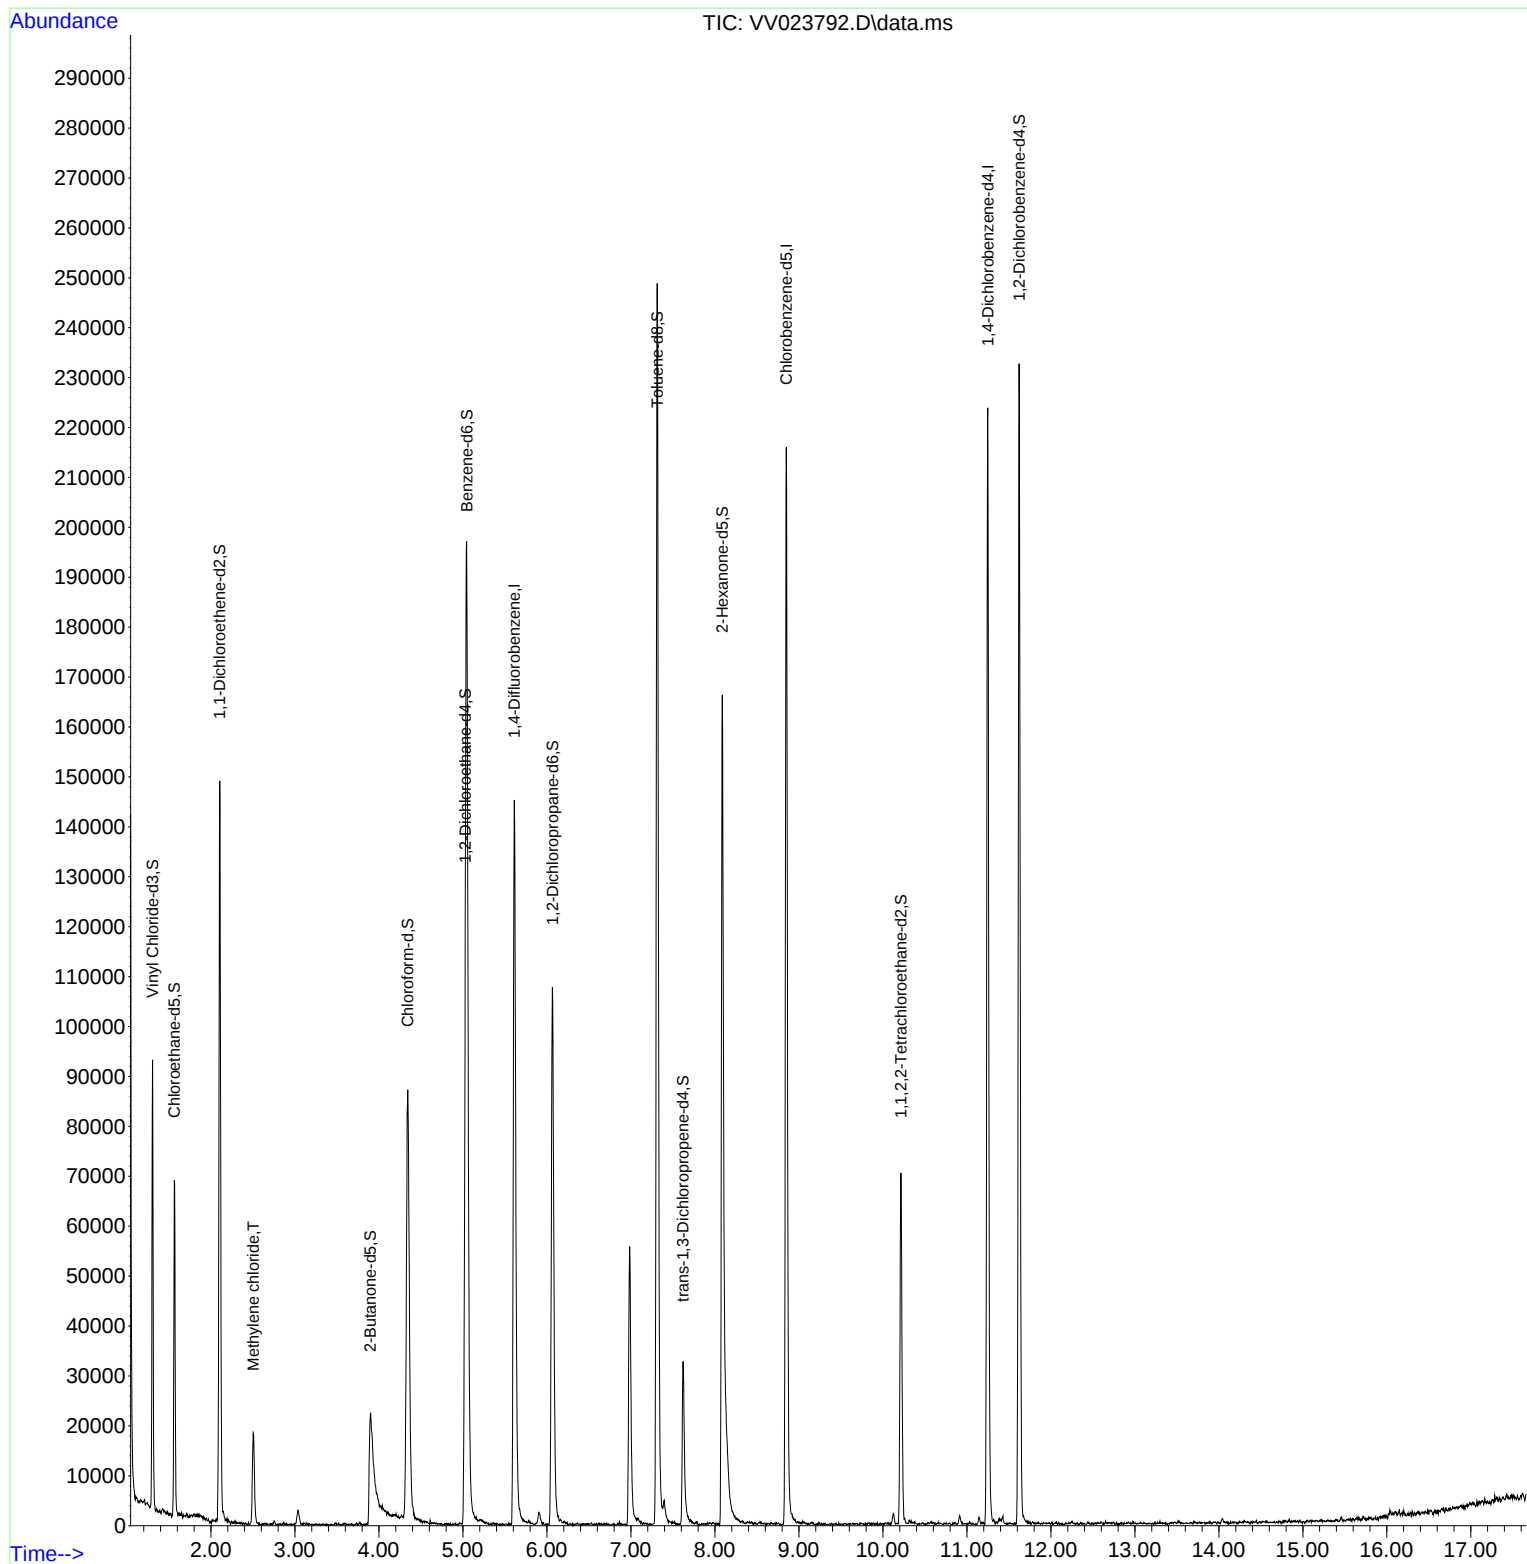

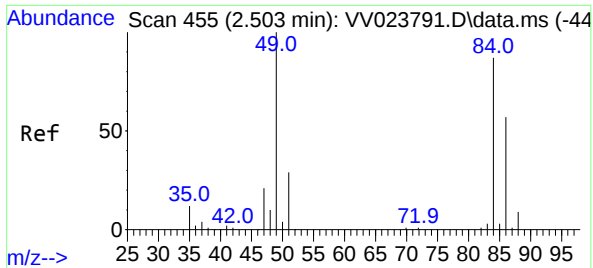

#16
Methylene chloride
Concen: 0.648 ug/L
RT: 2.503 min Scan# 4
Delta R.T. -0.003 min
Lab File: VV023792.D
Acq: 06 Dec 2021 12:51

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Tgt Ion: 84 Resp: 8130
Ion Ratio Lower Upper
84 100
86 63.3 42.6 79.0
49 103.3 79.7 147.9

