

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
 Data File : VV023792.D
 Acq On : 06 Dec 2021 12:51
 Operator : SY/MD
 Sample : VV1206WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	90465	90931	18.70%	2.352%
2	1.564	153	163	176	rBV	67504	76646	15.76%	1.983%
3	2.105	321	331	343	rBV	148203	207889	42.74%	5.378%
4	2.503	442	455	470	rBV	18303	32019	6.58%	0.828%
5	3.037	613	621	633	rVB5	2798	5232	1.08%	0.135%
6	3.902	879	890	911	rBV2	22406	78488	16.14%	2.030%
7	4.342	1012	1027	1053	rVB	85949	214232	44.05%	5.542%
8	5.043	1229	1245	1275	rBV3	196859	486381	100.00%	12.582%
9	5.612	1411	1422	1440	rBV	145137	295415	60.74%	7.642%
10	6.066	1551	1563	1583	rBV	107688	223407	45.93%	5.779%
11	6.985	1838	1849	1875	rBV	55824	107778	22.16%	2.788%
12	7.313	1937	1951	1971	rBV	248529	434197	89.27%	11.232%
13	7.397	1972	1977	1992	rVB6	4526	8315	1.71%	0.215%
14	7.622	2037	2047	2064	rBV	32628	60212	12.38%	1.558%
15	8.088	2182	2192	2229	rBV	166299	356958	73.39%	9.234%
16	8.850	2418	2429	2448	rBV	215747	360358	74.09%	9.322%
17	10.214	2843	2853	2865	rBV2	70334	113437	23.32%	2.934%
18	11.249	3164	3175	3194	rBV	223617	349939	71.95%	9.052%
19	11.622	3278	3291	3306	rBV	232511	363986	74.84%	9.415%




Sum of corrected areas: 3865820

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
Data File : VV023792.D
Acq On : 06 Dec 2021 12:51
Operator : SY/MD
Sample : VV1206WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

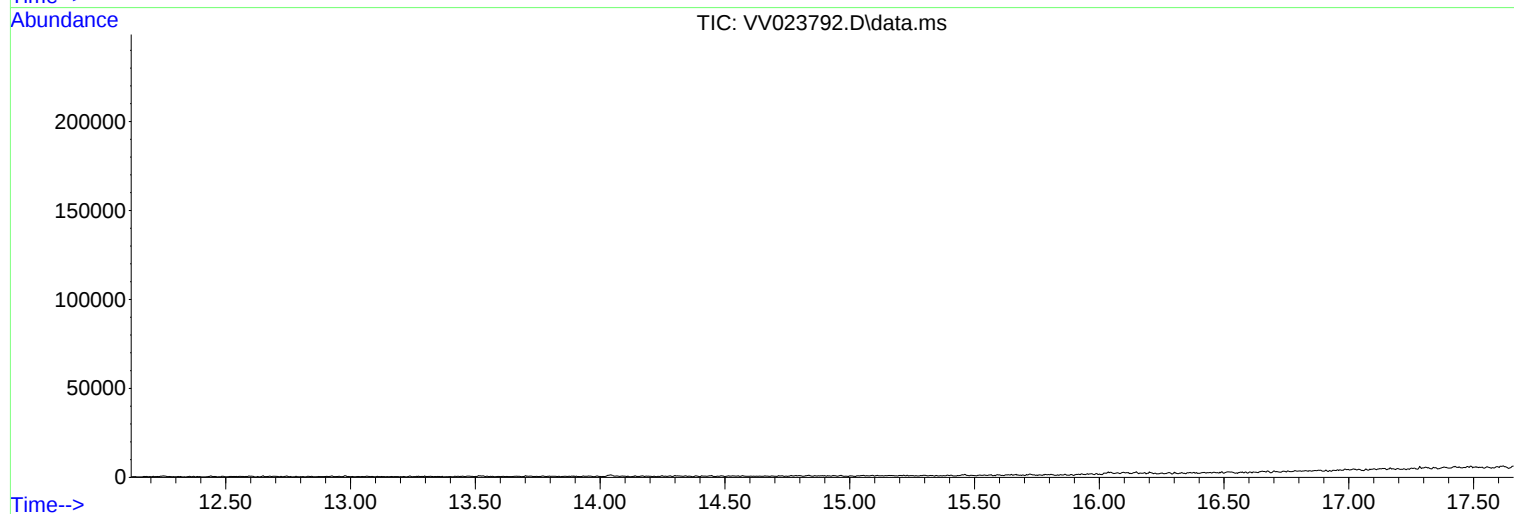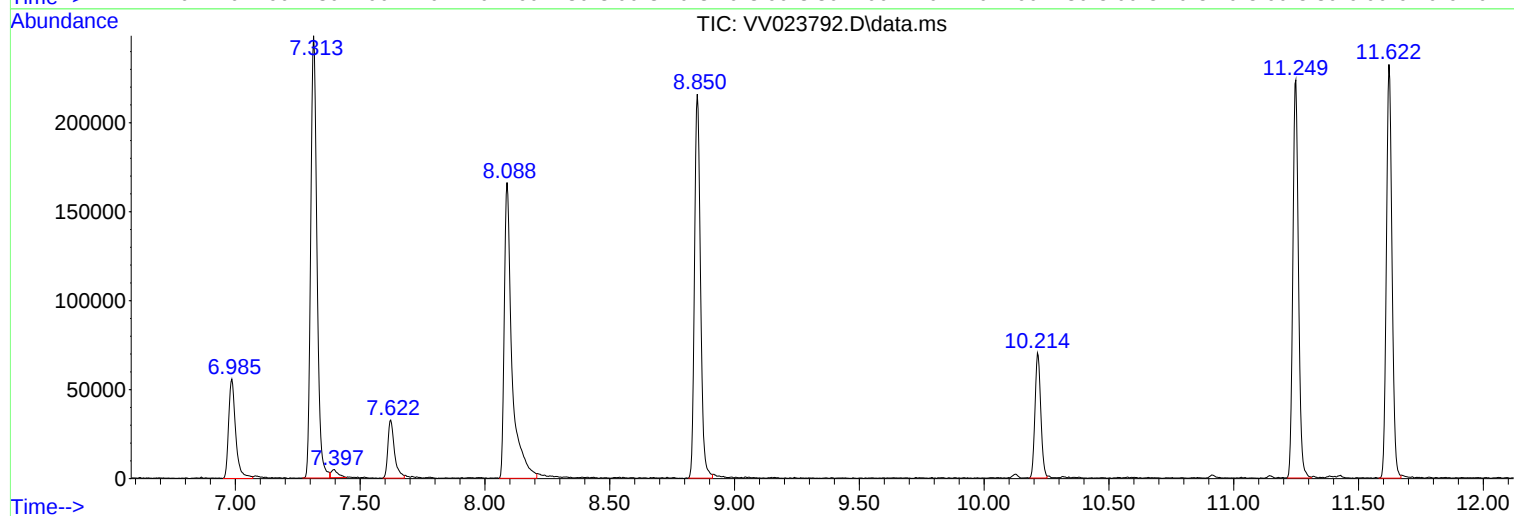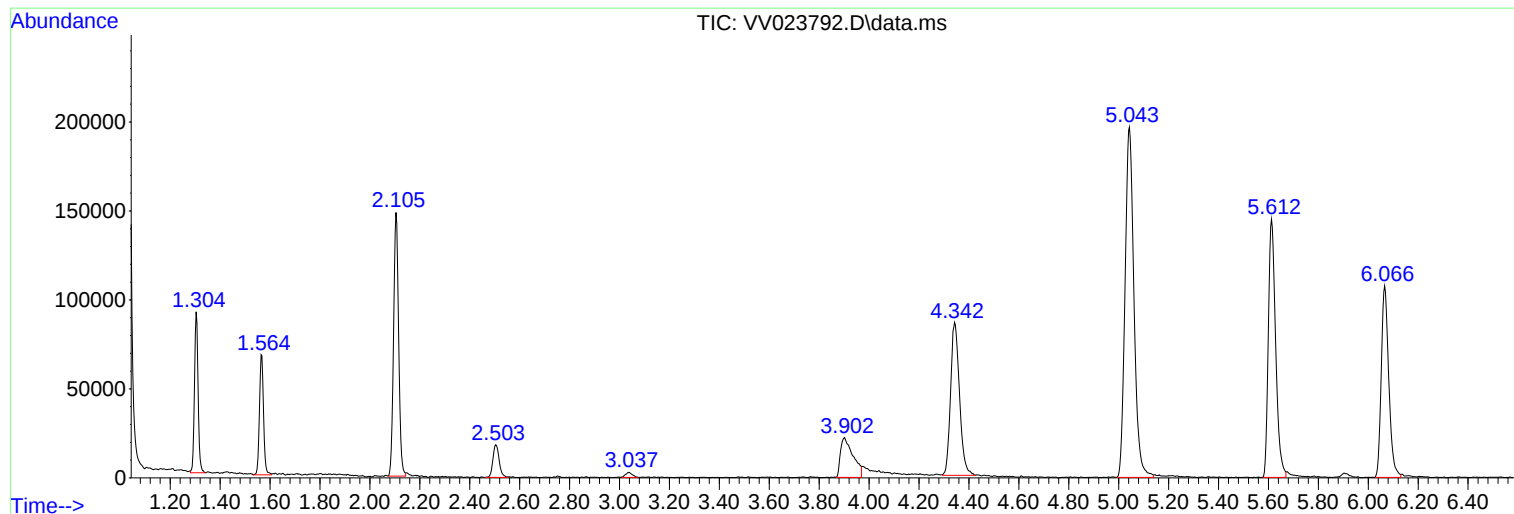

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
Data File : VV023792.D
Acq On : 06 Dec 2021 12:51
Operator : SY/MD
Sample : VV1206WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
Data File : VV023792.D
Acq On : 06 Dec 2021 12:51
Operator : SY/MD
Sample : VV1206WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc