
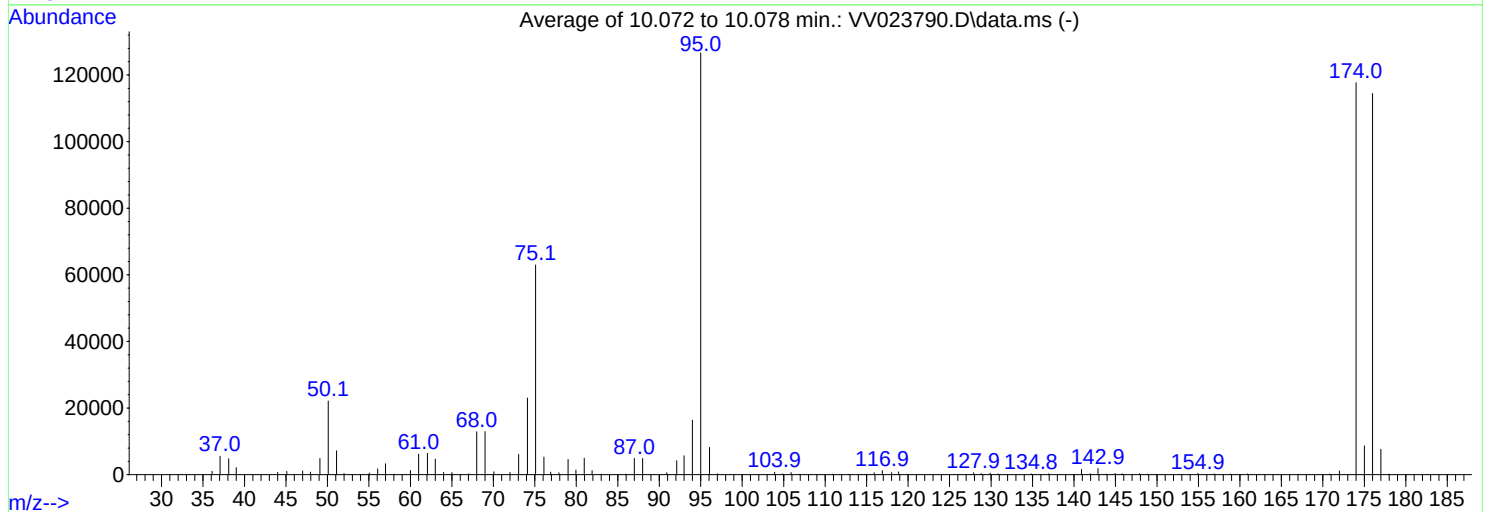


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120621\
 Data File : VV023790.D
 Acq On : 06 Dec 2021 09:23
 Operator : SY/MD
 Sample : BFB245
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB245

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 02 02:08:23 2021

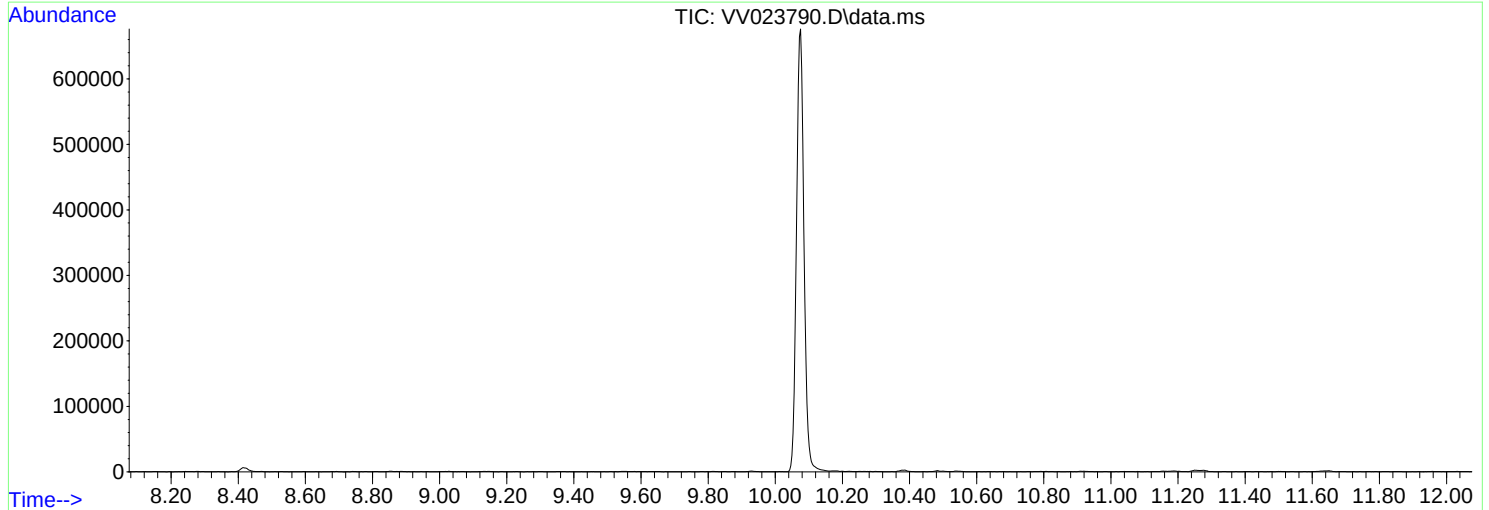

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	22123	PASS
75	95	30	80	49.7	62920	PASS
95	95	100	100	100.0	126651	PASS
96	95	5	9	6.5	8182	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.9	117693	PASS
175	174	5	9	7.4	8674	PASS
176	174	95	105	97.3	114469	PASS
177	176	5	10	6.7	7643	PASS

m/z	Abundance
39.90	153.0
44.00	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	988.0
37.00	4945.0
38.10	4358.0
39.00	1984.0
40.00	140.0
44.00	822.0
45.10	851.0
47.00	1181.0
47.90	720.0
49.10	4419.0
50.10	20688.0
51.10	6629.0
52.00	353.0
55.10	435.0
56.10	1630.0
57.00	2946.0
58.10	161.0
60.00	1245.0
61.00	5795.0
62.10	6114.0
63.00	4317.0
64.00	606.0
65.00	497.0
66.90	316.0
68.00	11881.0
69.00	12067.0
70.10	789.0
72.00	721.0
73.00	5734.0
74.10	21728.0
75.10	58192.0
76.10	4792.0
76.90	726.0
77.90	546.0
79.00	4259.0
80.00	1303.0
80.90	4664.0
81.90	1161.0
83.00	115.0
85.90	143.0
87.00	4434.0
88.00	4444.0
90.90	623.0
92.10	3965.0
93.00	5180.0
94.00	15499.0
95.00	119312.0
96.10	7820.0
97.00	264.0
103.90	609.0
104.90	241.0
105.90	666.0
107.00	136.0
110.00	112.0
110.90	134.0
112.80	104.0
114.90	189.0
115.90	598.0
116.90	1110.0
118.00	613.0
118.90	795.0
127.90	556.0
128.80	322.0
129.90	512.0
130.80	197.0
134.90	256.0
137.00	266.0
140.90	1551.0
141.90	255.0
142.90	1753.0
143.90	195.0
145.00	359.0
145.80	295.0
147.90	371.0
148.90	156.0
149.90	153.0
152.70	113.0
154.00	108.0
155.00	390.0
156.90	258.0
158.90	188.0
160.90	218.0
170.80	138.0
172.00	1010.0
174.00	112952.0
175.00	8065.0
176.00	110376.0
177.00	7143.0
177.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	1040.0
37.10	5788.0
38.10	5024.0
39.00	2228.0
40.00	204.0
44.00	836.0
45.10	1007.0
46.00	151.0
47.00	1160.0
47.90	830.0
49.10	5000.0
50.10	22880.0
51.10	7404.0
52.00	366.0
53.00	103.0
55.00	481.0
56.00	1753.0
57.00	3330.0
58.10	192.0
60.00	1311.0
61.00	6402.0
62.00	6652.0
63.00	4821.0
64.00	735.0
65.00	664.0
66.20	129.0
67.10	323.0
68.00	13399.0
69.00	13498.0
70.00	891.0
72.00	692.0
73.10	6296.0
74.10	23944.0
75.10	64952.0
76.10	5460.0
76.90	751.0
77.90	600.0
79.00	4763.0
79.90	1452.0
80.90	5071.0
81.90	1281.0
83.00	152.0
86.00	156.0
87.00	4942.0
88.00	5034.0
90.90	579.0
92.10	4363.0
93.00	5877.0
94.00	17024.0
95.00	130888.0
96.10	8425.0
97.10	307.0
103.90	783.0
104.90	268.0
105.90	705.0
106.90	167.0
110.00	114.0
110.90	168.0
111.80	108.0
112.80	134.0
115.00	186.0
115.90	620.0
116.90	1254.0
118.00	635.0
118.90	816.0
127.90	595.0
128.80	376.0
129.90	513.0
130.90	242.0
134.80	235.0
137.00	270.0
140.00	149.0
140.90	1638.0
141.90	323.0
142.90	1914.0
143.80	211.0
144.90	406.0
145.80	316.0
147.90	347.0
148.90	151.0
149.90	167.0
155.00	384.0
156.90	285.0
158.90	216.0
160.90	248.0
170.80	207.0
172.00	1174.0
174.00	121944.0
175.00	8960.0
176.00	119072.0
177.00	8010.0
177.90	233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

m/z	Abundance
36.10	1017.0
37.10	5869.0
38.10	4992.0
39.00	2175.0
40.00	221.0
44.00	826.0
45.10	1024.0
46.00	201.0
47.00	974.0
48.00	816.0
49.10	5127.0
50.10	22800.0
51.10	7391.0
52.00	313.0
53.00	129.0
55.00	525.0
56.00	1774.0
57.00	3484.0
58.00	164.0
60.00	1185.0
61.00	6302.0
62.00	6442.0
63.00	4852.0
64.00	769.0
65.00	684.0
66.10	133.0
67.10	271.0
68.00	13299.0
69.00	13160.0
70.00	948.0
72.00	625.0
73.10	6109.0
74.10	23376.0
75.10	65616.0
76.10	5586.0
76.90	780.0
77.90	566.0
79.00	4735.0
79.90	1410.0
81.00	5061.0
81.90	1188.0
83.00	199.0
86.00	154.0
87.00	5274.0
88.00	5084.0
90.90	502.0
92.10	4167.0
93.00	5930.0
94.00	16584.0
95.00	129752.0
96.00	8302.0
97.10	301.0
103.90	831.0
104.90	277.0
105.90	585.0
106.90	179.0
110.00	101.0
110.90	177.0
111.80	126.0
112.80	143.0
114.90	156.0
115.90	541.0
116.90	1203.0
118.00	589.0
118.80	808.0
127.90	596.0
128.80	379.0
129.90	487.0
130.90	240.0
134.80	212.0
136.90	259.0
139.90	141.0
140.90	1591.0
142.00	335.0
142.90	1897.0
143.80	182.0
145.00	449.0
145.80	309.0
147.90	341.0
148.80	151.0
149.90	158.0
153.70	100.0
154.90	337.0
156.90	263.0
158.90	203.0
160.90	213.0
170.80	250.0
172.00	1167.0
174.00	118184.0
175.00	8997.0
176.00	113960.0
177.00	7775.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245

178.00

239.0

Instrument :
MSVOA_V
ClientSampleId :
BFB245