

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
 Data File : VV029404.D
 Acq On : 06 Dec 2022 10:40
 Operator : SY/MD
 Sample : VV1206WBL06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK285

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	108753	108439	17.50%	2.083%
2	1.565	156	163	177	rVB	80157	90206	14.56%	1.733%
3	2.105	320	331	350	rBV	158790	227168	36.67%	4.364%
4	2.507	446	456	468	rVB3	6531	10777	1.74%	0.207%
5	3.912	881	893	942	rBV2	33985	159692	25.78%	3.068%
6	4.343	1010	1027	1059	rBV2	103415	256784	41.45%	4.933%
7	5.040	1227	1244	1274	rBV2	246056	619535	100.00%	11.901%
8	5.609	1408	1421	1441	rBV	225958	470021	75.87%	9.029%
9	6.063	1548	1562	1584	rBV	134974	281735	45.48%	5.412%
10	6.982	1836	1848	1880	rBV	70584	136209	21.99%	2.617%
11	7.310	1935	1950	1970	rBV	306839	552642	89.20%	10.616%
12	7.616	2032	2045	2071	rBV	40168	75429	12.18%	1.449%
13	8.085	2180	2191	2225	rBV	223173	456330	73.66%	8.766%
14	8.844	2412	2427	2450	rBV	331850	551941	89.09%	10.603%
15	10.207	2839	2851	2868	rBV	97007	152222	24.57%	2.924%
16	11.239	3160	3172	3190	rBV	374271	578345	93.35%	11.110%
17	11.612	3276	3288	3304	rBV	288316	458546	74.01%	8.809%
18	12.243	3472	3484	3495	rBV3	4796	8437	1.36%	0.162%
19	14.030	4029	4040	4050	rBV2	7037	11244	1.81%	0.216%




Sum of corrected areas: 5205702

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029404.D
Acq On : 06 Dec 2022 10:40
Operator : SY/MD
Sample : VV1206WBL06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

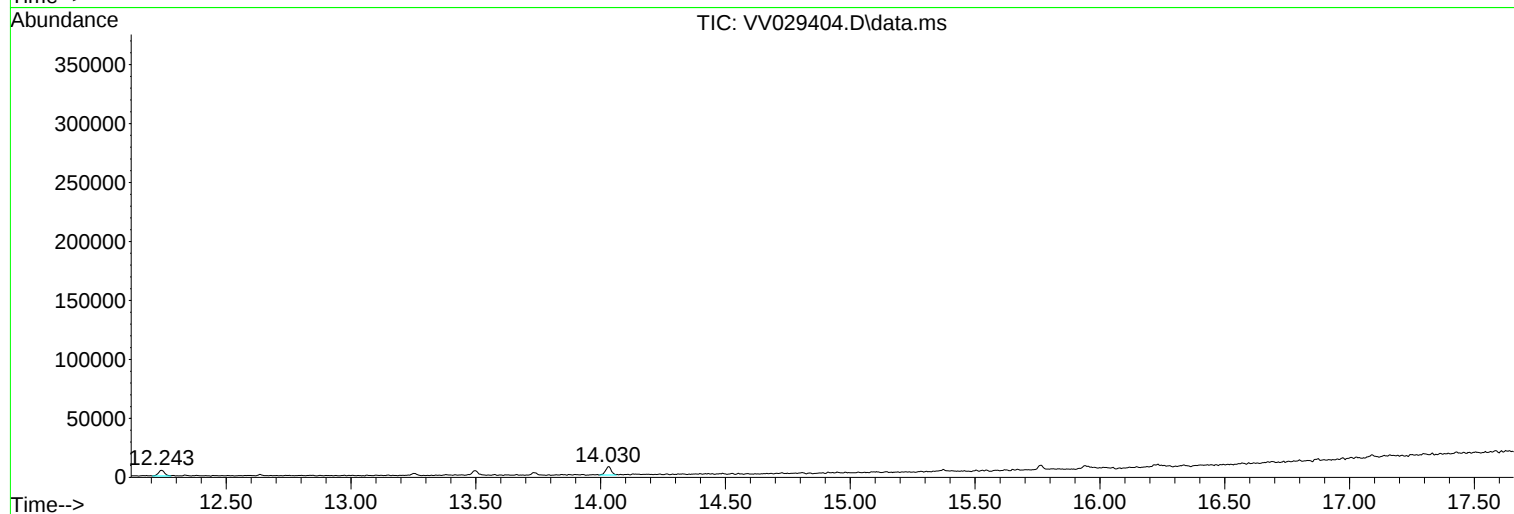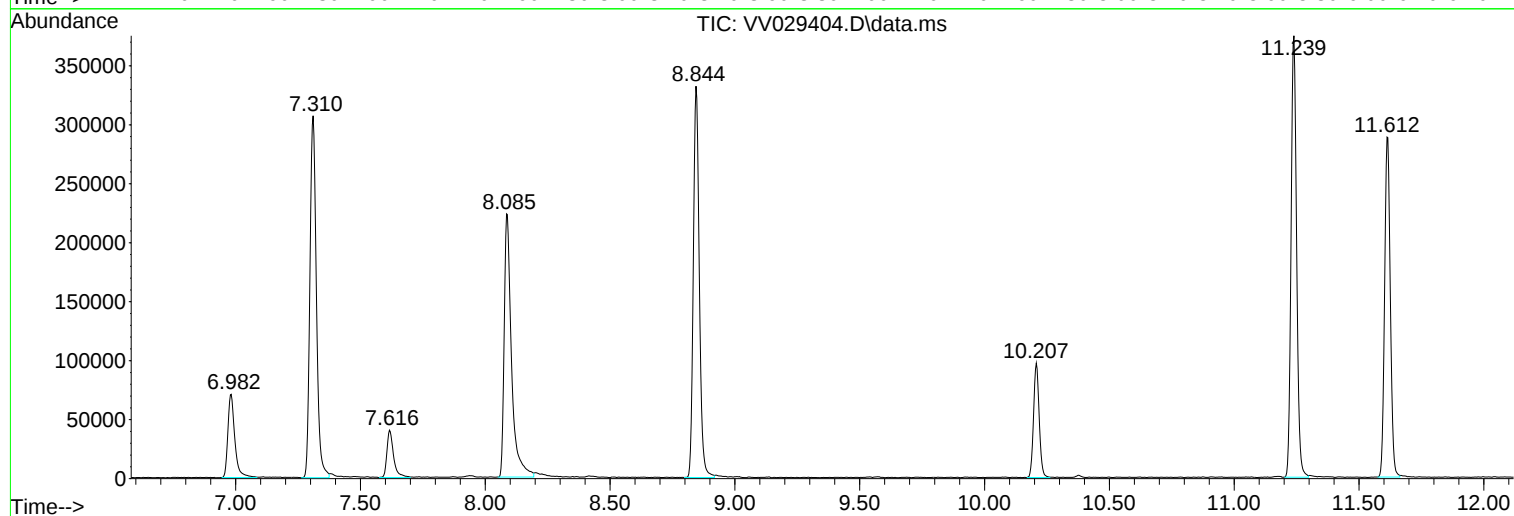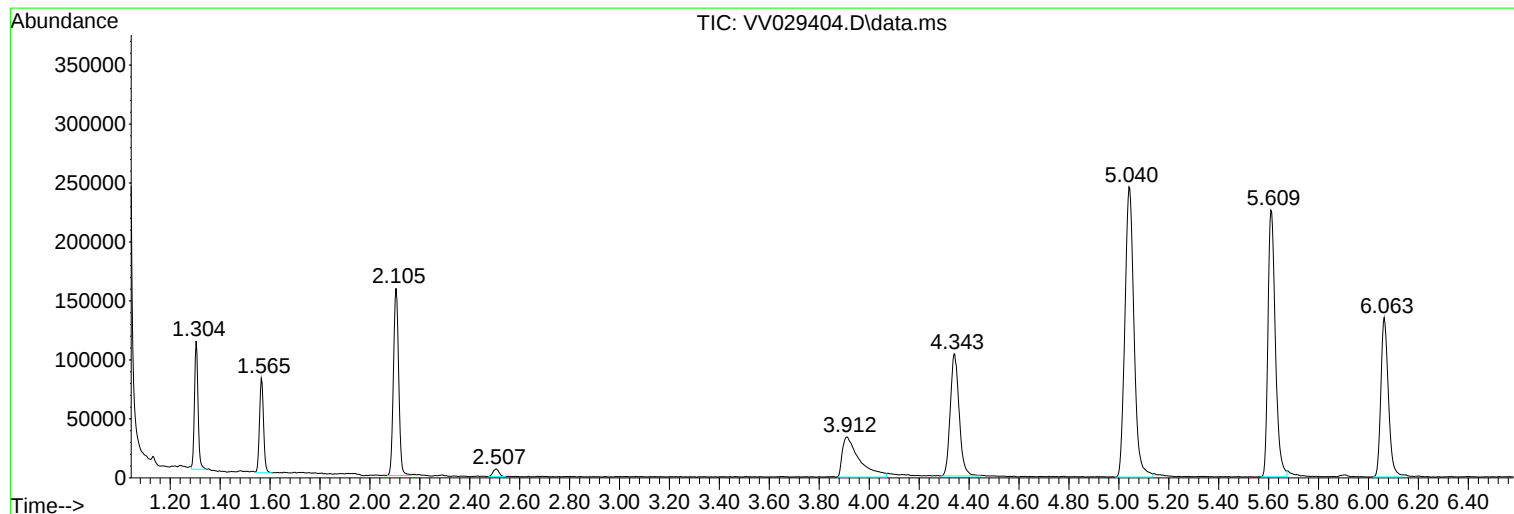

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029404.D
Acq On : 06 Dec 2022 10:40
Operator : SY/MD
Sample : VV1206WBL06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029404.D
Acq On : 06 Dec 2022 10:40
Operator : SY/MD
Sample : VV1206WBL06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc