

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
 Data File : VV029405.D
 Acq On : 06 Dec 2022 11:04
 Operator : SY/MD
 Sample : VV1206WBL07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK286

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	105632	108027	18.20%	2.112%
2	1.564	155	163	175	rBV	79777	89862	15.14%	1.757%
3	2.105	320	331	347	rBV	151838	217538	36.65%	4.254%
4	2.503	446	455	465	rVB2	5443	8916	1.50%	0.174%
5	3.899	875	889	923	rBV	37804	144616	24.37%	2.828%
6	4.342	1009	1027	1051	rBV	99004	248375	41.85%	4.856%
7	5.043	1227	1245	1270	rBV2	236305	593517	100.00%	11.605%
8	5.612	1409	1422	1449	rBV	230292	476639	80.31%	9.320%
9	6.063	1549	1562	1595	rBV	130562	277444	46.75%	5.425%
10	6.982	1837	1848	1877	rBV	66865	129027	21.74%	2.523%
11	7.310	1937	1950	1978	rBV	301722	541900	91.30%	10.596%
12	7.619	2036	2046	2064	rBV2	38050	70889	11.94%	1.386%
13	8.085	2180	2191	2227	rBV	215038	439238	74.01%	8.588%
14	8.844	2415	2427	2455	rBV	334031	563322	94.91%	11.015%
15	10.207	2839	2851	2870	rVB	92640	147175	24.80%	2.878%
16	11.239	3161	3172	3193	rBV	376633	588723	99.19%	11.511%
17	11.612	3277	3288	3308	rBV	286100	454488	76.58%	8.887%
18	12.242	3470	3484	3495	rBV2	4303	8327	1.40%	0.163%
19	14.030	4033	4040	4050	rVB	3814	6277	1.06%	0.123%




Sum of corrected areas: 5114300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029405.D
Acq On : 06 Dec 2022 11:04
Operator : SY/MD
Sample : VV1206WBL07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

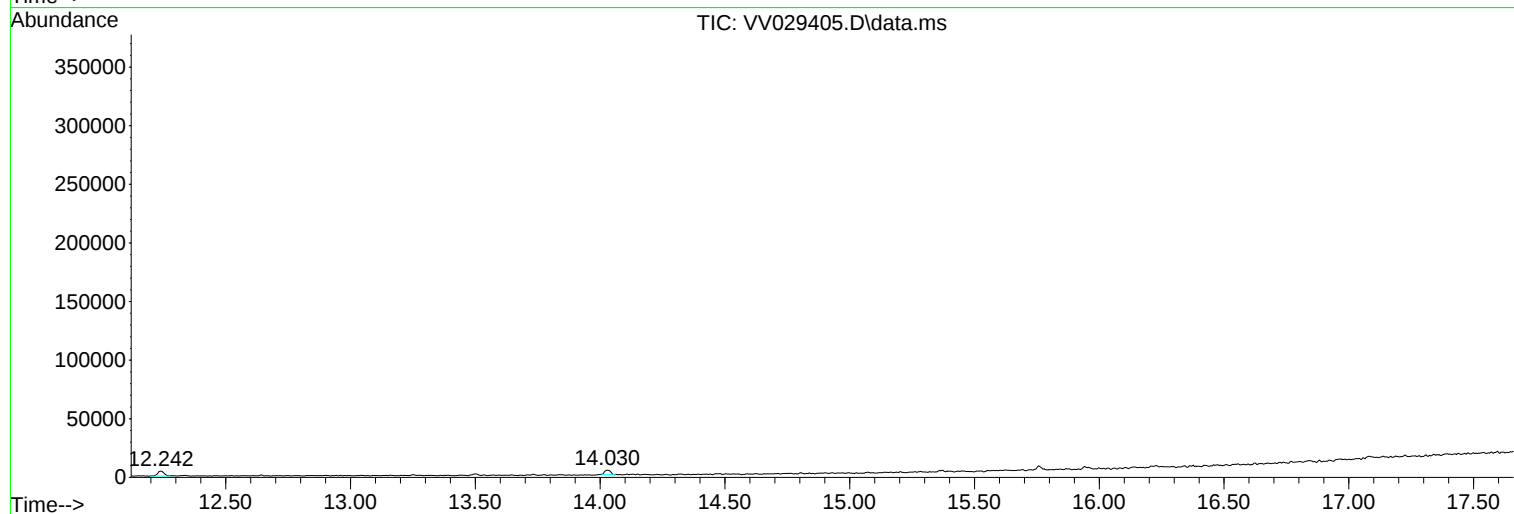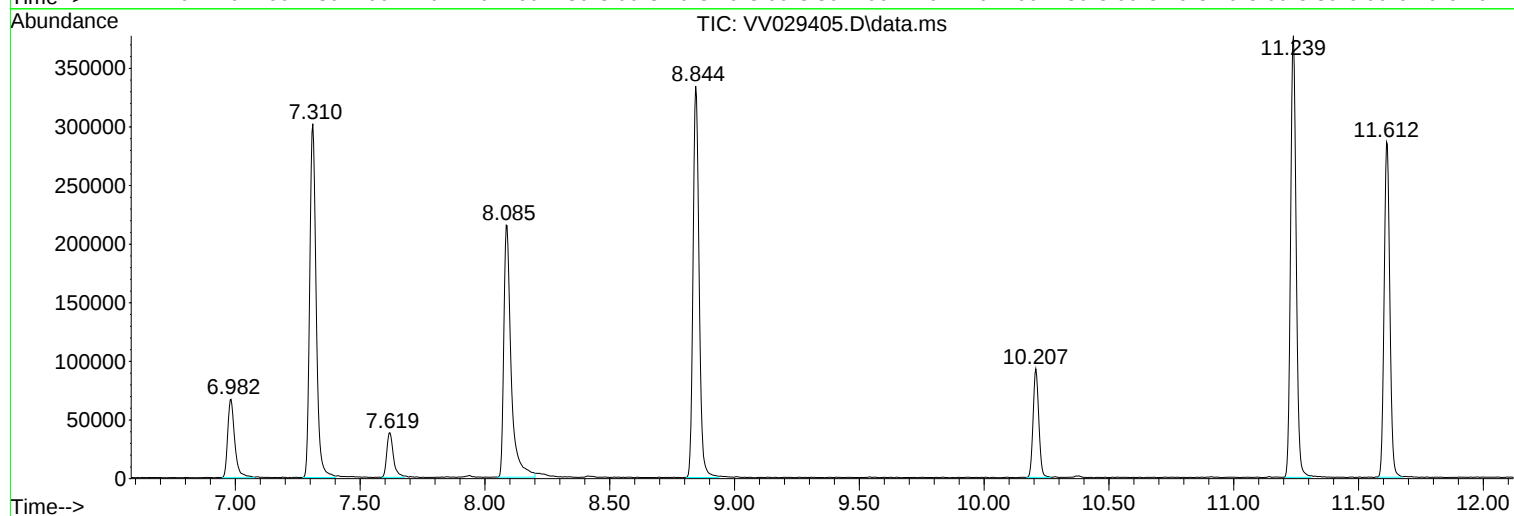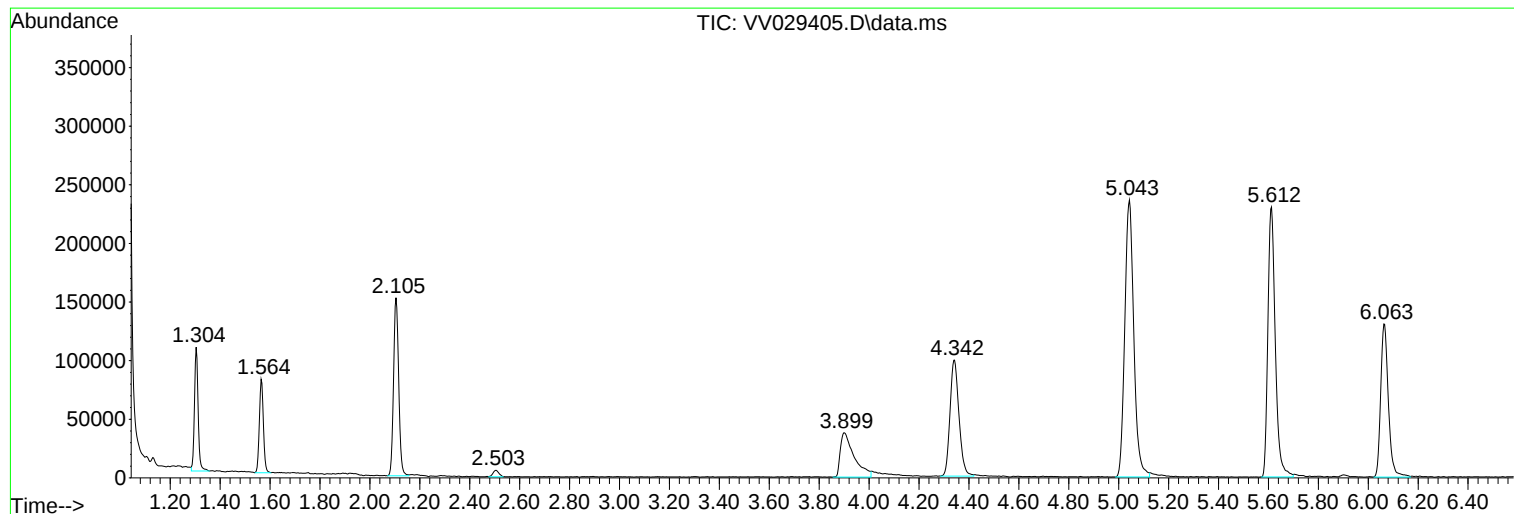

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029405.D
Acq On : 06 Dec 2022 11:04
Operator : SY/MD
Sample : VV1206WBL07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029405.D
Acq On : 06 Dec 2022 11:04
Operator : SY/MD
Sample : VV1206WBL07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK286

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc