


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120622\
Data File : VV029402.D
Acq On : 06 Dec 2022 09:14
Operator : SY/MD
Sample : BFB209
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB209

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Dec 06 21:48:39 2022

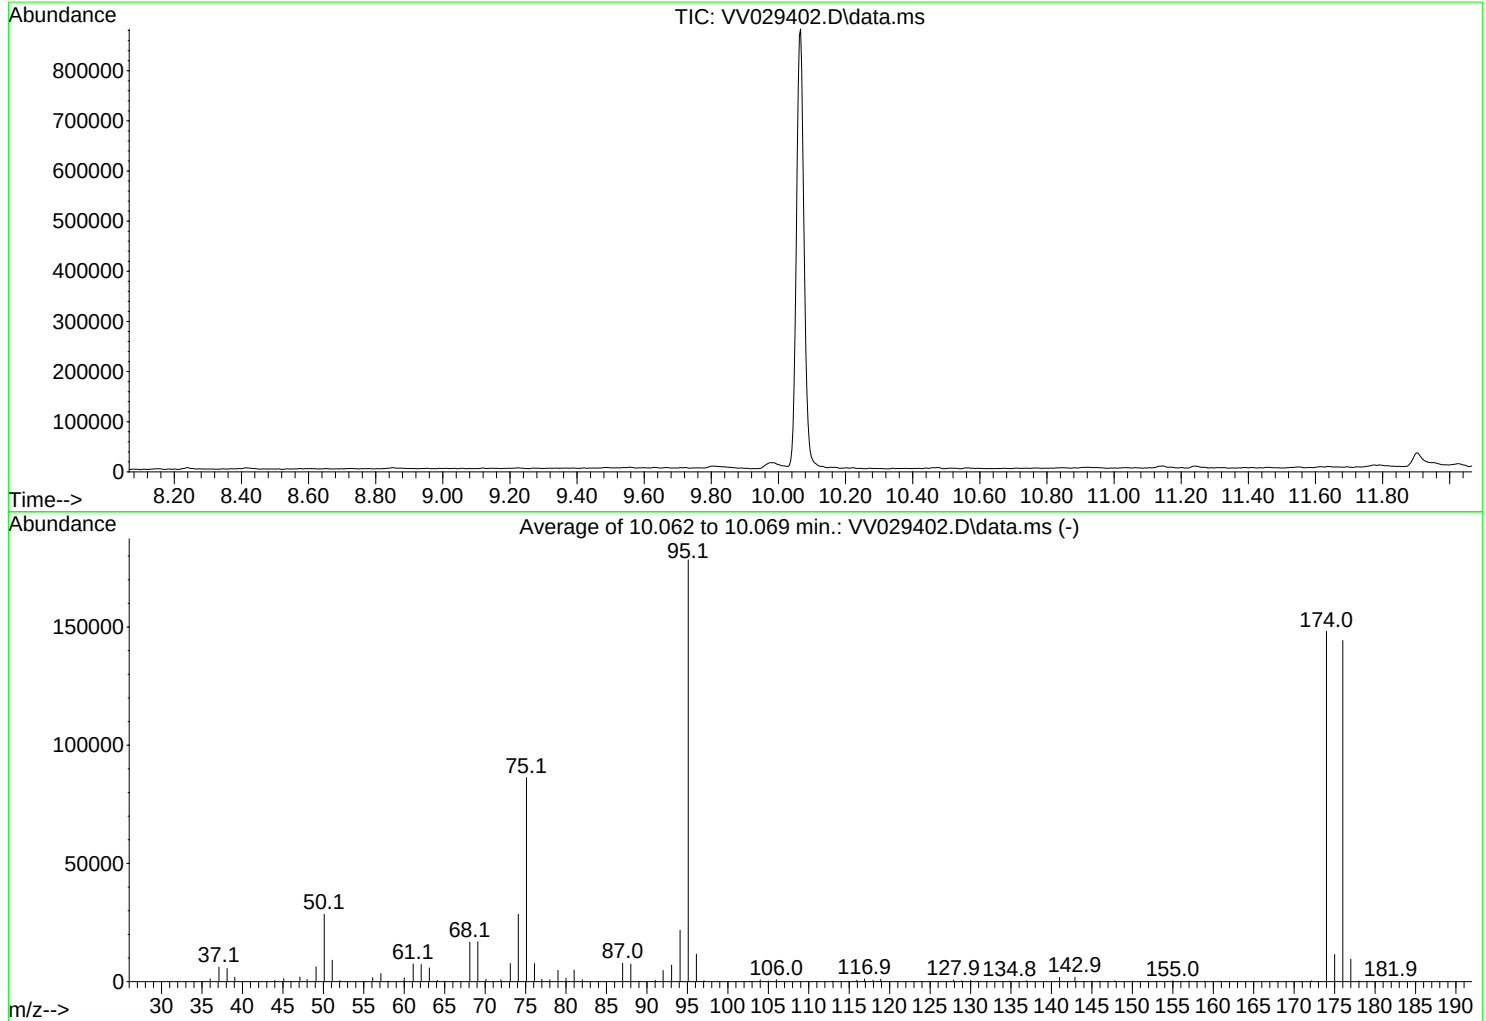

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	28491	PASS
75	95	30	80	48.4	86317	PASS
95	95	100	100	100.0	178410	PASS
96	95	5	9	6.5	11646	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.0	148139	PASS
175	174	5	9	7.8	11487	PASS
176	174	95	105	97.4	144277	PASS
177	176	5	10	6.6	9562	PASS

m/z	Abundance
39.00	408.0
40.00	568.0
41.10	1017.0
42.00	496.0
43.10	816.0
44.10	1169.0
45.10	175.0
53.00	156.0
54.10	146.0
55.10	943.0
56.10	735.0
57.10	848.0
58.00	120.0
67.10	361.0
68.10	258.0
69.10	547.0
70.10	187.0
71.20	269.0
71.90	114.0
77.00	192.0
81.10	252.0
82.10	267.0
83.20	168.0
84.10	635.0
85.00	296.0
91.20	357.0
92.90	160.0
95.20	107.0
100.10	147.0
110.00	117.0
207.00	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1137.0
37.10	6490.0
38.10	5860.0
39.10	2386.0
40.00	691.0
41.00	604.0
42.00	236.0
43.10	756.0
44.00	1669.0
45.10	1424.0
46.10	120.0
47.10	2035.0
48.00	956.0
49.10	6426.0
50.10	29528.0
51.10	9664.0
52.10	510.0
53.10	100.0
54.10	105.0
55.10	1100.0
56.10	2578.0
57.10	4436.0
58.00	337.0
60.00	1617.0
61.10	7635.0
62.10	7433.0
63.10	6187.0
64.10	648.0
65.10	245.0
66.10	112.0
68.10	17576.0
69.10	18056.0
70.10	1465.0
71.10	259.0
72.00	945.0
73.10	7786.0
74.10	29192.0
75.10	89776.0
76.10	7770.0
77.00	1324.0
78.00	880.0
79.00	4982.0
80.00	1461.0
81.00	5247.0
82.00	1192.0
83.10	225.0
84.10	347.0
85.10	190.0
85.90	206.0
87.00	8148.0
88.00	7696.0
91.10	893.0
92.00	4844.0
93.10	7261.0
94.10	22136.0
95.10	184064.0
96.10	12208.0
97.10	405.0
102.80	101.0
104.00	781.0
105.00	381.0
106.00	828.0
107.00	152.0
110.00	152.0
111.00	206.0
111.90	176.0
112.90	193.0
115.00	217.0
116.00	689.0
116.90	1145.0
118.00	586.0
118.90	1033.0
123.80	102.0
127.90	633.0
128.90	391.0
130.00	591.0
130.90	291.0
134.90	380.0
136.90	387.0
140.00	141.0
141.00	1876.0
142.10	192.0
142.90	1933.0
144.00	160.0
145.00	292.0
145.90	255.0
147.00	119.0
147.80	369.0
148.90	113.0
150.00	276.0
151.90	127.0
152.90	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

153.90	114.0
155.00	453.0
157.00	349.0
158.90	264.0
161.00	190.0
170.80	113.0
172.10	391.0
174.00	147776.0
175.00	11643.0
176.00	143616.0
177.00	9815.0
178.00	313.0
182.00	169.0
207.00	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1261.0
37.10	6444.0
38.10	5820.0
39.10	2391.0
40.00	678.0
41.10	542.0
42.00	243.0
43.10	729.0
44.00	1659.0
45.10	1512.0
46.00	136.0
47.10	1995.0
48.00	946.0
49.10	6502.0
50.10	29296.0
51.10	9418.0
52.10	488.0
54.00	126.0
55.10	1040.0
56.10	2458.0
57.10	4405.0
58.00	327.0
60.00	1579.0
61.10	7728.0
62.10	7597.0
63.10	6100.0
64.10	596.0
64.90	252.0
66.20	112.0
67.00	576.0
68.10	17624.0
69.10	17952.0
70.10	1296.0
71.00	256.0
72.00	957.0
73.10	7964.0
74.10	29544.0
75.10	89160.0
76.10	7975.0
77.00	1294.0
78.00	858.0
79.00	4963.0
80.00	1480.0
81.00	5297.0
82.00	1165.0
83.10	230.0
84.10	292.0
85.10	187.0
85.90	245.0
87.00	8059.0
88.00	7684.0
91.00	899.0
92.00	4910.0
93.10	7382.0
94.10	22456.0
95.10	184640.0
96.10	12071.0
97.10	423.0
102.90	111.0
104.00	793.0
105.10	377.0
106.00	877.0
107.10	136.0
110.00	163.0
111.00	166.0
112.00	154.0
112.90	191.0
114.90	235.0
116.00	734.0
116.90	1082.0
117.90	663.0
118.90	1019.0
123.90	111.0
127.90	697.0
128.90	404.0
130.00	555.0
130.90	311.0
134.80	385.0
136.90	403.0
140.00	143.0
141.00	1830.0
142.90	1981.0
144.00	187.0
144.90	268.0
145.90	276.0
147.00	159.0
147.90	414.0
148.90	124.0
150.00	286.0
151.90	113.0
152.90	191.0
153.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

155.00	516.0
157.00	318.0
158.90	266.0
160.90	214.0
172.10	420.0
174.00	153664.0
175.00	11949.0
176.00	149184.0
177.00	9953.0
178.00	280.0
180.00	133.0
182.00	172.0
207.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

m/z	Abundance
36.00	1245.0
37.10	5633.0
38.10	5063.0
39.10	2192.0
40.00	677.0
41.10	577.0
42.00	259.0
43.10	678.0
44.00	1672.0
45.10	1363.0
46.00	141.0
47.10	1883.0
48.00	897.0
49.10	5878.0
50.10	26648.0
51.10	8100.0
52.00	443.0
53.00	116.0
54.00	135.0
55.10	925.0
56.10	2225.0
57.10	3931.0
58.00	242.0
60.00	1449.0
61.10	7110.0
62.10	6780.0
63.10	5288.0
64.10	479.0
64.90	233.0
68.10	15820.0
69.10	16125.0
70.10	1112.0
71.10	286.0
72.00	835.0
73.10	7297.0
74.10	26760.0
75.10	80016.0
76.10	7171.0
77.00	1109.0
78.00	780.0
79.00	4485.0
80.00	1281.0
81.00	4847.0
82.00	997.0
83.00	228.0
84.10	239.0
85.10	239.0
85.90	254.0
87.00	7358.0
88.00	7030.0
91.00	802.0
92.00	4491.0
93.10	6692.0
94.10	20528.0
95.10	166848.0
96.10	10659.0
97.00	368.0
102.80	105.0
104.00	712.0
105.10	318.0
106.00	806.0
107.10	153.0
110.00	158.0
111.00	123.0
112.10	156.0
112.90	157.0
114.90	237.0
115.90	721.0
116.90	949.0
117.90	684.0
118.90	942.0
123.90	114.0
127.90	656.0
128.90	333.0
130.00	518.0
130.90	289.0
134.80	333.0
136.90	350.0
141.00	1604.0
142.90	1752.0
144.00	173.0
144.90	218.0
145.90	272.0
147.00	181.0
147.90	436.0
148.90	144.0
150.00	291.0
152.90	142.0
153.90	143.0
155.00	470.0
157.00	248.0
158.90	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209

160.90	208.0
172.20	424.0
174.00	142976.0
175.00	10870.0
176.00	140032.0
177.00	8918.0
178.00	236.0
180.00	141.0
181.90	126.0
207.10	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB209