

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033113.D
 Acq On : 06 Dec 2023 13:57
 Operator : SY/MD
 Sample : 05644-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033113.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	112894	117151	13.29%	1.555%
2	1.420	112	118	124	rVB	6368	6777	0.77%	0.090%
3	1.474	132	135	137	rBV	1365	714	0.08%	0.009%
4	1.532	146	153	164	rBV	81778	96257	10.92%	1.278%
5	1.603	171	175	181	rVB	1398	1375	0.16%	0.018%
6	1.632	181	184	186	rVV	494	337	0.04%	0.004%
7	1.645	186	188	189	rVV	428	195	0.02%	0.003%
8	1.658	189	192	196	rVB2	1361	957	0.11%	0.013%
9	1.683	196	200	203	rBV3	391	323	0.04%	0.004%
10	1.699	203	205	206	rBV	434	183	0.02%	0.002%
11	1.709	206	208	210	rVB	640	237	0.03%	0.003%
12	1.719	210	211	213	rVB	260	98	0.01%	0.001%
13	1.754	218	222	223	rBV3	984	589	0.07%	0.008%
14	1.773	226	228	232	rVB	966	633	0.07%	0.008%
15	1.796	232	235	236	rBV2	938	564	0.06%	0.007%
16	1.809	237	239	242	rVB2	889	545	0.06%	0.007%
17	1.825	242	244	248	rVB	1147	708	0.08%	0.009%
18	1.854	248	253	258	rBV	1064	811	0.09%	0.011%
19	1.880	258	261	263	rBV2	581	265	0.03%	0.004%
20	1.896	263	266	272	rVB	767	696	0.08%	0.009%
21	1.925	272	275	279	rVB2	1193	820	0.09%	0.011%
22	1.944	279	281	283	rVB	861	382	0.04%	0.005%
23	1.957	283	285	288	rBV	781	517	0.06%	0.007%
24	1.973	288	290	291	rBV3	247	77	0.01%	0.001%
25	1.986	291	294	296	rBV2	568	381	0.04%	0.005%
26	1.998	296	298	301	rVB	741	395	0.04%	0.005%
27	2.063	301	318	333	rBV	170764	252584	28.66%	3.353%
28	2.117	333	335	340	rVB5	1293	847	0.10%	0.011%
29	2.169	340	351	354	rBV	3801	6455	0.73%	0.086%
30	2.188	354	357	359	rBV2	1320	971	0.11%	0.013%
31	2.439	432	435	437	rBV	1715	1314	0.15%	0.017%
32	3.066	627	630	631	rBV	1490	948	0.11%	0.013%
33	3.117	643	646	648	rBV	2013	1351	0.15%	0.018%
34	3.381	726	728	731	rBV3	1128	664	0.08%	0.009%
35	3.400	731	734	737	rBV	1618	1098	0.12%	0.015%
36	3.732	835	837	840	rBV	1126	551	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033113.D
 Acq On : 06 Dec 2023 13:57
 Operator : SY/MD
 Sample : 05644-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	3.783	844	853	879	rBV	55426	146744	16.65%	1.948%
38	4.249	983	998	1021	rBV	148685	377701	42.86%	5.015%
39	4.654	1121	1124	1129	rBV	1408	1623	0.18%	0.022%
40	4.812	1170	1173	1176	rBV	1461	923	0.10%	0.012%
41	4.957	1201	1218	1242	rBV2	330976	881228	100.00%	11.700%
42	5.268	1312	1315	1318	rVB	1509	886	0.10%	0.012%
43	5.362	1342	1344	1346	rBV2	1395	847	0.10%	0.011%
44	5.436	1364	1367	1371	rBV	1541	1128	0.13%	0.015%
45	5.535	1387	1398	1428	rBV	330995	679207	77.08%	9.017%
46	5.838	1480	1492	1519	rVB3	50436	117355	13.32%	1.558%
47	5.989	1528	1539	1561	rBV	186542	381546	43.30%	5.066%
48	6.066	1561	1563	1566	rVB	1408	625	0.07%	0.008%
49	6.915	1816	1827	1845	rBV	108558	203312	23.07%	2.699%
50	7.175	1904	1908	1911	rBV	2452	1972	0.22%	0.026%
51	7.194	1911	1914	1917	rVB2	1437	825	0.09%	0.011%
52	7.243	1918	1929	1951	rBV	410202	723032	82.05%	9.599%
53	7.555	2017	2026	2040	rBV2	78119	138991	15.77%	1.845%
54	8.024	2163	2172	2202	rBV	204728	378359	42.94%	5.023%
55	8.281	2249	2252	2257	rBV2	1381	1150	0.13%	0.015%
56	8.783	2398	2408	2429	rBV	522962	854926	97.02%	11.350%
57	8.966	2460	2465	2468	rBV	1685	1893	0.21%	0.025%
58	9.030	2483	2485	2488	rVB	1942	979	0.11%	0.013%
59	9.175	2527	2530	2535	rBV	2254	2040	0.23%	0.027%
60	9.622	2666	2669	2672	rBV	1229	1121	0.13%	0.015%
61	9.689	2688	2690	2694	rVB	1839	1304	0.15%	0.017%
62	9.815	2726	2729	2733	rBV2	1404	1404	0.16%	0.019%
63	9.866	2742	2745	2746	rBV	1377	694	0.08%	0.009%
64	10.152	2823	2834	2852	rBV	286161	449176	50.97%	5.963%
65	10.374	2900	2903	2906	rVB	1343	812	0.09%	0.011%
66	10.394	2907	2909	2912	rBV	1227	836	0.09%	0.011%
67	10.445	2922	2925	2927	rBV	1274	886	0.10%	0.012%
68	10.693	2999	3002	3004	rBV	1261	670	0.08%	0.009%
69	10.857	3049	3053	3059	rBV	1384	1592	0.18%	0.021%
70	10.886	3059	3062	3063	rBV	1327	824	0.09%	0.011%
71	11.095	3124	3127	3130	rBV	1179	858	0.10%	0.011%
72	11.185	3145	3155	3181	rBV	557387	871626	98.91%	11.572%
73	11.381	3213	3216	3218	rBV3	1196	906	0.10%	0.012%
74	11.561	3261	3272	3296	rBV	497284	774297	87.87%	10.280%
75	11.895	3373	3376	3382	rBV	1656	1390	0.16%	0.018%
76	12.262	3488	3490	3494	rVB	2739	1757	0.20%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033113.D
 Acq On : 06 Dec 2023 13:57
 Operator : SY/MD
 Sample : 05644-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.284	3494	3497	3499	rBV2	1094	900	0.10%	0.012%
78	12.744	3637	3640	3647	rBV	1720	1980	0.22%	0.026%
79	12.831	3664	3667	3669	rBV	1509	859	0.10%	0.011%
80	13.680	3928	3931	3937	rBV5	1551	1580	0.18%	0.021%
81	13.770	3957	3959	3964	rVB2	1769	1462	0.17%	0.019%
82	13.799	3965	3968	3971	rBV	1601	1074	0.12%	0.014%
83	13.853	3983	3985	3987	rBV	1378	799	0.09%	0.011%
84	13.988	4024	4027	4029	rBV3	1396	1053	0.12%	0.014%
85	14.056	4044	4048	4051	rBV	2172	1974	0.22%	0.026%
86	14.156	4075	4079	4089	rVB	1940	2929	0.33%	0.039%
87	14.348	4136	4139	4140	rBV	1605	900	0.10%	0.012%
88	14.667	4234	4238	4240	rBV	1375	1302	0.15%	0.017%
89	14.766	4264	4269	4273	rBV2	1632	2083	0.24%	0.028%
90	14.844	4290	4293	4297	rVB	1758	1333	0.15%	0.018%
91	15.458	4482	4484	4486	rBV3	1569	832	0.09%	0.011%
92	15.512	4498	4501	4505	rBV	1576	966	0.11%	0.013%
93	15.757	4574	4577	4580	rBV	2021	1340	0.15%	0.018%
94	16.905	4931	4934	4938	rBV3	3000	2578	0.29%	0.034%




Sum of corrected areas: 7532159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033113.D
Acq On : 06 Dec 2023 13:57
Operator : SY/MD
Sample : 05644-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

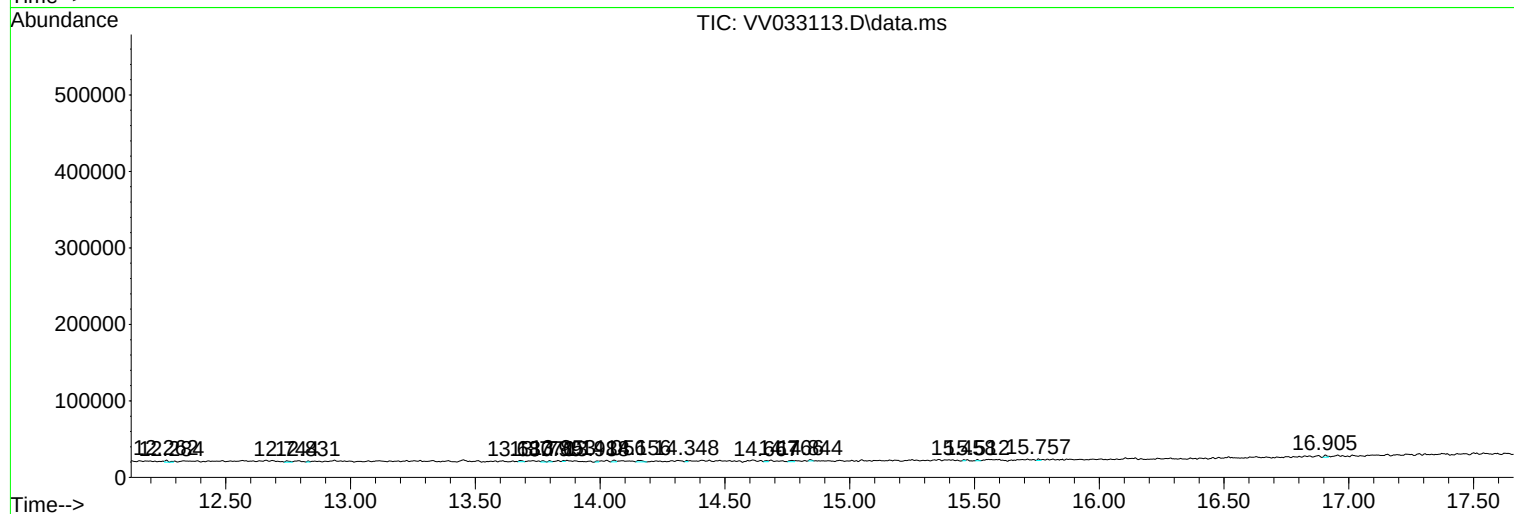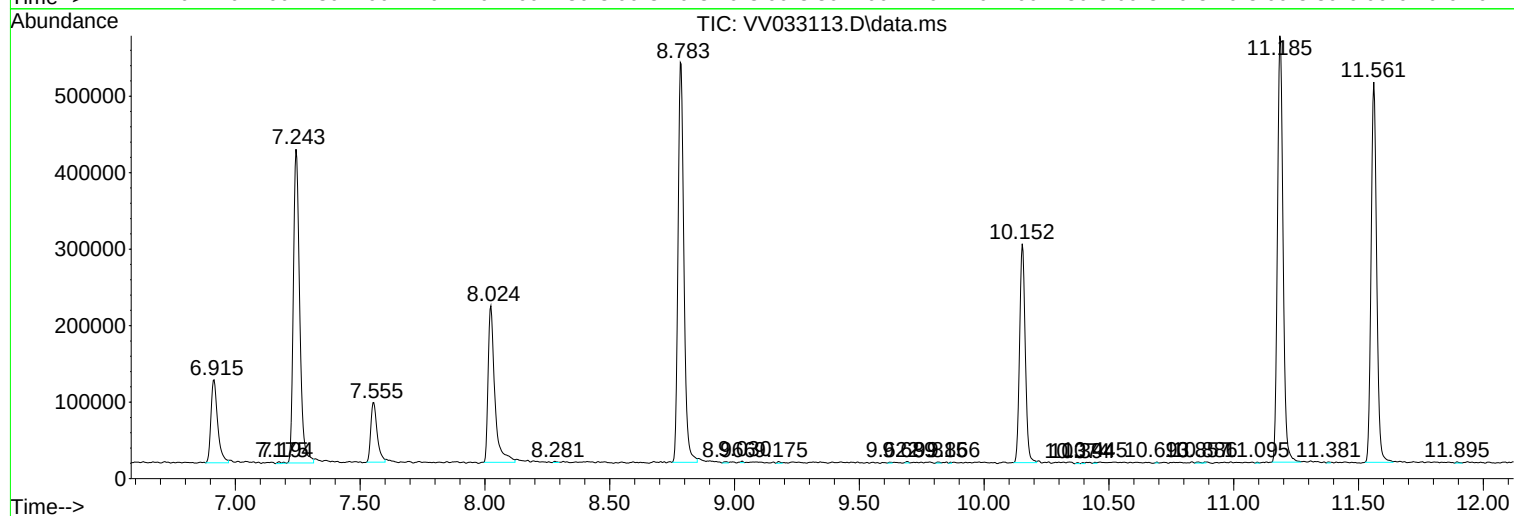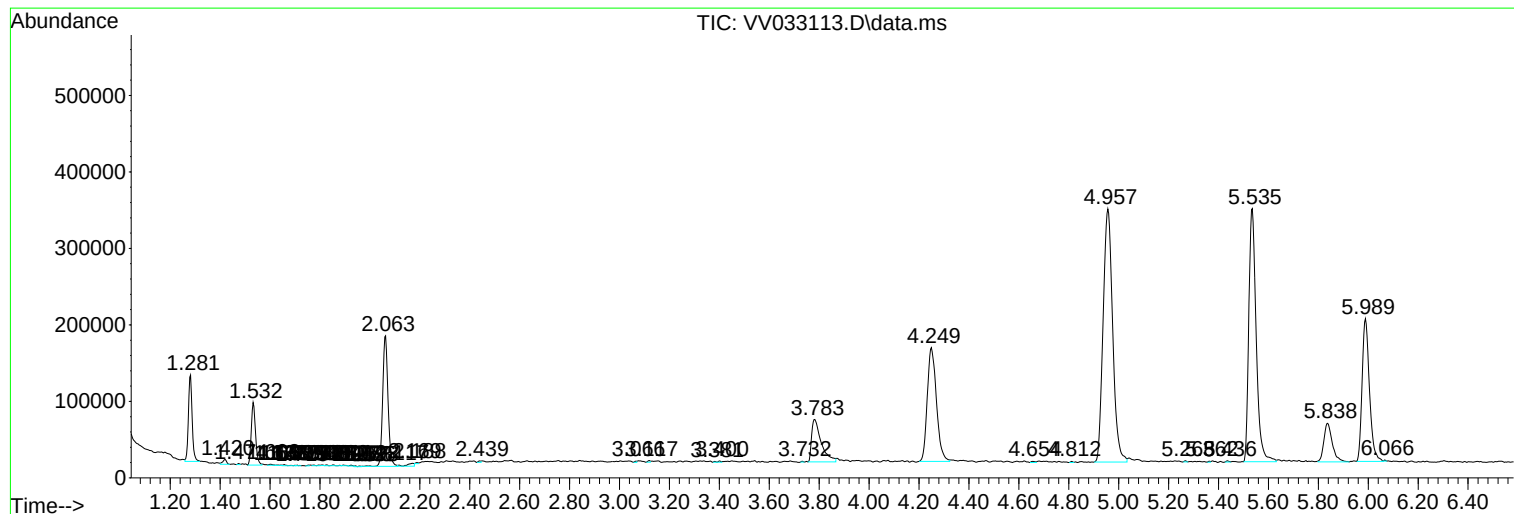

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033113.D
Acq On : 06 Dec 2023 13:57
Operator : SY/MD
Sample : 05644-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033113.D
Acq On : 06 Dec 2023 13:57
Operator : SY/MD
Sample : 05644-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc