

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033114.D
 Acq On : 06 Dec 2023 14:20
 Operator : SY/MD
 Sample : 05644-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	109449	119947	13.67%	1.619%
2	1.384	105	107	110	rBV3	916	617	0.07%	0.008%
3	1.423	111	119	124	rVB2	6486	8506	0.97%	0.115%
4	1.487	136	139	142	rVB2	1791	1285	0.15%	0.017%
5	1.503	142	144	145	rBV	741	329	0.04%	0.004%
6	1.536	145	154	165	rVB	79061	95370	10.87%	1.287%
7	1.645	181	188	192	rVB2	1703	2004	0.23%	0.027%
8	1.674	192	197	199	rBV4	1091	980	0.11%	0.013%
9	1.703	204	206	208	rVB3	779	315	0.04%	0.004%
10	1.728	208	214	217	rBV2	1329	1437	0.16%	0.019%
11	1.748	218	220	223	rVB2	1427	806	0.09%	0.011%
12	1.777	223	229	232	rBV3	1212	1104	0.13%	0.015%
13	1.793	232	234	236	rVB2	567	236	0.03%	0.003%
14	1.815	236	241	244	rBV	1092	1160	0.13%	0.016%
15	1.831	244	246	250	rVB	778	383	0.04%	0.005%
16	1.854	250	253	256	rVB2	459	250	0.03%	0.003%
17	1.870	256	258	259	rBV2	269	104	0.01%	0.001%
18	1.880	259	261	266	rVB	1028	782	0.09%	0.011%
19	1.909	266	270	272	rBV2	874	821	0.09%	0.011%
20	1.928	274	276	279	rVB	1566	831	0.09%	0.011%
21	1.947	279	282	287	rVB2	874	769	0.09%	0.010%
22	1.982	287	293	296	rBV3	1311	1365	0.16%	0.018%
23	2.002	296	299	303	rBV2	730	568	0.06%	0.008%
24	2.018	303	304	307	rBV2	568	251	0.03%	0.003%
25	2.063	307	318	330	rBV	166991	246058	28.04%	3.320%
26	2.153	340	346	350	rBV	2970	3526	0.40%	0.048%
27	2.188	350	357	359	rVV	2953	3306	0.38%	0.045%
28	2.217	359	366	379	rVV2	9844	20095	2.29%	0.271%
29	2.436	431	434	435	rBV	1265	763	0.09%	0.010%
30	2.619	489	491	494	rBV	1372	829	0.09%	0.011%
31	2.748	529	531	534	rVB	1504	808	0.09%	0.011%
32	2.892	572	576	578	rBV3	1645	1361	0.16%	0.018%
33	3.474	754	757	762	rVB	1780	1569	0.18%	0.021%
34	3.783	844	853	881	rBV	58180	159204	18.14%	2.148%
35	4.043	931	934	937	rBV	1893	1359	0.15%	0.018%
36	4.249	982	998	1025	rBV3	146615	379504	43.24%	5.121%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033114.D
 Acq On : 06 Dec 2023 14:20
 Operator : SY/MD
 Sample : 05644-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.426	1050	1053	1054	rBV2	1430	924	0.11%	0.012%
38	4.584	1099	1102	1106	rBV2	1576	1245	0.14%	0.017%
39	4.693	1132	1136	1141	rBV	1870	2321	0.26%	0.031%
40	4.957	1202	1218	1238	rBV2	327683	865375	98.61%	11.677%
41	5.477	1378	1380	1384	rBV2	1377	1111	0.13%	0.015%
42	5.535	1386	1398	1427	rVV	332063	687527	78.34%	9.278%
43	5.838	1483	1492	1510	rVB7	11067	26828	3.06%	0.362%
44	5.989	1527	1539	1558	rBV2	182910	378807	43.16%	5.112%
45	6.188	1598	1601	1604	rBV2	1945	1188	0.14%	0.016%
46	6.301	1634	1636	1640	rBV	1706	1007	0.11%	0.014%
47	6.516	1701	1703	1709	rBV	1292	1130	0.13%	0.015%
48	6.648	1742	1744	1747	rBV	1399	988	0.11%	0.013%
49	6.690	1754	1757	1760	rVB	1889	1123	0.13%	0.015%
50	6.722	1764	1767	1770	rBV	1529	1044	0.12%	0.014%
51	6.915	1816	1827	1849	rBV	107356	208231	23.73%	2.810%
52	7.108	1884	1887	1893	rVB	1718	1343	0.15%	0.018%
53	7.243	1919	1929	1953	rBV	394289	701998	79.99%	9.473%
54	7.555	2017	2026	2047	rBV	81040	140445	16.00%	1.895%
55	7.776	2092	2095	2100	rVB	2027	1727	0.20%	0.023%
56	7.802	2100	2103	2111	rBV	1400	1779	0.20%	0.024%
57	7.838	2111	2114	2118	rVV	1637	1233	0.14%	0.017%
58	8.024	2164	2172	2201	rBV	192713	367168	41.84%	4.955%
59	8.690	2376	2379	2382	rBV	1841	1231	0.14%	0.017%
60	8.786	2398	2409	2434	rBV	519486	858796	97.86%	11.589%
61	9.217	2539	2543	2544	rBV	1687	1228	0.14%	0.017%
62	9.783	2716	2719	2725	rBV	1713	1987	0.23%	0.027%
63	10.153	2824	2834	2854	rVB	282349	436880	49.78%	5.895%
64	10.918	3070	3072	3074	rBV	1213	544	0.06%	0.007%
65	10.950	3079	3082	3086	rVB	2839	1874	0.21%	0.025%
66	11.030	3104	3107	3115	rBV	1442	1882	0.21%	0.025%
67	11.185	3144	3155	3172	rBV	568512	877588	100.00%	11.842%
68	11.561	3261	3272	3286	rBV	491653	758128	86.39%	10.230%
69	12.339	3511	3514	3515	rBV	1636	846	0.10%	0.011%
70	12.638	3602	3607	3611	rVB	2337	2009	0.23%	0.027%
71	13.059	3736	3738	3741	rVB	1857	990	0.11%	0.013%
72	13.445	3855	3858	3860	rBV	1561	1191	0.14%	0.016%
73	13.677	3928	3930	3940	rVB	2256	2636	0.30%	0.036%
74	13.718	3940	3943	3949	rBV3	1242	1524	0.17%	0.021%
75	13.783	3959	3963	3968	rBV3	1710	2090	0.24%	0.028%
76	13.805	3968	3970	3973	rVB	1273	695	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033114.D
Acq On : 06 Dec 2023 14:20
Operator : SY/MD
Sample : 05644-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

77	13.889	3993	3996	3997	rBV	1496	983	0.11%	0.013%
78	14.297	4121	4123	4127	rBV	1153	781	0.09%	0.011%
79	14.757	4264	4266	4269	rBV	1229	631	0.07%	0.009%
80	14.898	4308	4310	4311	rBV	1029	444	0.05%	0.006%
81	15.014	4344	4346	4349	rVB	1602	878	0.10%	0.012%
82	15.673	4549	4551	4554	rBV	1890	937	0.11%	0.013%
83	15.924	4627	4629	4632	rBV3	1501	739	0.08%	0.010%




Sum of corrected areas: 7410656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033114.D
Acq On : 06 Dec 2023 14:20
Operator : SY/MD
Sample : 05644-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

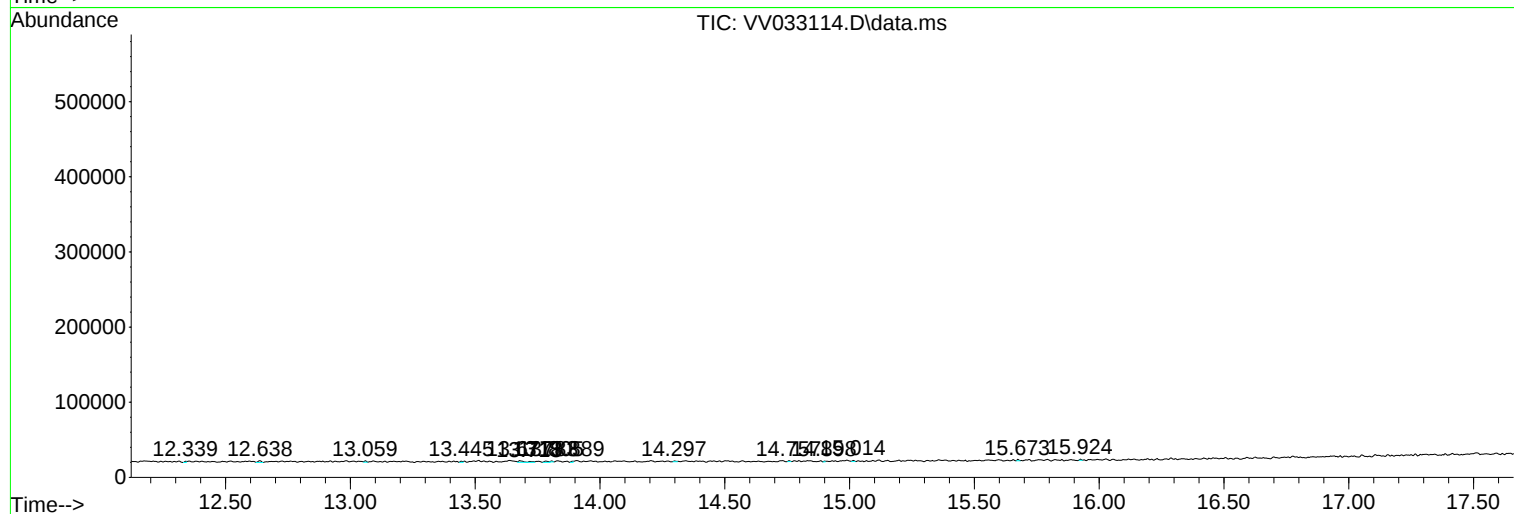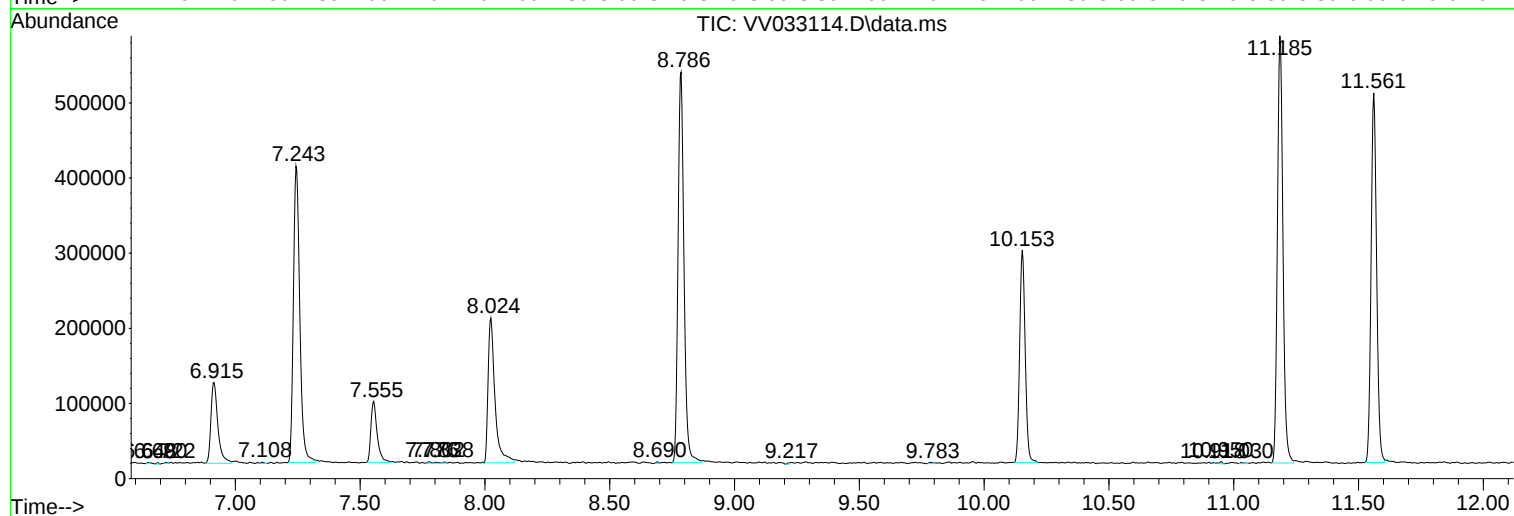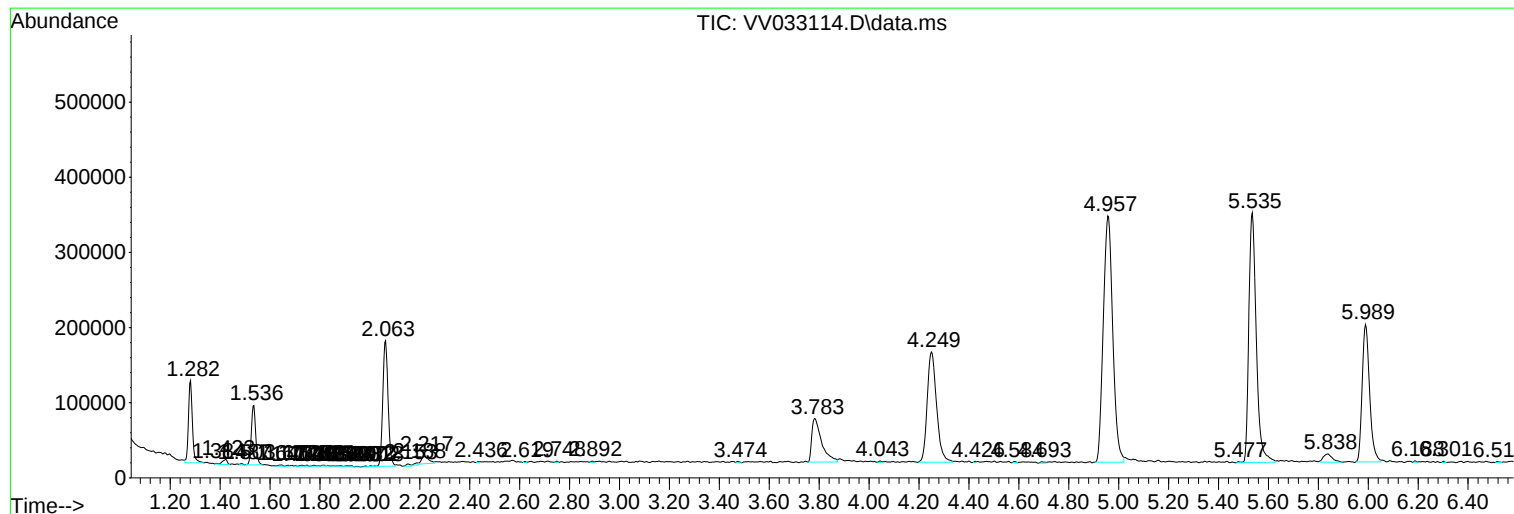

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033114.D
Acq On : 06 Dec 2023 14:20
Operator : SY/MD
Sample : 05644-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033114.D
Acq On : 06 Dec 2023 14:20
Operator : SY/MD
Sample : 05644-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc