

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033115.D
 Acq On : 06 Dec 2023 14:44
 Operator : SY/MD
 Sample : 05644-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	112871	124142	13.78%	1.627%
2	1.416	113	117	127	rVB2	6231	7211	0.80%	0.094%
3	1.532	145	153	164	rBV	82483	101813	11.30%	1.334%
4	1.609	174	177	178	rBV	465	196	0.02%	0.003%
5	1.625	178	182	187	rVB2	1231	1270	0.14%	0.017%
6	1.651	187	190	193	rVB	1390	725	0.08%	0.010%
7	1.683	194	200	204	rVB2	1820	1872	0.21%	0.025%
8	1.706	204	207	208	rBV	487	281	0.03%	0.004%
9	1.722	208	212	215	rBV2	1547	1308	0.15%	0.017%
10	1.738	215	217	219	rVB	1329	610	0.07%	0.008%
11	1.760	219	224	230	rVB2	1470	1583	0.18%	0.021%
12	1.809	236	239	242	rBV2	1354	863	0.10%	0.011%
13	1.825	242	244	247	rVB2	551	325	0.04%	0.004%
14	1.838	247	248	250	rBV2	529	257	0.03%	0.003%
15	1.857	250	254	257	rVB3	775	631	0.07%	0.008%
16	1.873	257	259	262	rVB2	791	390	0.04%	0.005%
17	1.889	262	264	266	rBV2	739	498	0.06%	0.007%
18	1.902	266	268	271	rVB	788	445	0.05%	0.006%
19	1.928	275	276	279	rVB	1238	584	0.06%	0.008%
20	1.947	279	282	285	rBV2	948	601	0.07%	0.008%
21	1.969	285	289	296	rVB2	1025	1069	0.12%	0.014%
22	2.011	299	302	307	rVB2	925	506	0.06%	0.007%
23	2.063	307	318	331	rBV	170615	253849	28.18%	3.326%
24	2.150	338	345	346	rBV2	1502	1024	0.11%	0.013%
25	2.169	346	351	354	rVV	2051	2190	0.24%	0.029%
26	2.223	355	368	380	rVV3	10484	24115	2.68%	0.316%
27	2.285	385	387	391	rVV	1166	961	0.11%	0.013%
28	2.371	410	414	418	rBV	1824	1551	0.17%	0.020%
29	2.394	418	421	424	rVB	1740	1058	0.12%	0.014%
30	2.719	520	522	526	rVB	1965	1281	0.14%	0.017%
31	2.741	526	529	533	rBV	1935	1743	0.19%	0.023%
32	3.500	763	765	768	rBV	1231	813	0.09%	0.011%
33	3.783	844	853	875	rBV	60421	161217	17.90%	2.113%
34	4.146	964	966	970	rVB	2023	1125	0.12%	0.015%
35	4.249	984	998	1022	rBV	153979	392641	43.59%	5.145%
36	4.481	1067	1070	1073	rBV	1437	1089	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033115.D
 Acq On : 06 Dec 2023 14:44
 Operator : SY/MD
 Sample : 05644-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.603	1105	1108	1111	rBV3	1016	783	0.09%	0.010%
38	4.719	1141	1144	1146	rBV2	1203	871	0.10%	0.011%
39	4.956	1202	1218	1242	rBV2	335598	900835	100.00%	11.805%
40	5.252	1307	1310	1313	rBV	1779	1223	0.14%	0.016%
41	5.365	1341	1345	1350	rBV	1717	1733	0.19%	0.023%
42	5.535	1386	1398	1422	rBV	334955	687753	76.35%	9.012%
43	5.738	1458	1461	1464	rBV3	1337	1145	0.13%	0.015%
44	5.831	1481	1490	1505	rVB10	10837	23693	2.63%	0.310%
45	5.989	1526	1539	1566	rBV	191427	401597	44.58%	5.263%
46	6.114	1575	1578	1580	rBV2	1846	1071	0.12%	0.014%
47	6.481	1690	1692	1695	rBV2	1072	595	0.07%	0.008%
48	6.590	1724	1726	1730	rBV	1326	827	0.09%	0.011%
49	6.760	1774	1779	1781	rBV2	2290	2022	0.22%	0.026%
50	6.911	1815	1826	1843	rBV	111103	212858	23.63%	2.789%
51	7.175	1904	1908	1910	rBV3	1780	1328	0.15%	0.017%
52	7.243	1919	1929	1949	rBV	414780	717953	79.70%	9.408%
53	7.554	2015	2026	2044	rBV2	81987	146289	16.24%	1.917%
54	7.805	2101	2104	2107	rBV	1663	1077	0.12%	0.014%
55	7.905	2130	2135	2140	rVB2	2113	2575	0.29%	0.034%
56	7.934	2141	2144	2147	rVV	1508	998	0.11%	0.013%
57	7.972	2153	2156	2159	rBV	1197	770	0.09%	0.010%
58	8.024	2163	2172	2200	rBV	205500	384923	42.73%	5.044%
59	8.352	2272	2274	2277	rBV	1260	804	0.09%	0.011%
60	8.786	2398	2409	2432	rBV	531093	871885	96.79%	11.425%
61	9.136	2515	2518	2520	rBV2	1140	770	0.09%	0.010%
62	9.255	2553	2555	2558	rBV	1273	651	0.07%	0.009%
63	9.513	2631	2635	2637	rBV	2080	1635	0.18%	0.021%
64	9.577	2652	2655	2658	rBV	1856	1465	0.16%	0.019%
65	9.982	2778	2781	2783	rBV	1587	1255	0.14%	0.016%
66	10.152	2823	2834	2852	rBV	287297	458430	50.89%	6.007%
67	10.371	2899	2902	2903	rBV	1138	708	0.08%	0.009%
68	10.599	2969	2973	2976	rBV	2044	1457	0.16%	0.019%
69	10.644	2984	2987	2990	rVB	2120	1494	0.17%	0.020%
70	10.763	3020	3024	3027	rBV	2056	2071	0.23%	0.027%
71	10.898	3063	3066	3069	rBV	1244	849	0.09%	0.011%
72	11.185	3145	3155	3179	rBV	570531	883268	98.05%	11.575%
73	11.368	3210	3212	3215	rBV	1431	774	0.09%	0.010%
74	11.403	3219	3223	3226	rBV	1902	1758	0.20%	0.023%
75	11.451	3235	3238	3240	rBV	1463	896	0.10%	0.012%
76	11.561	3261	3272	3287	rBV	498414	789418	87.63%	10.345%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033115.D
 Acq On : 06 Dec 2023 14:44
 Operator : SY/MD
 Sample : 05644-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.873	3366	3369	3373	rBV	1529	1359	0.15%	0.018%
78	11.976	3399	3401	3405	rBV	1474	848	0.09%	0.011%
79	12.303	3501	3503	3509	rBV3	1397	1685	0.19%	0.022%
80	12.348	3513	3517	3520	rBV	1520	1254	0.14%	0.016%
81	12.538	3573	3576	3581	rVB	1951	1451	0.16%	0.019%
82	12.828	3664	3666	3669	rBV	1369	807	0.09%	0.011%
83	12.940	3698	3701	3706	rBV2	1410	1107	0.12%	0.015%
84	13.136	3759	3762	3767	rVB	1754	1366	0.15%	0.018%
85	13.165	3767	3771	3772	rBV2	1156	901	0.10%	0.012%
86	13.284	3806	3808	3809	rBV2	1431	673	0.07%	0.009%
87	13.316	3816	3818	3821	rBV	1680	1070	0.12%	0.014%
88	13.458	3859	3862	3866	rVB2	2480	1743	0.19%	0.023%
89	13.599	3904	3906	3908	rBV2	1154	684	0.08%	0.009%
90	13.644	3917	3920	3922	rBV2	1229	920	0.10%	0.012%
91	13.828	3974	3977	3981	rVB	2221	1527	0.17%	0.020%
92	13.853	3982	3985	3988	rBV	1806	1245	0.14%	0.016%
93	13.898	3997	3999	4001	rBV	1160	633	0.07%	0.008%
94	14.258	4108	4111	4113	rBV	1736	1173	0.13%	0.015%
95	14.554	4200	4203	4205	rBV2	1333	991	0.11%	0.013%
96	14.998	4339	4341	4344	rBV	1452	766	0.09%	0.010%
97	15.043	4352	4355	4358	rVB	1661	1021	0.11%	0.013%
98	15.345	4446	4449	4451	rBV2	1468	985	0.11%	0.013%
99	16.075	4673	4676	4678	rBV2	1876	1156	0.13%	0.015%
100	16.413	4779	4781	4785	rVB2	2041	1406	0.16%	0.018%




Sum of corrected areas: 7631115

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033115.D
Acq On : 06 Dec 2023 14:44
Operator : SY/MD
Sample : 05644-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

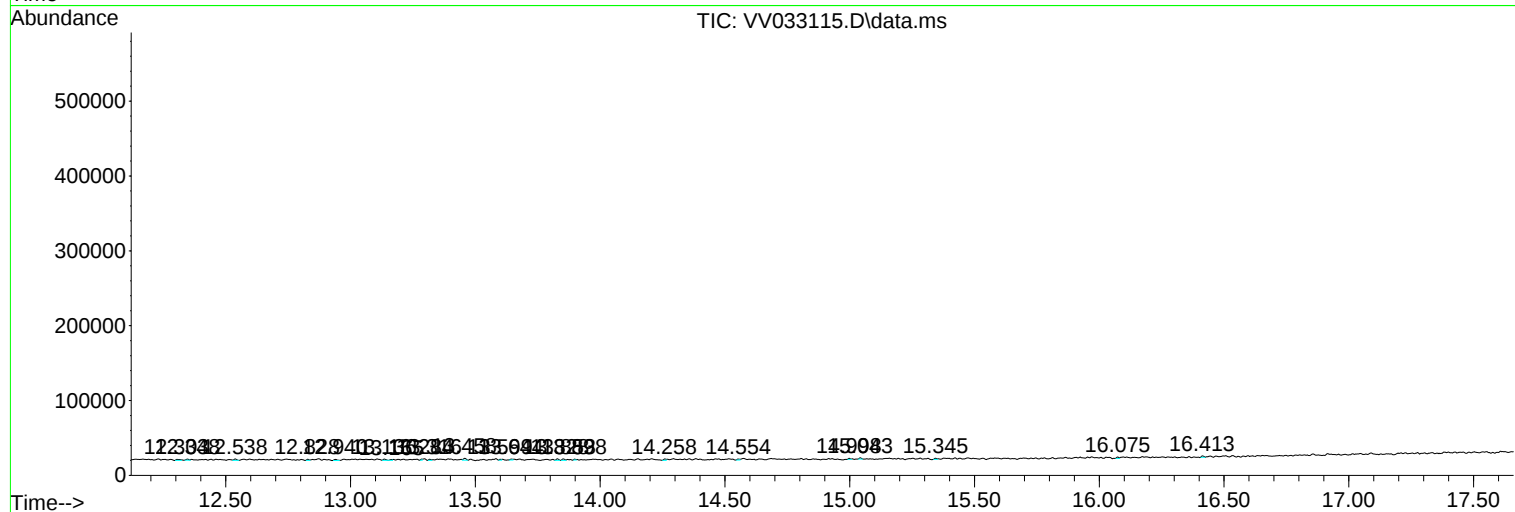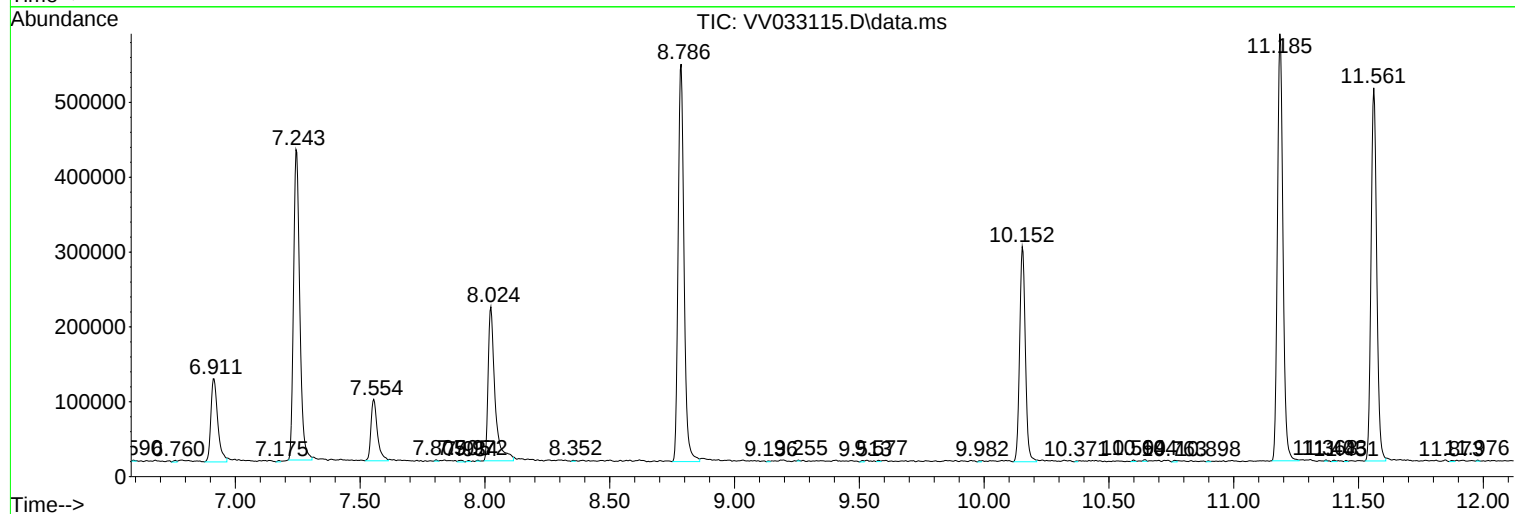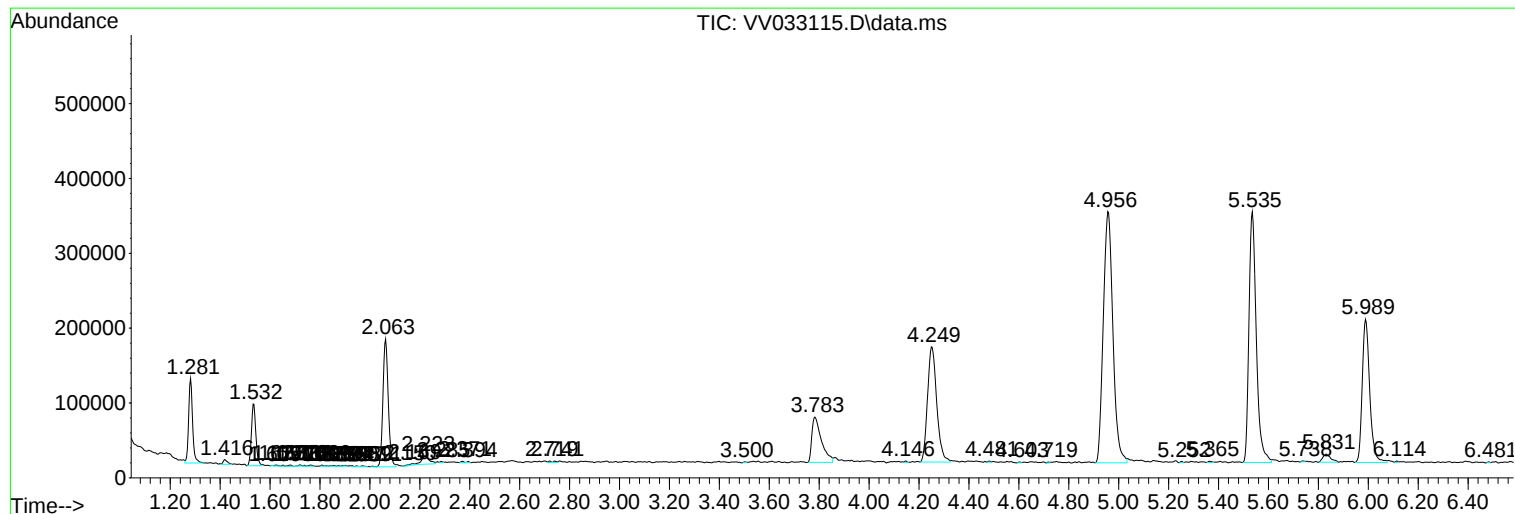

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033115.D
Acq On : 06 Dec 2023 14:44
Operator : SY/MD
Sample : 05644-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033115.D
Acq On : 06 Dec 2023 14:44
Operator : SY/MD
Sample : 05644-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc