

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033117.D
 Acq On : 06 Dec 2023 15:30
 Operator : SY/MD
 Sample : 05644-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	84	rVB	104424	106903	11.27%	1.296%
2	1.420	114	118	126	rVB	6289	7108	0.75%	0.086%
3	1.500	140	143	145	rBV2	982	552	0.06%	0.007%
4	1.532	145	153	167	rVB	81586	97091	10.23%	1.177%
5	1.600	171	174	179	rVB3	957	811	0.09%	0.010%
6	1.629	179	183	186	rBV2	627	512	0.05%	0.006%
7	1.654	186	191	193	rBV3	777	688	0.07%	0.008%
8	1.683	198	200	202	rBV2	903	511	0.05%	0.006%
9	1.709	205	208	212	rVB2	901	461	0.05%	0.006%
10	1.725	212	213	216	rBV2	431	197	0.02%	0.002%
11	1.741	216	218	220	rVB	495	188	0.02%	0.002%
12	1.754	220	222	223	rBV	318	116	0.01%	0.001%
13	1.770	223	227	231	rBV2	1104	798	0.08%	0.010%
14	1.786	231	232	235	rVB2	679	258	0.03%	0.003%
15	1.831	241	246	249	rBV4	1150	799	0.08%	0.010%
16	1.850	249	252	257	rBV2	1088	933	0.10%	0.011%
17	1.883	259	262	268	rVB	837	640	0.07%	0.008%
18	1.912	268	271	281	rVB4	1462	1645	0.17%	0.020%
19	1.950	281	283	286	rVB2	1095	551	0.06%	0.007%
20	1.986	286	294	297	rVB2	1375	1329	0.14%	0.016%
21	2.011	297	302	303	rBV	934	857	0.09%	0.010%
22	2.059	303	317	335	rBV2	173453	270610	28.52%	3.281%
23	2.150	341	345	348	rBV	2251	2150	0.23%	0.026%
24	2.178	348	354	356	rVV	1920	2101	0.22%	0.025%
25	2.201	357	361	363	rVV2	1841	1627	0.17%	0.020%
26	2.220	363	367	373	rVV3	2617	4080	0.43%	0.049%
27	2.590	479	482	484	rBV2	1246	759	0.08%	0.009%
28	2.703	514	517	519	rBV2	1281	901	0.09%	0.011%
29	3.104	640	642	645	rBV	1205	755	0.08%	0.009%
30	3.722	832	834	837	rVB	1766	1001	0.11%	0.012%
31	3.780	844	852	891	rBV3	57735	209012	22.03%	2.534%
32	4.249	984	998	1024	rBV3	145411	370938	39.10%	4.497%
33	4.371	1033	1036	1038	rBV	1919	1324	0.14%	0.016%
34	4.510	1071	1079	1080	rBV4	9772	9989	1.05%	0.121%
35	4.956	1201	1218	1243	rBV3	327526	873796	92.11%	10.594%
36	5.400	1353	1356	1360	rBV	1162	1256	0.13%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033117.D
 Acq On : 06 Dec 2023 15:30
 Operator : SY/MD
 Sample : 05644-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1426	rBV	310212	645703	68.06%	7.828%
38	5.718	1452	1455	1458	rBV	2711	2052	0.22%	0.025%
39	5.831	1478	1490	1512	rBV	474408	948681	100.00%	11.502%
40	5.989	1526	1539	1558	rBV	183633	380695	40.13%	4.615%
41	6.210	1606	1608	1613	rBV4	1163	857	0.09%	0.010%
42	6.400	1664	1667	1672	rBV	1632	1360	0.14%	0.016%
43	6.452	1680	1683	1685	rBV2	1357	918	0.10%	0.011%
44	6.915	1816	1827	1843	rBV	105361	196304	20.69%	2.380%
45	7.243	1919	1929	1955	rBV	396362	702638	74.06%	8.519%
46	7.554	2017	2026	2042	rBV	77521	133230	14.04%	1.615%
47	7.770	2089	2093	2095	rBV	1392	1252	0.13%	0.015%
48	7.799	2100	2102	2106	rVB	1995	1329	0.14%	0.016%
49	8.024	2163	2172	2201	rBV	201196	378925	39.94%	4.594%
50	8.313	2259	2262	2266	rBV	1880	1531	0.16%	0.019%
51	8.342	2269	2271	2275	rVB	1661	1155	0.12%	0.014%
52	8.554	2334	2337	2341	rBV	1518	965	0.10%	0.012%
53	8.786	2398	2409	2437	rBV	498547	824643	86.93%	9.998%
54	9.275	2558	2561	2567	rVB	1247	1432	0.15%	0.017%
55	9.931	2762	2765	2770	rVB	2244	1717	0.18%	0.021%
56	10.152	2823	2834	2861	rVB	279348	443554	46.75%	5.378%
57	10.316	2881	2885	2890	rBV3	2471	3114	0.33%	0.038%
58	10.635	2982	2984	2987	rVB	1458	755	0.08%	0.009%
59	10.757	3019	3022	3025	rVB	1354	752	0.08%	0.009%
60	10.882	3057	3061	3066	rBV	2244	2382	0.25%	0.029%
61	11.088	3122	3125	3130	rBV	1750	1826	0.19%	0.022%
62	11.185	3145	3155	3181	rBV	538201	831477	87.65%	10.081%
63	11.561	3261	3272	3292	rBV	484763	751838	79.25%	9.115%
64	11.895	3374	3376	3379	rVB	1390	728	0.08%	0.009%
65	11.966	3395	3398	3403	rBV	1799	2062	0.22%	0.025%
66	12.567	3582	3585	3591	rVB	2135	1557	0.16%	0.019%
67	13.191	3776	3779	3784	rBV2	1268	1205	0.13%	0.015%
68	13.512	3876	3879	3883	rVB	1985	1297	0.14%	0.016%
69	13.641	3917	3919	3921	rBV	1078	444	0.05%	0.005%
70	13.686	3931	3933	3936	rBV2	1138	676	0.07%	0.008%
71	13.741	3946	3950	3953	rBV	2083	1641	0.17%	0.020%
72	13.847	3980	3983	3985	rBV4	1464	1066	0.11%	0.013%
73	14.049	4044	4046	4049	rBV2	1038	584	0.06%	0.007%
74	14.763	4265	4268	4270	rBV2	1748	1121	0.12%	0.014%
75	15.471	4486	4488	4494	rBV2	1781	1534	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033117.D
Acq On : 06 Dec 2023 15:30
Operator : SY/MD
Sample : 05644-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G27

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis




Sum of corrected areas: 8248247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033117.D
Acq On : 06 Dec 2023 15:30
Operator : SY/MD
Sample : 05644-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

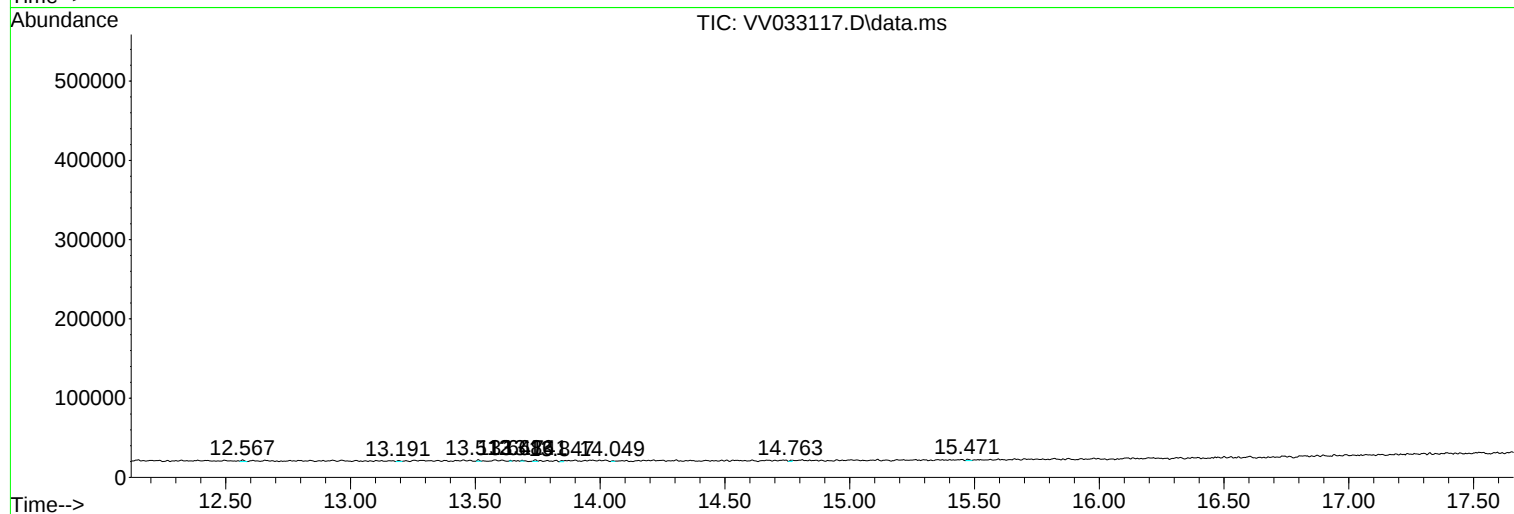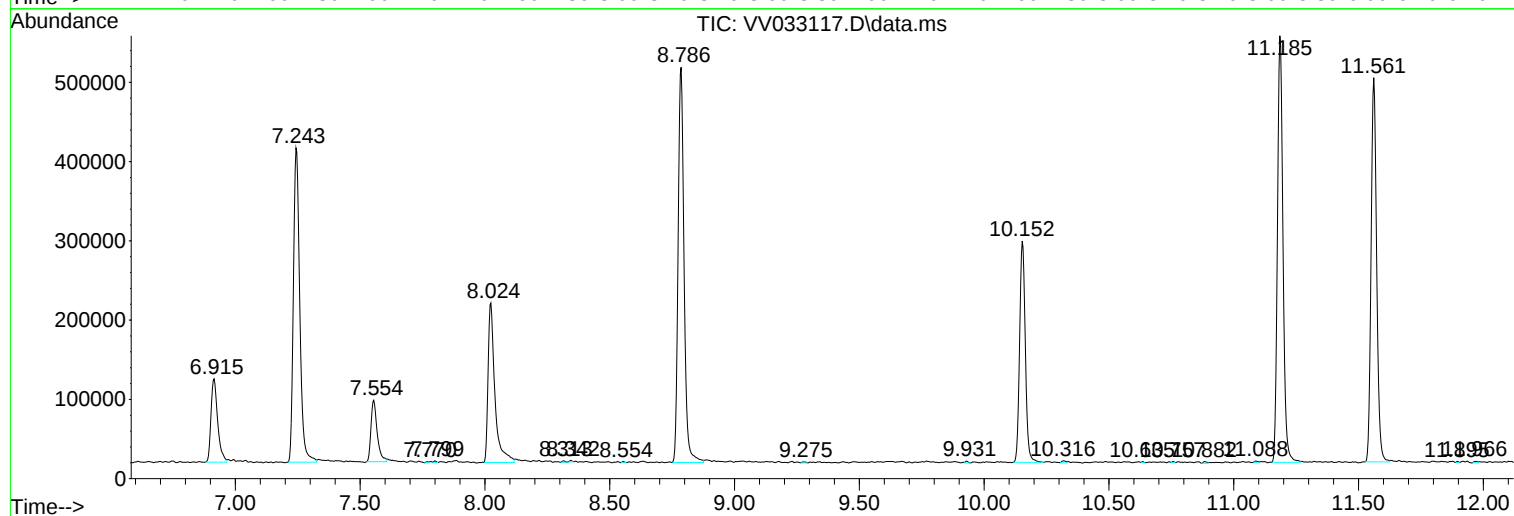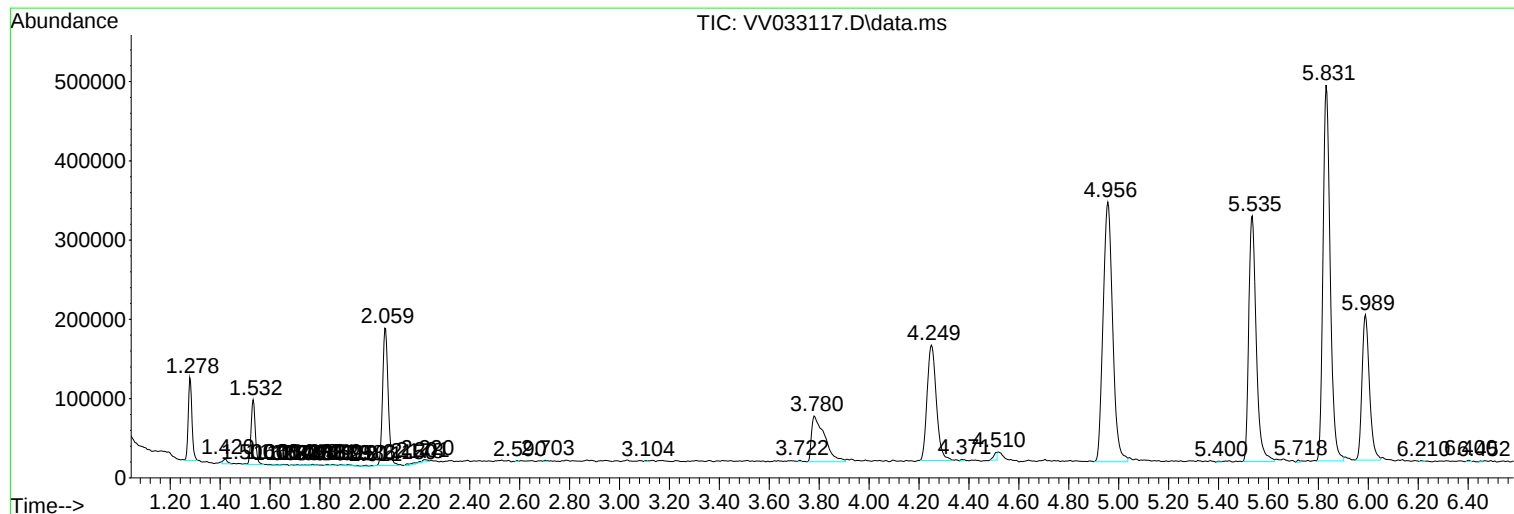

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033117.D
Acq On : 06 Dec 2023 15:30
Operator : SY/MD
Sample : 05644-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033117.D
Acq On : 06 Dec 2023 15:30
Operator : SY/MD
Sample : 05644-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc