

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033118.D
 Acq On : 06 Dec 2023 15:53
 Operator : SY/MD
 Sample : 05644-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	110313	116067	13.30%	1.658%
2	1.420	110	118	127	rVB2	5712	7662	0.88%	0.109%
3	1.484	135	138	139	rBV2	1042	686	0.08%	0.010%
4	1.532	145	153	166	rVB	86197	99531	11.40%	1.422%
5	1.584	166	169	173	rVB2	998	689	0.08%	0.010%
6	1.610	173	177	180	rBV	1602	1261	0.14%	0.018%
7	1.658	189	192	196	rBV2	707	551	0.06%	0.008%
8	1.703	201	206	211	rBV3	930	1229	0.14%	0.018%
9	1.738	215	217	219	rBV2	564	274	0.03%	0.004%
10	1.809	232	239	242	rBV	1568	1587	0.18%	0.023%
11	1.828	242	245	248	rVV3	1198	856	0.10%	0.012%
12	1.844	248	250	252	rVV	750	492	0.06%	0.007%
13	1.854	252	253	254	rVV	941	342	0.04%	0.005%
14	1.876	258	260	263	rVV	1244	731	0.08%	0.010%
15	1.902	263	268	275	rVB	2456	3501	0.40%	0.050%
16	1.941	275	280	282	rBV	854	679	0.08%	0.010%
17	1.957	282	285	287	rBV	910	388	0.04%	0.006%
18	1.970	287	289	290	rBV2	563	269	0.03%	0.004%
19	1.983	290	293	295	rVB2	800	375	0.04%	0.005%
20	2.008	300	301	303	rVB	230	49	0.01%	0.001%
21	2.024	303	306	307	rBV	279	109	0.01%	0.002%
22	2.060	307	317	330	rBV	169152	245361	28.11%	3.506%
23	2.108	330	332	337	rVB3	1264	832	0.10%	0.012%
24	2.156	337	347	349	rBV	2706	3745	0.43%	0.054%
25	2.172	349	352	356	rBV	2283	1915	0.22%	0.027%
26	2.198	357	360	361	rBV	1418	851	0.10%	0.012%
27	2.311	390	395	398	rBV2	1156	1419	0.16%	0.020%
28	3.153	655	657	660	rVB	1240	700	0.08%	0.010%
29	3.539	774	777	779	rBV	1825	1275	0.15%	0.018%
30	3.783	844	853	885	rBV	53277	147375	16.88%	2.106%
31	4.108	951	954	958	rBV	1680	1482	0.17%	0.021%
32	4.130	958	961	964	rVV2	1360	890	0.10%	0.013%
33	4.249	983	998	1024	rBV	143129	374366	42.89%	5.349%
34	4.368	1033	1035	1038	rVB2	1276	699	0.08%	0.010%
35	4.664	1125	1127	1130	rBV	1127	908	0.10%	0.013%
36	4.838	1179	1181	1184	rVB	1683	979	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033118.D
 Acq On : 06 Dec 2023 15:53
 Operator : SY/MD
 Sample : 05644-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1243	rBV2	327278	872912	100.00%	12.473%
38	5.391	1349	1353	1356	rVB	1860	1373	0.16%	0.020%
39	5.474	1376	1379	1382	rBV2	1524	1199	0.14%	0.017%
40	5.535	1386	1398	1420	rBV	276225	564940	64.72%	8.072%
41	5.828	1480	1489	1501	rBV9	8870	19397	2.22%	0.277%
42	5.918	1514	1517	1521	rBV	1562	1289	0.15%	0.018%
43	5.989	1528	1539	1562	rBV	184306	371425	42.55%	5.307%
44	6.156	1588	1591	1593	rBV2	1216	932	0.11%	0.013%
45	6.240	1615	1617	1619	rBV	974	512	0.06%	0.007%
46	6.281	1627	1630	1632	rBV2	1680	1272	0.15%	0.018%
47	6.439	1676	1679	1685	rVB2	1568	1496	0.17%	0.021%
48	6.497	1694	1697	1700	rBV2	1335	1056	0.12%	0.015%
49	6.545	1710	1712	1715	rBV	1857	1304	0.15%	0.019%
50	6.635	1738	1740	1744	rVB2	1216	811	0.09%	0.012%
51	6.703	1758	1761	1764	rBV2	1243	941	0.11%	0.013%
52	6.915	1817	1827	1848	rBV	106017	197024	22.57%	2.815%
53	7.056	1868	1871	1877	rVB2	1653	1470	0.17%	0.021%
54	7.085	1878	1880	1885	rVB2	1223	662	0.08%	0.009%
55	7.243	1919	1929	1954	rBV	401137	710875	81.44%	10.158%
56	7.481	2001	2003	2009	rVB	2421	1932	0.22%	0.028%
57	7.555	2017	2026	2043	rBV2	79679	143659	16.46%	2.053%
58	7.725	2076	2079	2085	rBV5	1432	1903	0.22%	0.027%
59	7.854	2116	2119	2120	rBV2	1158	610	0.07%	0.009%
60	8.024	2163	2172	2197	rBV	198258	370583	42.45%	5.295%
61	8.259	2242	2245	2250	rBV	1819	1791	0.21%	0.026%
62	8.355	2271	2275	2279	rBV2	1587	1724	0.20%	0.025%
63	8.381	2281	2283	2286	rBV	1302	842	0.10%	0.012%
64	8.786	2398	2409	2431	rBV	440952	724883	83.04%	10.358%
65	8.960	2461	2463	2466	rBV3	1139	876	0.10%	0.013%
66	10.050	2800	2802	2804	rBV	1374	841	0.10%	0.012%
67	10.153	2823	2834	2855	rBV	283317	448482	51.38%	6.408%
68	10.268	2867	2870	2872	rBV	1390	1061	0.12%	0.015%
69	10.297	2876	2879	2882	rBV	1600	1263	0.14%	0.018%
70	10.336	2888	2891	2893	rBV	1091	816	0.09%	0.012%
71	10.436	2918	2922	2927	rBV	2088	1724	0.20%	0.025%
72	10.465	2927	2931	2935	rVV	2113	1862	0.21%	0.027%
73	10.500	2939	2942	2948	rBV	1541	1610	0.18%	0.023%
74	10.596	2970	2972	2975	rBV	1089	701	0.08%	0.010%
75	10.895	3062	3065	3066	rBV2	1045	645	0.07%	0.009%
76	10.956	3082	3084	3087	rBV	1095	708	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033118.D
 Acq On : 06 Dec 2023 15:53
 Operator : SY/MD
 Sample : 05644-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.976	3087	3090	3093	rBV	1789	1450	0.17%	0.021%
78	11.053	3111	3114	3118	rBV	1347	1047	0.12%	0.015%
79	11.185	3145	3155	3179	rBV	473413	739082	84.67%	10.561%
80	11.452	3235	3238	3240	rBV	1133	653	0.07%	0.009%
81	11.561	3261	3272	3295	rBV	487633	768348	88.02%	10.979%
82	11.844	3358	3360	3362	rBV	1164	657	0.08%	0.009%
83	11.889	3371	3374	3376	rBV2	1993	1476	0.17%	0.021%
84	12.053	3423	3425	3428	rBV	1233	722	0.08%	0.010%
85	12.233	3478	3481	3484	rBV3	1562	1293	0.15%	0.018%
86	12.693	3622	3624	3626	rBV	1265	716	0.08%	0.010%
87	13.789	3962	3965	3967	rBV	1420	1022	0.12%	0.015%
88	13.995	4026	4029	4032	rVB	1713	981	0.11%	0.014%
89	15.927	4627	4630	4633	rBV	2108	1443	0.17%	0.021%




Sum of corrected areas: 6998421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033118.D
Acq On : 06 Dec 2023 15:53
Operator : SY/MD
Sample : 05644-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

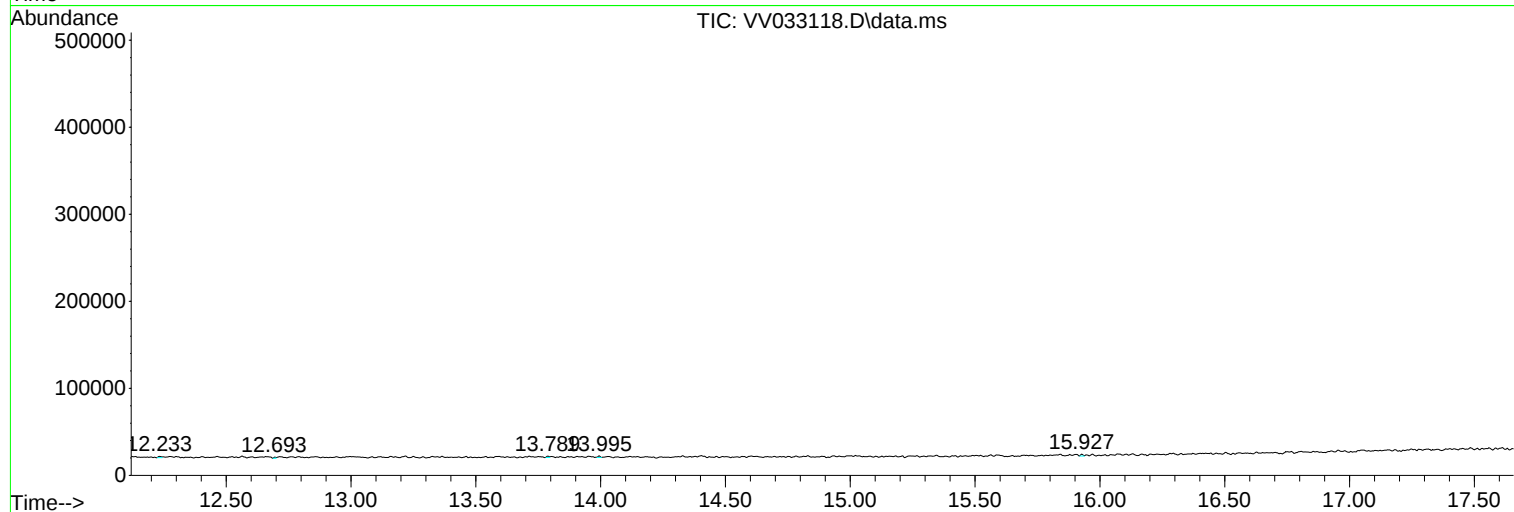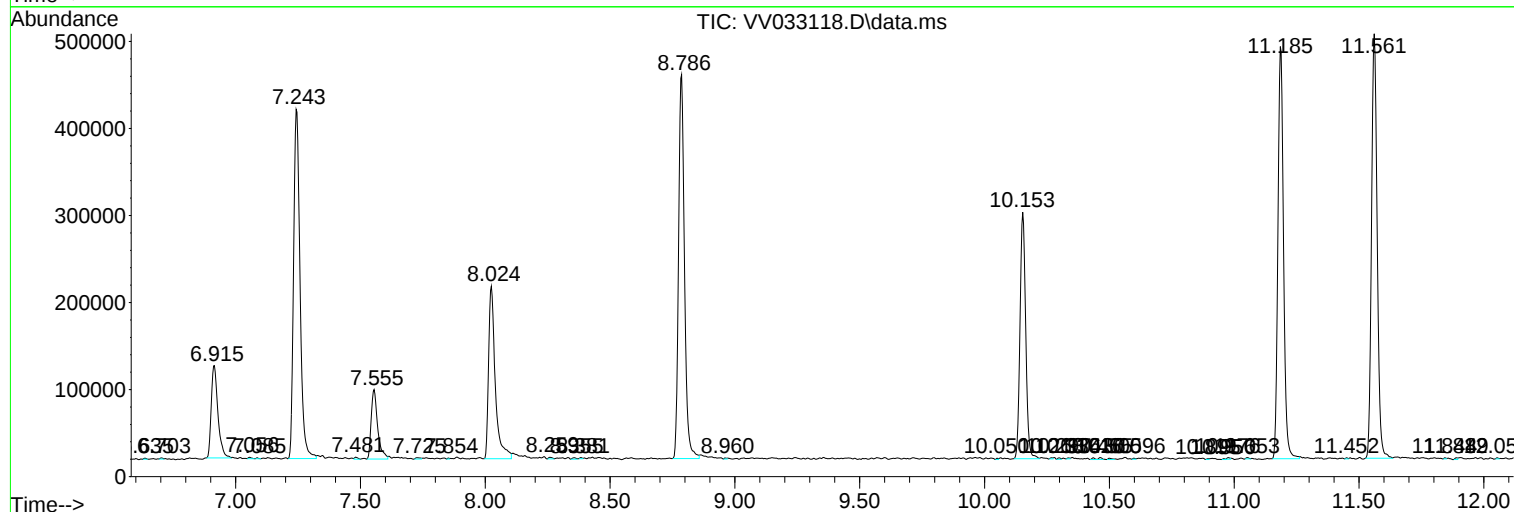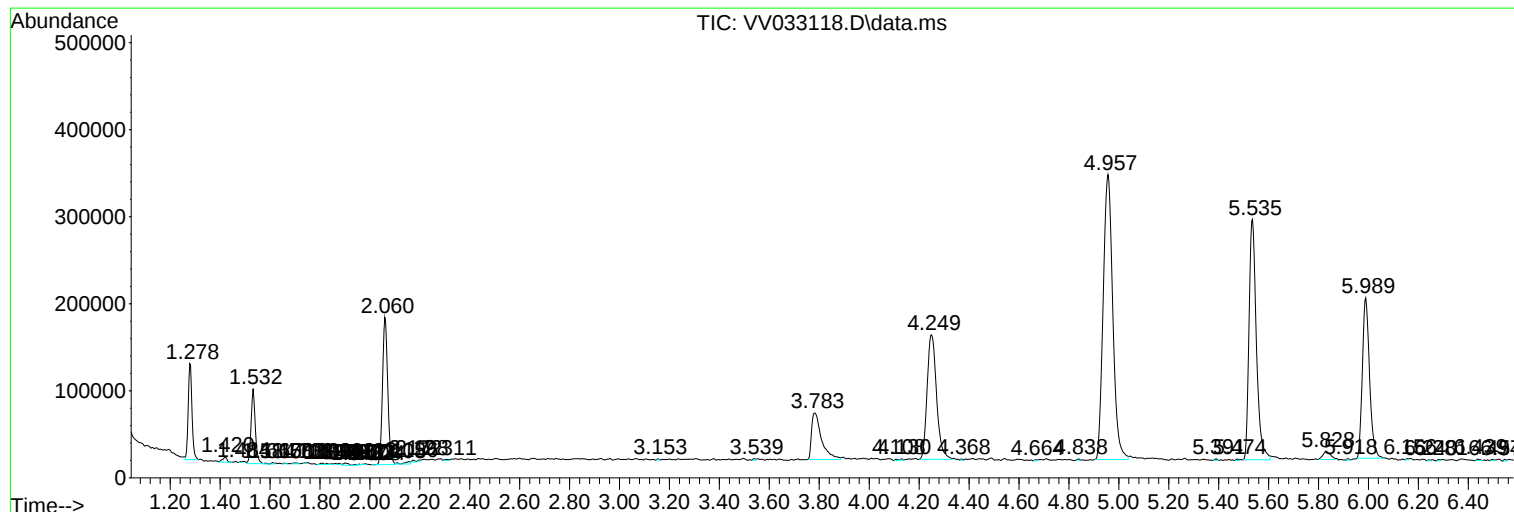

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033118.D
Acq On : 06 Dec 2023 15:53
Operator : SY/MD
Sample : 05644-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033118.D
Acq On : 06 Dec 2023 15:53
Operator : SY/MD
Sample : 05644-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------