

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033120.D
 Acq On : 06 Dec 2023 16:40
 Operator : SY/MD
 Sample : 05644-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	103506	112009	13.46%	1.570%
2	1.417	110	117	126	rVB2	5526	7932	0.95%	0.111%
3	1.471	132	134	140	rBV3	878	837	0.10%	0.012%
4	1.532	144	153	162	rBV	76641	90505	10.88%	1.268%
5	1.603	173	175	180	rVB	2087	1391	0.17%	0.019%
6	1.648	186	189	190	rBV2	1477	873	0.10%	0.012%
7	1.667	190	195	198	rBV3	501	539	0.06%	0.008%
8	1.712	205	209	210	rBV2	934	563	0.07%	0.008%
9	1.722	210	212	215	rVB	1196	603	0.07%	0.008%
10	1.774	225	228	231	rVB2	1047	609	0.07%	0.009%
11	1.802	231	237	243	rVB2	1561	2266	0.27%	0.032%
12	1.838	243	248	251	rBV2	1489	1488	0.18%	0.021%
13	1.873	256	259	261	rBV3	977	665	0.08%	0.009%
14	1.944	278	281	286	rVB4	858	836	0.10%	0.012%
15	1.989	292	295	298	rBV	1080	928	0.11%	0.013%
16	2.060	303	317	328	rBV	159792	236463	28.42%	3.314%
17	2.108	328	332	340	rVB3	5758	8784	1.06%	0.123%
18	2.140	340	342	344	rBV2	1366	870	0.10%	0.012%
19	2.220	358	367	378	rBV2	10124	19838	2.38%	0.278%
20	2.426	429	431	434	rBV	1003	555	0.07%	0.008%
21	2.446	435	437	440	rVV3	1473	817	0.10%	0.011%
22	2.545	465	468	470	rBV2	1415	1030	0.12%	0.014%
23	2.799	545	547	549	rBV	1436	687	0.08%	0.010%
24	2.912	578	582	586	rBV	2158	2645	0.32%	0.037%
25	3.320	702	709	719	rBV	2579	4994	0.60%	0.070%
26	3.413	735	738	741	rBV	1997	1355	0.16%	0.019%
27	3.584	788	791	793	rBV	1454	978	0.12%	0.014%
28	3.780	844	852	878	rBV	58272	153053	18.39%	2.145%
29	4.249	984	998	1020	rBV	141027	352943	42.42%	4.946%
30	4.394	1039	1043	1045	rBV	1170	936	0.11%	0.013%
31	4.667	1126	1128	1133	rBV2	1483	1106	0.13%	0.015%
32	4.957	1202	1218	1248	rBV2	309176	828482	99.57%	11.610%
33	5.230	1301	1303	1306	rBV2	1108	689	0.08%	0.010%
34	5.259	1310	1312	1318	rVB3	1392	1353	0.16%	0.019%
35	5.291	1319	1322	1324	rBV	1500	972	0.12%	0.014%
36	5.535	1387	1398	1423	rBV	312797	644649	77.48%	9.034%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033120.D
 Acq On : 06 Dec 2023 16:40
 Operator : SY/MD
 Sample : 05644-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.838	1482	1492	1507	rBV5	26920	56916	6.84%	0.798%
38	5.931	1518	1521	1525	rBV	1805	1664	0.20%	0.023%
39	5.989	1527	1539	1558	rVV	177330	362717	43.59%	5.083%
40	6.169	1591	1595	1601	rVB2	1558	1524	0.18%	0.021%
41	6.310	1632	1639	1642	rBV	1627	2222	0.27%	0.031%
42	6.545	1709	1712	1714	rBV	1303	942	0.11%	0.013%
43	6.754	1774	1777	1782	rBV	1349	1111	0.13%	0.016%
44	6.912	1814	1826	1848	rBV	100157	193760	23.29%	2.715%
45	7.195	1912	1914	1918	rBV2	1000	517	0.06%	0.007%
46	7.243	1919	1929	1949	rBV	380861	665077	79.93%	9.320%
47	7.439	1988	1990	1993	rBV	1347	801	0.10%	0.011%
48	7.522	2012	2016	2017	rBV	1802	1315	0.16%	0.018%
49	7.555	2017	2026	2045	rVV2	74207	132083	15.87%	1.851%
50	7.821	2106	2109	2112	rBV2	1123	1029	0.12%	0.014%
51	7.934	2141	2144	2147	rVB	1736	1023	0.12%	0.014%
52	7.953	2147	2150	2152	rBV	1030	614	0.07%	0.009%
53	8.024	2163	2172	2197	rBV	195500	356797	42.88%	5.000%
54	8.371	2278	2280	2283	rBV	1246	786	0.09%	0.011%
55	8.506	2320	2322	2325	rBV2	1139	661	0.08%	0.009%
56	8.548	2330	2335	2337	rBV2	1591	1850	0.22%	0.026%
57	8.654	2365	2368	2373	rBV	1197	1028	0.12%	0.014%
58	8.786	2397	2409	2436	rBV	492764	827105	99.40%	11.590%
59	9.172	2527	2529	2536	rVB	1509	1222	0.15%	0.017%
60	9.252	2551	2554	2557	rBV	1438	1179	0.14%	0.017%
61	9.461	2616	2619	2623	rBV	1751	1228	0.15%	0.017%
62	9.487	2624	2627	2630	rBV	1178	766	0.09%	0.011%
63	9.506	2630	2633	2635	rBV2	1311	783	0.09%	0.011%
64	9.609	2662	2665	2668	rBV	1720	1272	0.15%	0.018%
65	9.741	2703	2706	2708	rBV	1265	893	0.11%	0.013%
66	9.844	2735	2738	2740	rBV	1189	796	0.10%	0.011%
67	9.915	2757	2760	2762	rBV	1556	944	0.11%	0.013%
68	10.018	2788	2792	2795	rBV2	1656	1665	0.20%	0.023%
69	10.072	2806	2809	2812	rBV	1771	962	0.12%	0.013%
70	10.153	2823	2834	2850	rBV	273986	429117	51.57%	6.013%
71	10.288	2874	2876	2878	rBV2	1134	696	0.08%	0.010%
72	10.500	2939	2942	2947	rBV	1366	930	0.11%	0.013%
73	10.551	2956	2958	2961	rVB2	1316	605	0.07%	0.008%
74	10.661	2987	2992	2996	rBV	1843	2001	0.24%	0.028%
75	11.050	3109	3113	3121	rBV	1692	2253	0.27%	0.032%
76	11.101	3126	3129	3134	rVB	2065	1491	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033120.D
 Acq On : 06 Dec 2023 16:40
 Operator : SY/MD
 Sample : 05644-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G45

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3145	3155	3176	rBV	544768	832073	100.00%	11.660%
78	11.561	3261	3272	3287	rBV	466206	728633	87.57%	10.210%
79	11.789	3340	3343	3346	rBV2	1382	1248	0.15%	0.017%
80	12.480	3556	3558	3564	rVB	1797	1378	0.17%	0.019%
81	12.628	3601	3604	3610	rVB	1762	1779	0.21%	0.025%
82	13.214	3782	3786	3792	rBV3	1816	2231	0.27%	0.031%
83	13.503	3873	3876	3879	rBV2	1120	839	0.10%	0.012%
84	13.638	3914	3918	3921	rBV	2261	1785	0.21%	0.025%
85	13.657	3921	3924	3928	rVB	1707	1077	0.13%	0.015%
86	13.683	3929	3932	3934	rBV	1345	832	0.10%	0.012%
87	13.837	3977	3980	3986	rBV	1520	1422	0.17%	0.020%
88	13.869	3987	3990	3993	rBV	1634	969	0.12%	0.014%
89	13.982	4022	4025	4028	rBV	1637	1419	0.17%	0.020%
90	14.175	4083	4085	4088	rBV2	1705	1099	0.13%	0.015%
91	14.294	4119	4122	4126	rBV	1337	1146	0.14%	0.016%
92	14.503	4184	4187	4193	rVB	2152	1714	0.21%	0.024%
93	14.767	4266	4269	4271	rBV2	1514	1062	0.13%	0.015%
94	14.869	4296	4301	4304	rBV4	2045	2142	0.26%	0.030%
95	15.040	4352	4354	4356	rBV	1298	669	0.08%	0.009%
96	15.098	4369	4372	4376	rBV3	1745	1786	0.21%	0.025%
97	15.246	4412	4418	4420	rBV2	1985	2199	0.26%	0.031%
98	15.332	4442	4445	4446	rBV2	1683	968	0.12%	0.014%
99	15.593	4523	4526	4529	rVB	1526	889	0.11%	0.012%
100	16.146	4696	4698	4700	rBV2	1941	1199	0.14%	0.017%




Sum of corrected areas: 7136146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033120.D
Acq On : 06 Dec 2023 16:40
Operator : SY/MD
Sample : 05644-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

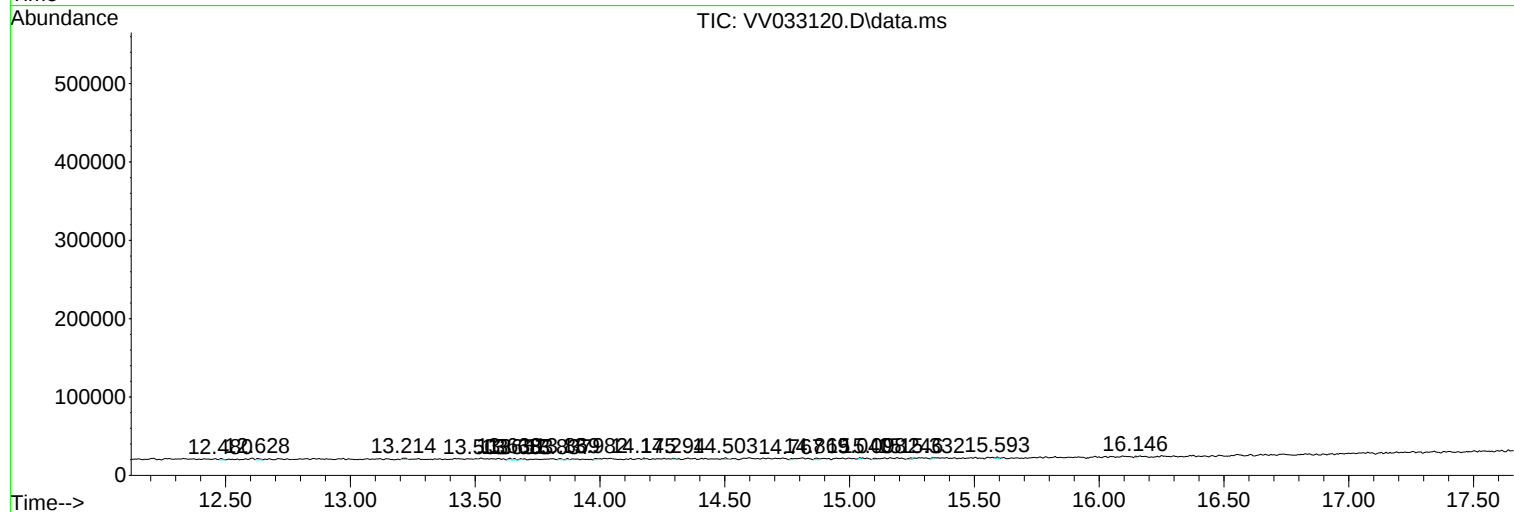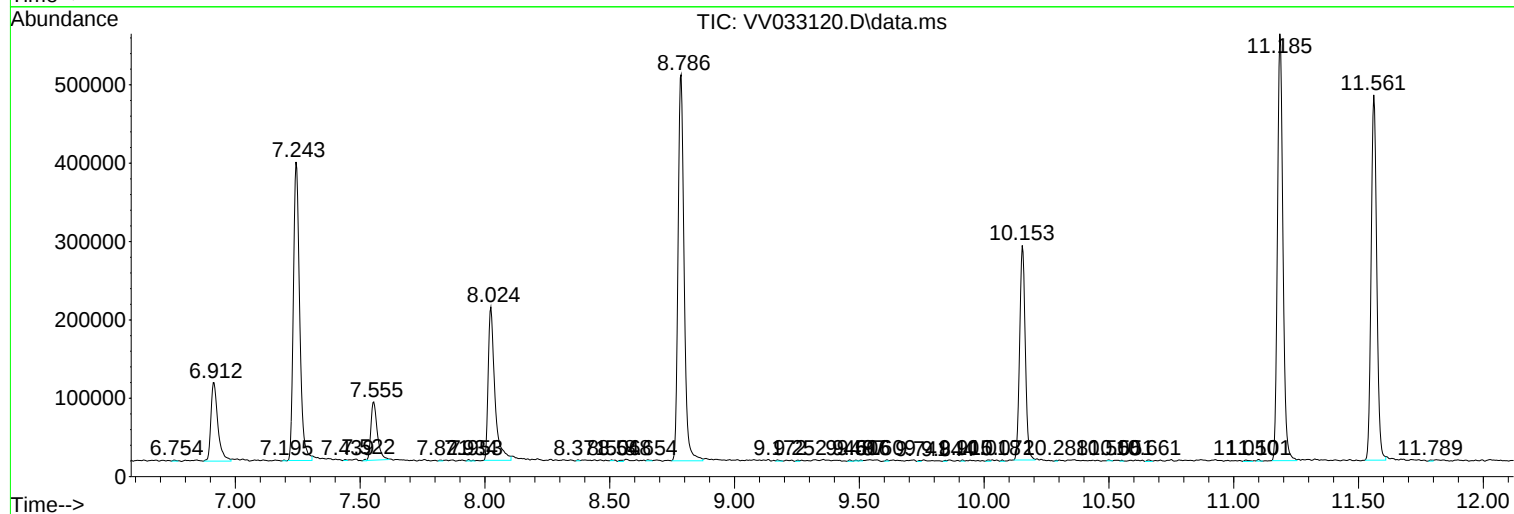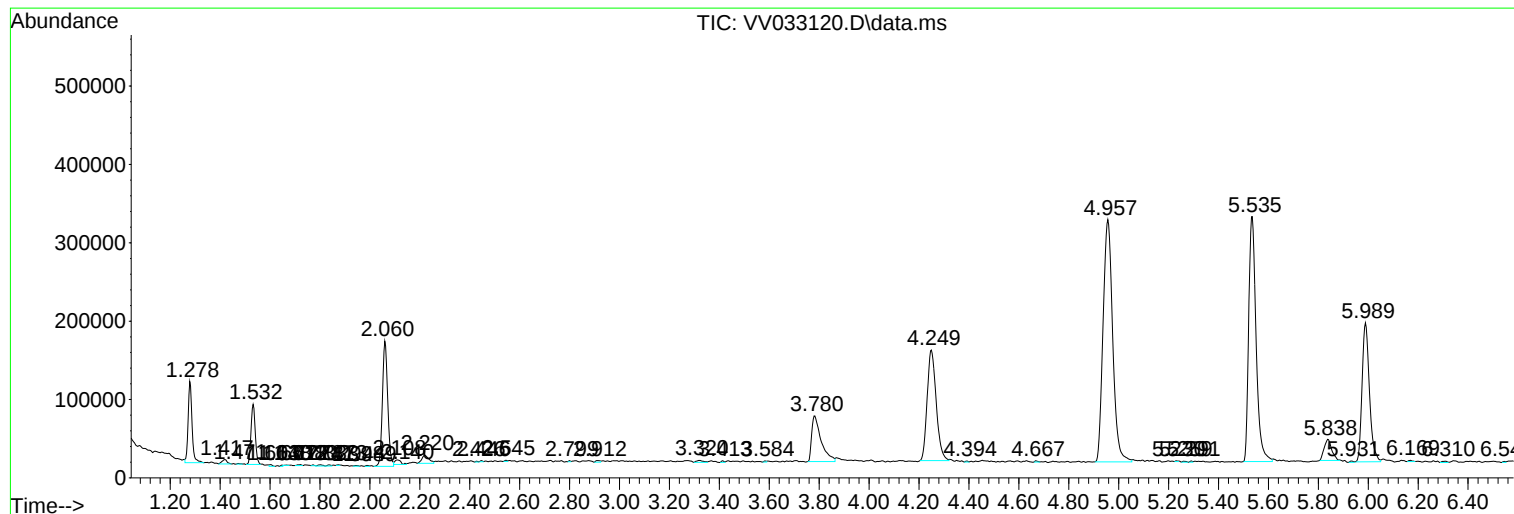

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033120.D
Acq On : 06 Dec 2023 16:40
Operator : SY/MD
Sample : 05644-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033120.D
Acq On : 06 Dec 2023 16:40
Operator : SY/MD
Sample : 05644-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------