

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033121.D
 Acq On : 06 Dec 2023 17:03
 Operator : SY/MD
 Sample : 05644-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	101327	107330	12.97%	1.557%
2	1.401	109	112	113	rBV	1049	571	0.07%	0.008%
3	1.417	113	117	125	rVB2	6294	8119	0.98%	0.118%
4	1.455	125	129	132	rBV2	1324	1045	0.13%	0.015%
5	1.532	144	153	166	rVB	73723	88968	10.75%	1.291%
6	1.581	166	168	174	rVB2	1369	1116	0.13%	0.016%
7	1.661	187	193	198	rBV3	1765	1915	0.23%	0.028%
8	1.690	198	202	208	rBV6	1304	1526	0.18%	0.022%
9	1.725	211	213	217	rVB2	1540	1105	0.13%	0.016%
10	1.748	217	220	224	rBV3	1564	1437	0.17%	0.021%
11	1.770	224	227	229	rBV2	1025	563	0.07%	0.008%
12	1.802	234	237	241	rVB3	1044	855	0.10%	0.012%
13	1.825	241	244	246	rVB2	692	426	0.05%	0.006%
14	1.864	252	256	258	rBV2	867	610	0.07%	0.009%
15	1.883	258	262	265	rVB3	1014	818	0.10%	0.012%
16	1.912	268	271	274	rVB3	1384	952	0.12%	0.014%
17	1.950	279	283	286	rBV2	979	658	0.08%	0.010%
18	1.973	286	290	292	rVB2	739	463	0.06%	0.007%
19	2.060	306	317	336	rBV2	165516	260996	31.55%	3.787%
20	2.156	341	347	348	rBV	2251	2022	0.24%	0.029%
21	2.172	348	352	354	rBV2	1630	1300	0.16%	0.019%
22	2.220	359	367	375	rBV2	8505	15345	1.85%	0.223%
23	2.687	509	512	514	rBV2	1852	1281	0.15%	0.019%
24	3.372	723	725	727	rBV	1516	961	0.12%	0.014%
25	3.699	823	827	830	rBV2	1650	1589	0.19%	0.023%
26	3.783	844	853	857	rBV2	60865	102532	12.39%	1.488%
27	3.934	898	900	903	rVB	2161	1150	0.14%	0.017%
28	4.150	964	967	970	rBV	1893	1574	0.19%	0.023%
29	4.249	982	998	1027	rBV	139581	360846	43.61%	5.236%
30	4.394	1040	1043	1046	rBV	1455	913	0.11%	0.013%
31	4.413	1046	1049	1050	rBV2	1056	601	0.07%	0.009%
32	4.516	1072	1081	1089	rBV5	7135	12933	1.56%	0.188%
33	4.635	1115	1118	1123	rBV	1198	1216	0.15%	0.018%
34	4.873	1189	1192	1193	rBV	1456	820	0.10%	0.012%
35	4.957	1202	1218	1249	rBV2	306881	827354	100.00%	12.005%
36	5.532	1387	1397	1424	rBV	300893	621541	75.12%	9.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033121.D
 Acq On : 06 Dec 2023 17:03
 Operator : SY/MD
 Sample : 05644-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.834	1483	1491	1503	rVB5	8082	15857	1.92%	0.230%
38	5.934	1520	1522	1525	rVB	1334	631	0.08%	0.009%
39	5.989	1527	1539	1562	rVV	171806	354637	42.86%	5.146%
40	6.166	1591	1594	1601	rBV2	1492	1671	0.20%	0.024%
41	6.532	1705	1708	1710	rBV	1455	871	0.11%	0.013%
42	6.564	1715	1718	1721	rBV	1415	1037	0.13%	0.015%
43	6.616	1731	1734	1737	rVB	1440	909	0.11%	0.013%
44	6.677	1751	1753	1756	rVB	1747	942	0.11%	0.014%
45	6.818	1795	1797	1802	rVB	1540	1026	0.12%	0.015%
46	6.915	1817	1827	1841	rBV	97364	177644	21.47%	2.578%
47	7.018	1857	1859	1862	rBV	1249	591	0.07%	0.009%
48	7.243	1919	1929	1954	rBV	363412	643936	77.83%	9.344%
49	7.555	2015	2026	2041	rBV2	72675	129185	15.61%	1.875%
50	7.748	2083	2086	2091	rVB	2109	1533	0.19%	0.022%
51	7.908	2133	2136	2141	rBV	2152	2150	0.26%	0.031%
52	8.024	2163	2172	2190	rBV	191765	347315	41.98%	5.040%
53	8.233	2233	2237	2241	rBV	2102	2205	0.27%	0.032%
54	8.461	2306	2308	2312	rVB	1319	731	0.09%	0.011%
55	8.564	2337	2340	2345	rBV	1961	1498	0.18%	0.022%
56	8.725	2387	2390	2393	rBV	1499	1019	0.12%	0.015%
57	8.786	2398	2409	2435	rBV	476030	792728	95.81%	11.503%
58	9.239	2547	2550	2556	rVB	1354	979	0.12%	0.014%
59	9.307	2568	2571	2573	rBV	1918	1461	0.18%	0.021%
60	9.400	2598	2600	2604	rBV3	1138	903	0.11%	0.013%
61	9.612	2663	2666	2669	rBV2	1197	820	0.10%	0.012%
62	9.825	2727	2732	2735	rBV	2317	2820	0.34%	0.041%
63	10.092	2813	2815	2817	rVB2	1029	441	0.05%	0.006%
64	10.153	2824	2834	2850	rVB	265511	413558	49.99%	6.001%
65	10.362	2896	2899	2901	rBV	1516	1108	0.13%	0.016%
66	10.484	2934	2937	2940	rBV2	1470	1035	0.13%	0.015%
67	10.516	2945	2947	2955	rVB	1691	1747	0.21%	0.025%
68	10.635	2982	2984	2987	rBV	1139	748	0.09%	0.011%
69	10.657	2988	2991	2994	rBV	1593	1152	0.14%	0.017%
70	10.741	3014	3017	3021	rBV	2007	1330	0.16%	0.019%
71	10.821	3039	3042	3045	rBV	1888	1242	0.15%	0.018%
72	10.873	3056	3058	3063	rBV2	993	763	0.09%	0.011%
73	10.924	3068	3074	3079	rBV	1316	1797	0.22%	0.026%
74	11.046	3109	3112	3115	rBV	1476	1078	0.13%	0.016%
75	11.066	3115	3118	3123	rVV	1340	1449	0.18%	0.021%
76	11.185	3143	3155	3176	rBV	521471	811735	98.11%	11.779%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033121.D
 Acq On : 06 Dec 2023 17:03
 Operator : SY/MD
 Sample : 05644-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.304	3190	3192	3195	rBV	1127	666	0.08%	0.010%
78	11.513	3255	3257	3259	rBV	1006	587	0.07%	0.009%
79	11.561	3261	3272	3290	rVV	450031	708404	85.62%	10.279%
80	11.702	3312	3316	3320	rVB	1607	1493	0.18%	0.022%
81	11.722	3320	3322	3327	rBV	1595	1291	0.16%	0.019%
82	11.944	3388	3391	3395	rVB	2055	1491	0.18%	0.022%
83	12.207	3471	3473	3475	rBV	1010	449	0.05%	0.007%
84	12.464	3549	3553	3558	rBV	1742	1952	0.24%	0.028%
85	12.612	3596	3599	3601	rBV2	1143	662	0.08%	0.010%
86	12.866	3675	3678	3682	rBV	1594	1179	0.14%	0.017%
87	12.972	3708	3711	3713	rBV	1369	742	0.09%	0.011%
88	13.178	3772	3775	3780	rBV2	1491	1172	0.14%	0.017%
89	13.336	3820	3824	3828	rBV2	1852	1636	0.20%	0.024%
90	13.802	3967	3969	3973	rBV2	1088	821	0.10%	0.012%
91	14.104	4060	4063	4066	rBV	1352	1172	0.14%	0.017%
92	14.201	4091	4093	4096	rBV	1104	550	0.07%	0.008%
93	14.660	4233	4236	4238	rBV2	1973	1128	0.14%	0.016%
94	14.677	4238	4241	4245	rVV	2119	1665	0.20%	0.024%
95	14.696	4245	4247	4250	rVB2	1165	798	0.10%	0.012%
96	15.037	4351	4353	4356	rBV	1349	725	0.09%	0.011%
97	15.114	4375	4377	4379	rBV2	1201	734	0.09%	0.011%
98	15.503	4495	4498	4501	rBV	2116	1485	0.18%	0.022%
99	15.596	4525	4527	4531	rBV3	1796	1138	0.14%	0.017%
100	16.233	4722	4725	4728	rBV2	2384	1838	0.22%	0.027%




Sum of corrected areas: 6891511

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033121.D
Acq On : 06 Dec 2023 17:03
Operator : SY/MD
Sample : 05644-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

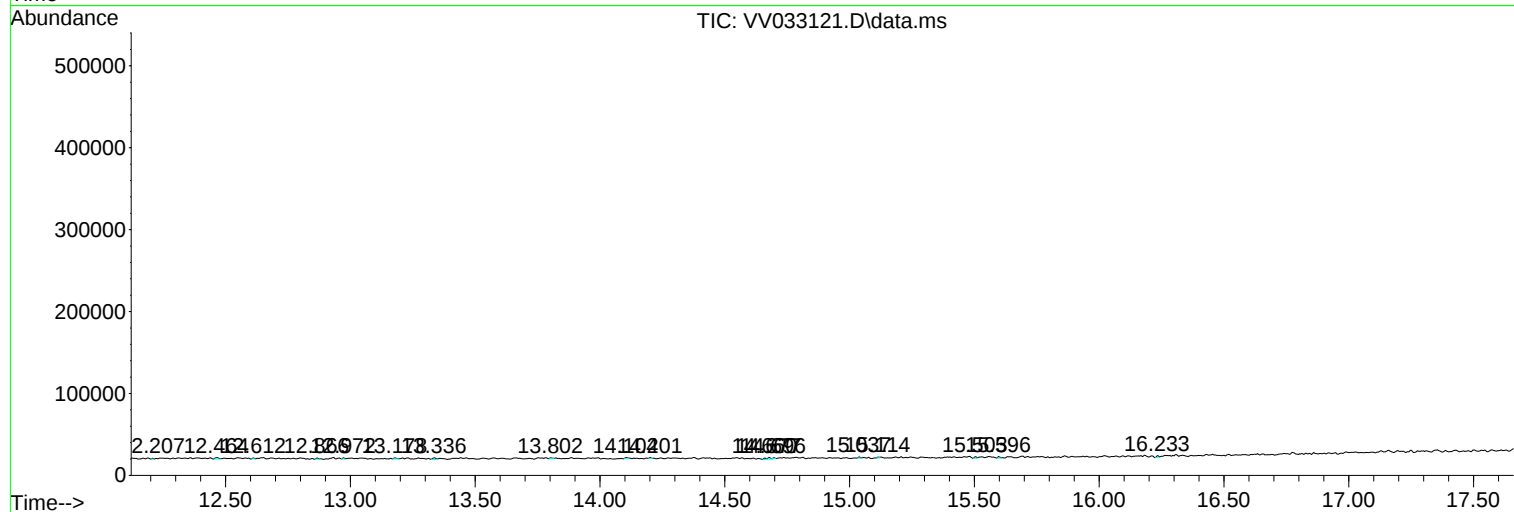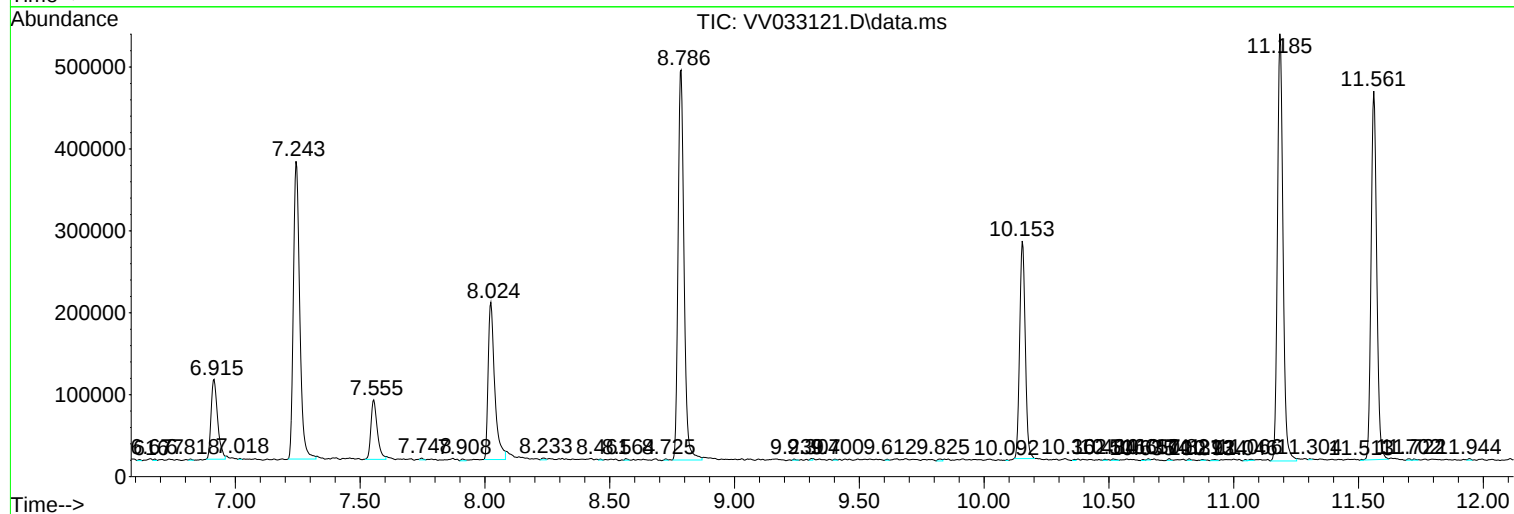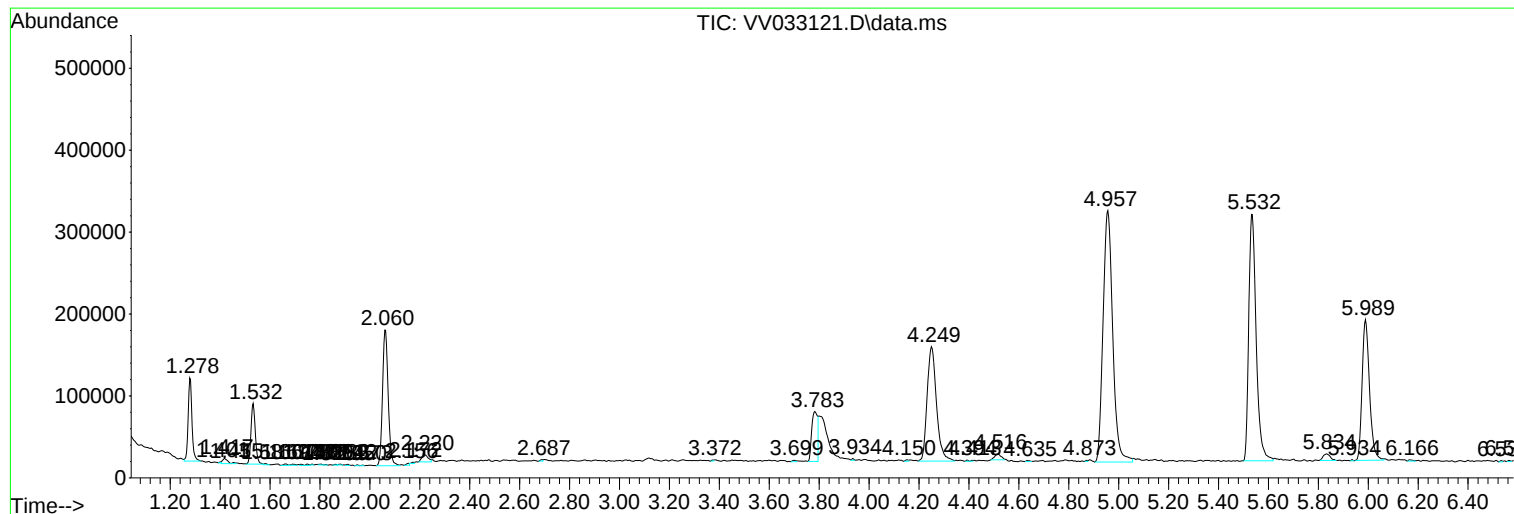

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033121.D
Acq On : 06 Dec 2023 17:03
Operator : SY/MD
Sample : 05644-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033121.D
Acq On : 06 Dec 2023 17:03
Operator : SY/MD
Sample : 05644-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc