

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033122.D
 Acq On : 06 Dec 2023 17:26
 Operator : SY/MD
 Sample : 05644-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	104867	111361	13.41%	1.415%
2	1.420	113	118	123	rVB3	5905	6224	0.75%	0.079%
3	1.471	131	134	137	rVB	1579	1100	0.13%	0.014%
4	1.491	137	140	142	rVV4	1176	827	0.10%	0.011%
5	1.532	143	153	169	rVB	77104	95239	11.47%	1.210%
6	1.593	169	172	176	rVB2	996	877	0.11%	0.011%
7	1.677	195	198	201	rVB	1434	984	0.12%	0.013%
8	1.696	201	204	206	rBV2	1009	786	0.09%	0.010%
9	1.725	209	213	216	rVB4	971	813	0.10%	0.010%
10	1.748	216	220	221	rBV	815	621	0.07%	0.008%
11	1.851	246	252	255	rBV	1743	1313	0.16%	0.017%
12	1.899	264	267	272	rVB3	1019	902	0.11%	0.011%
13	1.931	272	277	280	rVB3	1705	1780	0.21%	0.023%
14	1.970	280	289	292	rBV	1772	2332	0.28%	0.030%
15	2.060	305	317	331	rBV	165350	251914	30.34%	3.201%
16	2.111	331	333	340	rVB6	2129	1910	0.23%	0.024%
17	2.169	348	351	352	rBV	1048	545	0.07%	0.007%
18	2.182	352	355	357	rBV	1629	874	0.11%	0.011%
19	2.224	358	368	379	rBV2	8019	18005	2.17%	0.229%
20	2.339	401	404	407	rBV	1293	876	0.11%	0.011%
21	2.429	430	432	434	rBV	1181	756	0.09%	0.010%
22	2.532	461	464	467	rBV	1569	1069	0.13%	0.014%
23	2.860	564	566	568	rBV	1421	924	0.11%	0.012%
24	2.934	586	589	593	rBV	1435	1233	0.15%	0.016%
25	2.970	597	600	605	rBV	1676	1567	0.19%	0.020%
26	3.233	680	682	684	rBV2	1200	727	0.09%	0.009%
27	3.458	747	752	757	rBV2	2001	2951	0.36%	0.038%
28	3.564	782	785	790	rBV	1459	1118	0.13%	0.014%
29	3.642	806	809	811	rBV	1730	1243	0.15%	0.016%
30	3.780	844	852	881	rBV2	57669	193655	23.32%	2.461%
31	4.101	950	952	954	rBV2	1133	681	0.08%	0.009%
32	4.249	984	998	1023	rBV2	139121	354115	42.65%	4.500%
33	4.355	1029	1031	1035	rVB	1539	767	0.09%	0.010%
34	4.420	1048	1051	1055	rVB4	1559	1013	0.12%	0.013%
35	4.513	1072	1080	1100	rVB5	11517	30162	3.63%	0.383%
36	4.687	1131	1134	1137	rBV2	1258	819	0.10%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033122.D
 Acq On : 06 Dec 2023 17:26
 Operator : SY/MD
 Sample : 05644-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1240	rBV2	309661	817739	98.49%	10.392%
38	5.198	1291	1293	1296	rBV2	1176	725	0.09%	0.009%
39	5.265	1312	1314	1316	rBV	1311	869	0.10%	0.011%
40	5.535	1387	1398	1423	rBV	310561	637511	76.78%	8.102%
41	5.764	1466	1469	1472	rBV	1457	986	0.12%	0.013%
42	5.831	1478	1490	1512	rBV	361230	733499	88.35%	9.321%
43	5.989	1527	1539	1560	rBV2	176923	358192	43.14%	4.552%
44	6.182	1597	1599	1602	rVB	1620	830	0.10%	0.011%
45	6.555	1712	1715	1718	rBV2	1132	874	0.11%	0.011%
46	6.593	1725	1727	1730	rBV	1007	706	0.09%	0.009%
47	6.738	1769	1772	1775	rBV2	1144	702	0.08%	0.009%
48	6.802	1789	1792	1795	rBV2	1293	997	0.12%	0.013%
49	6.915	1817	1827	1850	rBV	100915	192825	23.22%	2.450%
50	7.114	1887	1889	1898	rVB2	1334	1537	0.19%	0.020%
51	7.243	1917	1929	1954	rBV	376958	674579	81.25%	8.573%
52	7.555	2017	2026	2042	rBV	73135	125832	15.16%	1.599%
53	8.024	2163	2172	2201	rBV	193782	369239	44.47%	4.692%
54	8.744	2393	2396	2397	rBV	1374	774	0.09%	0.010%
55	8.786	2398	2409	2426	rVV	489960	800928	96.47%	10.178%
56	9.442	2610	2613	2614	rBV	1047	695	0.08%	0.009%
57	9.526	2636	2639	2642	rBV	1279	999	0.12%	0.013%
58	9.545	2643	2645	2649	rBV2	1081	870	0.10%	0.011%
59	9.751	2707	2709	2714	rBV	1363	959	0.12%	0.012%
60	9.969	2774	2777	2779	rBV	1166	759	0.09%	0.010%
61	10.034	2793	2797	2801	rBV	1769	1560	0.19%	0.020%
62	10.091	2813	2815	2819	rVB2	1783	935	0.11%	0.012%
63	10.153	2824	2834	2856	rBV	268909	430736	51.88%	5.474%
64	10.458	2925	2929	2933	rBV	1849	1699	0.20%	0.022%
65	10.754	3018	3021	3025	rBV	1421	1386	0.17%	0.018%
66	10.866	3053	3056	3061	rVB	2773	2652	0.32%	0.034%
67	10.895	3062	3065	3068	rBV	2197	1601	0.19%	0.020%
68	11.185	3144	3155	3177	rBV	533132	830263	100.00%	10.551%
69	11.509	3253	3256	3259	rBV	1446	1127	0.14%	0.014%
70	11.561	3260	3272	3298	rVV	467841	739149	89.03%	9.393%
71	11.712	3316	3319	3321	rBV	1523	953	0.11%	0.012%
72	11.751	3328	3331	3333	rBV	2010	1194	0.14%	0.015%
73	12.124	3444	3447	3457	rVB	1524	2142	0.26%	0.027%
74	12.310	3502	3505	3509	rVB	1846	1608	0.19%	0.020%
75	12.333	3509	3512	3514	rBV	1379	915	0.11%	0.012%
76	12.532	3571	3574	3576	rBV	1509	999	0.12%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033122.D
 Acq On : 06 Dec 2023 17:26
 Operator : SY/MD
 Sample : 05644-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.612	3596	3599	3603	rBV	1312	1123	0.14%	0.014%
78	12.651	3606	3611	3614	rBV2	1815	1830	0.22%	0.023%
79	12.882	3679	3683	3691	rBV	2196	3172	0.38%	0.040%
80	13.053	3733	3736	3740	rVB	1950	1170	0.14%	0.015%
81	13.426	3850	3852	3855	rBV2	1114	658	0.08%	0.008%
82	13.477	3865	3868	3873	rBV	1696	1585	0.19%	0.020%
83	13.506	3874	3877	3879	rBV	1371	974	0.12%	0.012%
84	13.625	3911	3914	3915	rBV	1265	854	0.10%	0.011%
85	14.059	4047	4049	4052	rBV	1313	705	0.08%	0.009%
86	14.075	4052	4054	4057	rBV	1025	562	0.07%	0.007%
87	14.165	4078	4082	4085	rBV	1974	1664	0.20%	0.021%
88	14.223	4094	4100	4103	rBV	2113	2516	0.30%	0.032%
89	14.336	4132	4135	4137	rBV	1572	942	0.11%	0.012%
90	14.580	4208	4211	4215	rBV	1952	2144	0.26%	0.027%
91	14.966	4328	4331	4335	rBV	1754	1667	0.20%	0.021%
92	15.059	4358	4360	4362	rBV2	1177	688	0.08%	0.009%
93	15.095	4367	4371	4374	rBV	2450	2018	0.24%	0.026%
94	15.287	4429	4431	4434	rVB2	1670	839	0.10%	0.011%
95	15.307	4434	4437	4439	rBV	1536	1093	0.13%	0.014%
96	15.522	4501	4504	4508	rBV	2732	2379	0.29%	0.030%
97	15.593	4523	4526	4528	rBV3	1927	1464	0.18%	0.019%
98	15.673	4549	4551	4554	rVB	1625	819	0.10%	0.010%
99	15.863	4606	4610	4615	rBV	2282	1997	0.24%	0.025%
100	16.683	4862	4865	4868	rBV3	2244	1544	0.19%	0.020%




Sum of corrected areas: 7869035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033122.D
Acq On : 06 Dec 2023 17:26
Operator : SY/MD
Sample : 05644-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

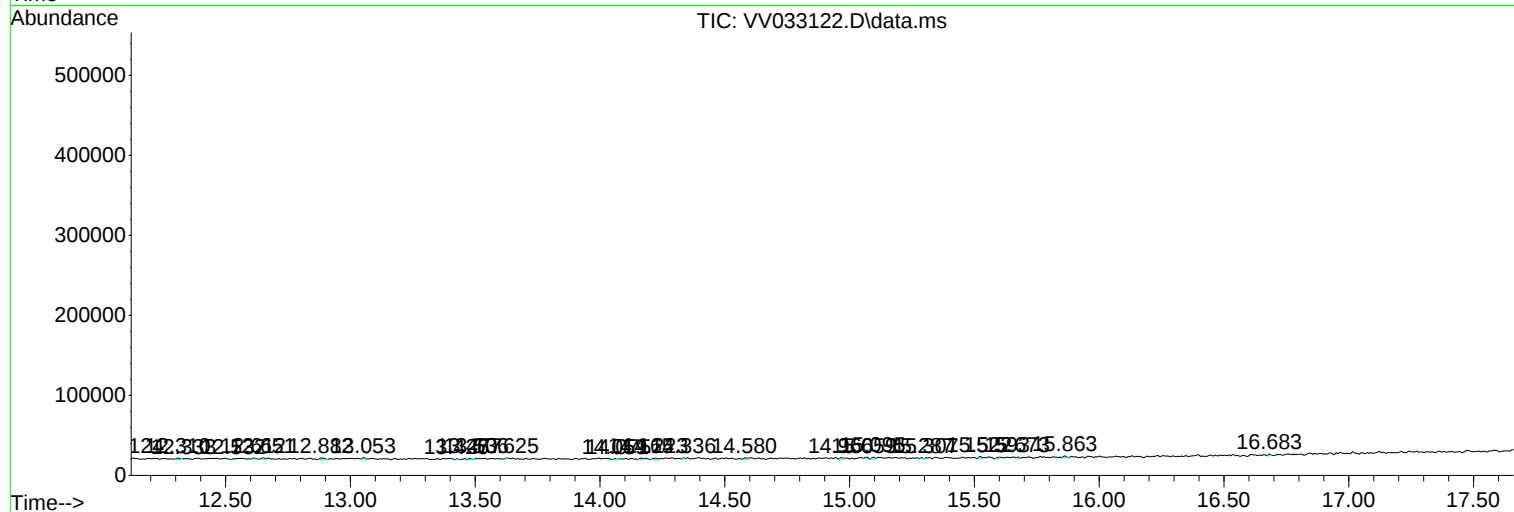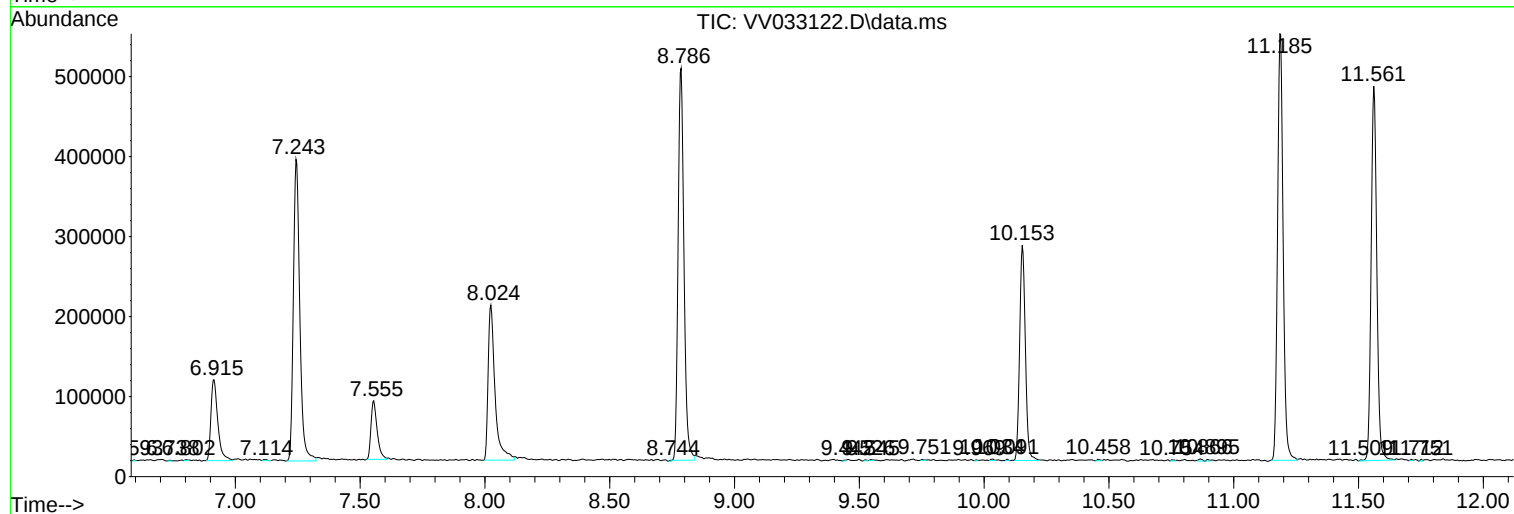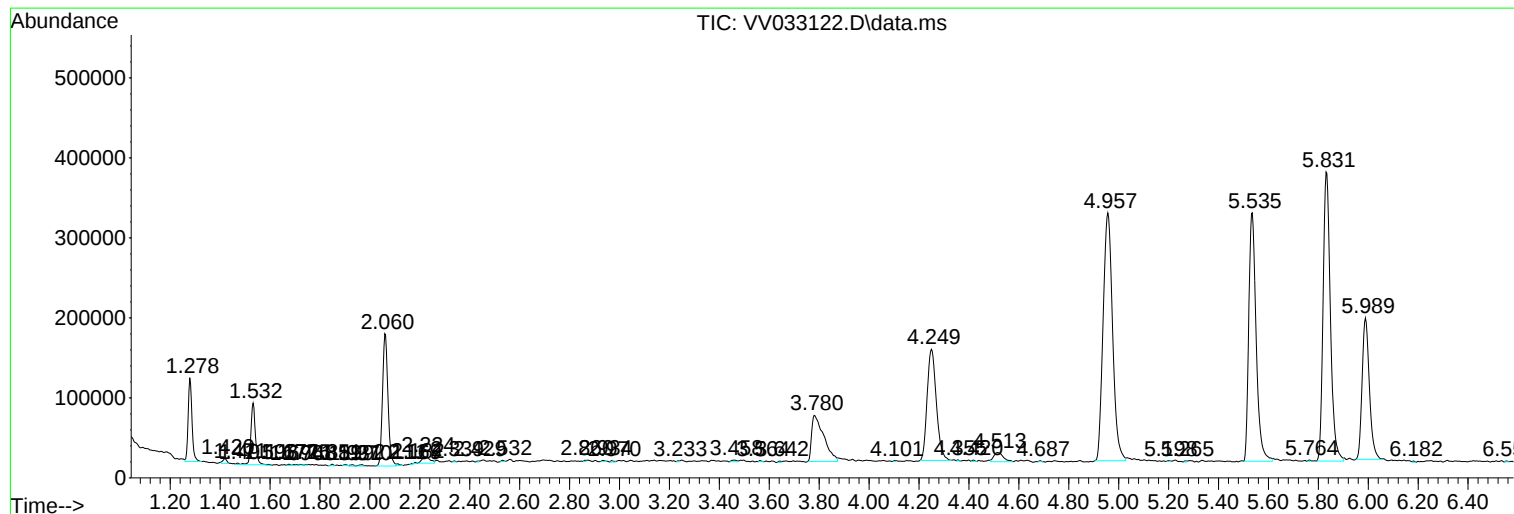

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033122.D
Acq On : 06 Dec 2023 17:26
Operator : SY/MD
Sample : 05644-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033122.D
Acq On : 06 Dec 2023 17:26
Operator : SY/MD
Sample : 05644-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------