

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033123.D
 Acq On : 06 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05644-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	103547	110800	13.18%	1.549%
2	1.420	111	118	127	rVB3	5882	8295	0.99%	0.116%
3	1.468	131	133	139	rVV3	1532	1381	0.16%	0.019%
4	1.497	139	142	145	rVV	1464	1143	0.14%	0.016%
5	1.532	145	153	170	rVB	77716	95492	11.36%	1.335%
6	1.600	170	174	179	rBV2	1259	1373	0.16%	0.019%
7	1.658	190	192	196	rVB	1043	651	0.08%	0.009%
8	1.680	196	199	200	rBV2	893	593	0.07%	0.008%
9	1.725	211	213	217	rVB	932	528	0.06%	0.007%
10	1.757	217	223	225	rBV2	1143	1337	0.16%	0.019%
11	1.783	229	231	233	rVB3	447	144	0.02%	0.002%
12	1.819	239	242	244	rVB2	811	381	0.05%	0.005%
13	1.847	244	251	254	rBV2	1224	1616	0.19%	0.023%
14	1.886	259	263	266	rBV2	938	607	0.07%	0.008%
15	1.899	266	267	271	rVB2	499	328	0.04%	0.005%
16	1.921	271	274	279	rVB2	1479	1444	0.17%	0.020%
17	1.947	279	282	284	rBV	427	226	0.03%	0.003%
18	1.963	284	287	288	rBV	504	263	0.03%	0.004%
19	1.979	288	292	295	rVB2	1388	1217	0.14%	0.017%
20	1.999	295	298	300	rBV2	668	478	0.06%	0.007%
21	2.015	300	303	306	rBV	1316	896	0.11%	0.013%
22	2.060	306	317	335	rBV2	170947	264026	31.40%	3.690%
23	2.124	335	337	339	rVB2	358	181	0.02%	0.003%
24	2.166	339	350	354	rBV	2891	5277	0.63%	0.074%
25	2.188	354	357	359	rBV	1130	710	0.08%	0.010%
26	2.407	422	425	428	rBV	1730	1201	0.14%	0.017%
27	2.976	599	602	606	rBV	1546	1088	0.13%	0.015%
28	3.124	646	648	651	rBV3	1291	751	0.09%	0.010%
29	3.378	724	727	729	rBV	1445	861	0.10%	0.012%
30	3.519	768	771	773	rBV	1495	1047	0.12%	0.015%
31	3.780	844	852	881	rBV	56959	183846	21.87%	2.569%
32	4.002	918	921	926	rVB	1767	1233	0.15%	0.017%
33	4.249	984	998	1021	rBV2	139766	356918	42.45%	4.988%
34	4.513	1069	1080	1084	rBV6	4809	9360	1.11%	0.131%
35	4.770	1156	1160	1163	rBV	1785	1638	0.19%	0.023%
36	4.957	1202	1218	1250	rBV2	316510	840795	100.00%	11.751%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033123.D
 Acq On : 06 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05644-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1423	rBV	307519	634418	75.45%	8.867%
38	5.728	1455	1458	1462	rBV3	1386	1307	0.16%	0.018%
39	5.838	1483	1492	1508	rVB7	17420	42219	5.02%	0.590%
40	5.989	1527	1539	1567	rBV	176471	366778	43.62%	5.126%
41	6.198	1600	1604	1607	rVB	2264	1879	0.22%	0.026%
42	6.224	1608	1612	1620	rBV	1957	2948	0.35%	0.041%
43	6.770	1780	1782	1785	rBV2	1201	769	0.09%	0.011%
44	6.799	1789	1791	1794	rBV	1048	516	0.06%	0.007%
45	6.915	1817	1827	1845	rBV2	101600	190443	22.65%	2.662%
46	7.156	1899	1902	1910	rBV	1462	2367	0.28%	0.033%
47	7.243	1918	1929	1950	rBV	378215	669676	79.65%	9.359%
48	7.555	2017	2026	2040	rBV	73873	131013	15.58%	1.831%
49	8.024	2162	2172	2203	rBV	204541	385866	45.89%	5.393%
50	8.281	2250	2252	2258	rVB	1612	1266	0.15%	0.018%
51	8.703	2378	2383	2388	rVB	1664	2196	0.26%	0.031%
52	8.738	2389	2394	2397	rBV	2313	2523	0.30%	0.035%
53	8.786	2398	2409	2430	rBV	487603	799001	95.03%	11.167%
54	9.101	2504	2507	2510	rBV2	1213	937	0.11%	0.013%
55	9.410	2601	2603	2607	rVB	2098	1140	0.14%	0.016%
56	9.686	2686	2689	2692	rBV	1393	819	0.10%	0.011%
57	10.069	2805	2808	2811	rBV	1737	1328	0.16%	0.019%
58	10.153	2823	2834	2848	rBV	279654	437030	51.98%	6.108%
59	10.291	2874	2877	2882	rBV2	1414	1074	0.13%	0.015%
60	10.873	3056	3058	3061	rVB	1594	878	0.10%	0.012%
61	10.892	3061	3064	3066	rBV3	1003	662	0.08%	0.009%
62	11.185	3145	3155	3178	rBV	520998	815252	96.96%	11.394%
63	11.561	3261	3272	3288	rBV	467738	734444	87.35%	10.265%
64	11.702	3312	3316	3319	rBV	1794	1440	0.17%	0.020%
65	12.468	3551	3554	3556	rBV	1533	986	0.12%	0.014%
66	12.503	3562	3565	3570	rBV	1318	1351	0.16%	0.019%
67	12.815	3659	3662	3664	rBV4	1190	777	0.09%	0.011%
68	13.101	3749	3751	3756	rBV	1330	904	0.11%	0.013%
69	13.152	3765	3767	3772	rBV	1540	1270	0.15%	0.018%
70	13.416	3846	3849	3856	rVB	2257	2252	0.27%	0.031%
71	13.452	3856	3860	3863	rBV	2760	2501	0.30%	0.035%
72	13.577	3897	3899	3901	rBV	1314	717	0.09%	0.010%
73	13.686	3930	3933	3935	rBV	1859	1383	0.16%	0.019%
74	14.037	4039	4042	4047	rBV	1681	1637	0.19%	0.023%
75	14.095	4057	4060	4066	rBV4	1578	1845	0.22%	0.026%
76	14.201	4088	4093	4094	rBV2	1221	1172	0.14%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033123.D
Acq On : 06 Dec 2023 17:49
Operator : SY/MD
Sample : 05644-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

77	14.265	4110	4113	4116	rBV2	1567	1190	0.14%	0.017%
78	14.632	4223	4227	4228	rBV	1592	1147	0.14%	0.016%
79	14.670	4236	4239	4243	rBV	1886	1511	0.18%	0.021%
80	14.750	4261	4264	4269	rBV	1583	1564	0.19%	0.022%
81	15.033	4350	4352	4355	rBV3	1300	787	0.09%	0.011%
82	15.297	4432	4434	4436	rVB	1879	795	0.09%	0.011%
83	16.136	4692	4695	4697	rBV3	1722	1192	0.14%	0.017%
84	16.262	4731	4734	4737	rBV2	2149	1869	0.22%	0.026%


Sum of corrected areas: 7155164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033123.D
Acq On : 06 Dec 2023 17:49
Operator : SY/MD
Sample : 05644-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

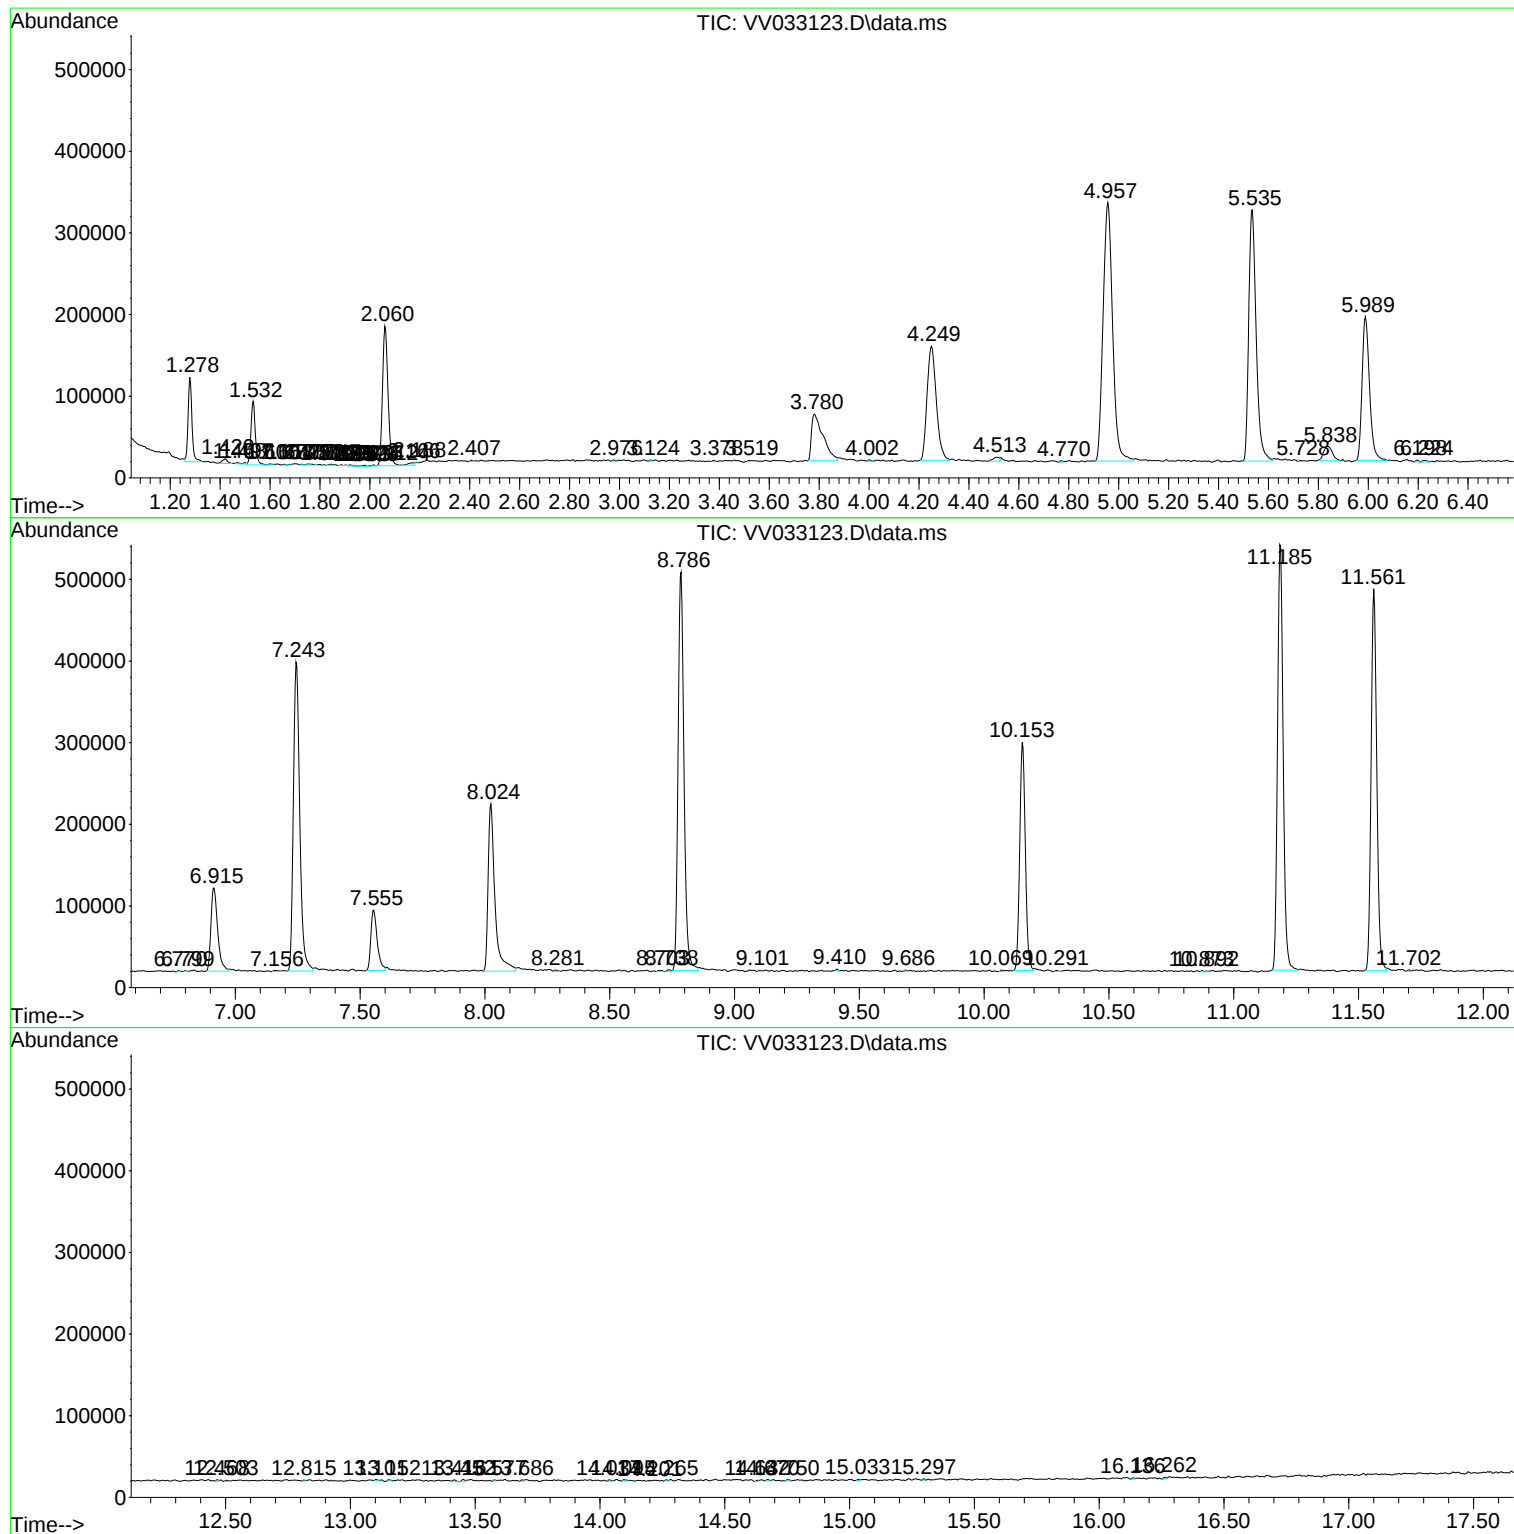

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033123.D
Acq On : 06 Dec 2023 17:49
Operator : SY/MD
Sample : 05644-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033123.D
Acq On : 06 Dec 2023 17:49
Operator : SY/MD
Sample : 05644-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------