

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033124.D
 Acq On : 06 Dec 2023 18:13
 Operator : SY/MD
 Sample : 05644-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	102884	108673	12.90%	1.533%
2	1.346	93	95	97	rBV	833	520	0.06%	0.007%
3	1.416	113	117	124	rVB2	6264	5951	0.71%	0.084%
4	1.461	129	131	133	rBV2	755	453	0.05%	0.006%
5	1.487	137	139	142	rVB2	785	417	0.05%	0.006%
6	1.532	144	153	165	rVB	76605	91124	10.82%	1.286%
7	1.632	181	184	187	rVV	939	749	0.09%	0.011%
8	1.648	187	189	191	rVV	667	382	0.05%	0.005%
9	1.670	193	196	200	rVB3	1287	1068	0.13%	0.015%
10	1.706	204	207	212	rBV	1209	1459	0.17%	0.021%
11	1.757	218	223	226	rBV3	1316	1094	0.13%	0.015%
12	1.777	226	229	233	rVB2	923	519	0.06%	0.007%
13	1.805	233	238	241	rBV	1510	1474	0.18%	0.021%
14	1.822	241	243	245	rVV	696	374	0.04%	0.005%
15	1.850	249	252	255	rBV3	736	624	0.07%	0.009%
16	1.924	271	275	278	rBV2	1575	1153	0.14%	0.016%
17	1.960	283	286	292	rVB4	958	957	0.11%	0.014%
18	1.989	292	295	296	rBV4	373	227	0.03%	0.003%
19	2.005	296	300	303	rVB4	829	720	0.09%	0.010%
20	2.024	303	306	307	rBV	657	323	0.04%	0.005%
21	2.059	307	317	334	rBV	159556	234745	27.87%	3.312%
22	2.162	342	349	350	rBV	2505	2481	0.29%	0.035%
23	2.175	351	353	357	rVV2	1531	1378	0.16%	0.019%
24	2.198	357	360	362	rVV	1486	1071	0.13%	0.015%
25	2.211	362	364	367	rVB2	886	553	0.07%	0.008%
26	2.233	368	371	373	rBV2	1643	1171	0.14%	0.017%
27	2.542	464	467	470	rBV2	1697	1205	0.14%	0.017%
28	2.561	471	473	477	rVB	1598	1142	0.14%	0.016%
29	2.822	551	554	555	rBV	1771	1010	0.12%	0.014%
30	2.950	589	594	603	rBV	1629	3261	0.39%	0.046%
31	3.153	654	657	662	rVB	2466	1740	0.21%	0.025%
32	3.333	710	713	715	rBV	1439	794	0.09%	0.011%
33	3.526	771	773	777	rBV	1470	856	0.10%	0.012%
34	3.661	812	815	824	rVB	2589	3015	0.36%	0.043%
35	3.699	824	827	830	rBV	1822	1467	0.17%	0.021%
36	3.783	844	853	877	rBV	54736	145916	17.33%	2.059%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033124.D
 Acq On : 06 Dec 2023 18:13
 Operator : SY/MD
 Sample : 05644-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.249	984	998	1024	rVB	139377	356767	42.36%	5.034%
38	4.503	1073	1077	1079	rBV	2011	1545	0.18%	0.022%
39	4.783	1161	1164	1167	rBV2	1589	1358	0.16%	0.019%
40	4.956	1202	1218	1242	rBV3	313243	829150	98.46%	11.699%
41	5.162	1280	1282	1284	rBV	1366	846	0.10%	0.012%
42	5.368	1343	1346	1350	rVB	1632	1177	0.14%	0.017%
43	5.535	1386	1398	1426	rBV	313420	645047	76.60%	9.101%
44	5.744	1459	1463	1466	rBV	1804	1622	0.19%	0.023%
45	5.783	1472	1475	1478	rVB	1883	1166	0.14%	0.016%
46	5.837	1479	1492	1506	rVV7	20958	51423	6.11%	0.726%
47	5.989	1527	1539	1567	rBV	177833	367490	43.64%	5.185%
48	6.140	1583	1586	1589	rBV3	1525	1033	0.12%	0.015%
49	6.522	1703	1705	1708	rVB	1095	544	0.06%	0.008%
50	6.699	1757	1760	1763	rBV	1310	828	0.10%	0.012%
51	6.715	1763	1765	1766	rBV	1058	468	0.06%	0.007%
52	6.915	1817	1827	1846	rBV	100268	185987	22.09%	2.624%
53	7.243	1919	1929	1954	rBV	374406	663723	78.81%	9.365%
54	7.461	1994	1997	1999	rBV3	1467	993	0.12%	0.014%
55	7.554	2017	2026	2045	rBV2	73213	131069	15.56%	1.849%
56	7.828	2108	2111	2114	rBV	1365	1042	0.12%	0.015%
57	7.870	2120	2124	2127	rBV3	1400	1546	0.18%	0.022%
58	8.024	2163	2172	2202	rBV	201971	369992	43.93%	5.220%
59	8.786	2398	2409	2433	rBV	504355	816782	96.99%	11.524%
60	9.011	2476	2479	2481	rBV2	1050	725	0.09%	0.010%
61	9.162	2523	2526	2528	rBV	1333	885	0.11%	0.012%
62	9.271	2557	2560	2563	rBV2	1824	1353	0.16%	0.019%
63	9.400	2597	2600	2601	rBV	1209	646	0.08%	0.009%
64	9.461	2617	2619	2629	rVB3	1233	1611	0.19%	0.023%
65	9.770	2713	2715	2719	rVB	1566	985	0.12%	0.014%
66	9.847	2737	2739	2743	rBV	1082	889	0.11%	0.013%
67	9.963	2773	2775	2777	rBV	1188	521	0.06%	0.007%
68	10.011	2786	2790	2792	rBV	1596	1376	0.16%	0.019%
69	10.095	2814	2816	2819	rVB	1449	682	0.08%	0.010%
70	10.152	2824	2834	2850	rVV2	270219	427783	50.80%	6.036%
71	10.326	2884	2888	2893	rBV2	2145	2419	0.29%	0.034%
72	10.496	2939	2941	2944	rBV	1293	978	0.12%	0.014%
73	10.876	3057	3059	3061	rBV	1041	659	0.08%	0.009%
74	10.921	3070	3073	3076	rBV	1150	950	0.11%	0.013%
75	11.040	3104	3110	3115	rBV	1760	2433	0.29%	0.034%
76	11.188	3145	3156	3176	rBV	540081	842139	100.00%	11.882%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033124.D
 Acq On : 06 Dec 2023 18:13
 Operator : SY/MD
 Sample : 05644-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.493	3248	3251	3253	rBV	1271	974	0.12%	0.014%
78	11.561	3262	3272	3288	rBV	474878	725129	86.11%	10.231%
79	11.728	3321	3324	3326	rBV2	1711	1041	0.12%	0.015%
80	11.873	3367	3369	3374	rBV	1450	1363	0.16%	0.019%
81	12.066	3426	3429	3432	rBV	1127	864	0.10%	0.012%
82	12.303	3499	3503	3509	rBV	2029	2770	0.33%	0.039%
83	12.850	3670	3673	3676	rVB	1426	837	0.10%	0.012%
84	12.898	3685	3688	3690	rBV	1035	716	0.09%	0.010%
85	12.940	3698	3701	3703	rBV	1371	929	0.11%	0.013%
86	13.265	3797	3802	3805	rBV	1521	1453	0.17%	0.021%
87	13.410	3845	3847	3848	rBV	916	397	0.05%	0.006%
88	13.461	3861	3863	3866	rBV2	1290	810	0.10%	0.011%
89	13.795	3964	3967	3968	rBV	1273	770	0.09%	0.011%
90	13.879	3990	3993	3995	rBV2	1165	681	0.08%	0.010%
91	14.017	4034	4036	4037	rBV	952	437	0.05%	0.006%
92	14.200	4091	4093	4095	rBV	1298	827	0.10%	0.012%
93	14.265	4111	4113	4114	rBV	1239	617	0.07%	0.009%
94	14.776	4267	4272	4276	rBV	1791	2123	0.25%	0.030%
95	14.911	4311	4314	4315	rBV3	1139	643	0.08%	0.009%
96	15.036	4351	4353	4357	rVB	1324	735	0.09%	0.010%
97	15.059	4357	4360	4362	rBV	1491	1066	0.13%	0.015%
98	15.136	4381	4384	4386	rBV	1391	994	0.12%	0.014%
99	15.364	4452	4455	4459	rBV	2019	1557	0.18%	0.022%
100	15.953	4635	4638	4640	rBV	1805	1001	0.12%	0.014%




Sum of corrected areas: 7087432

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033124.D
Acq On : 06 Dec 2023 18:13
Operator : SY/MD
Sample : 05644-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

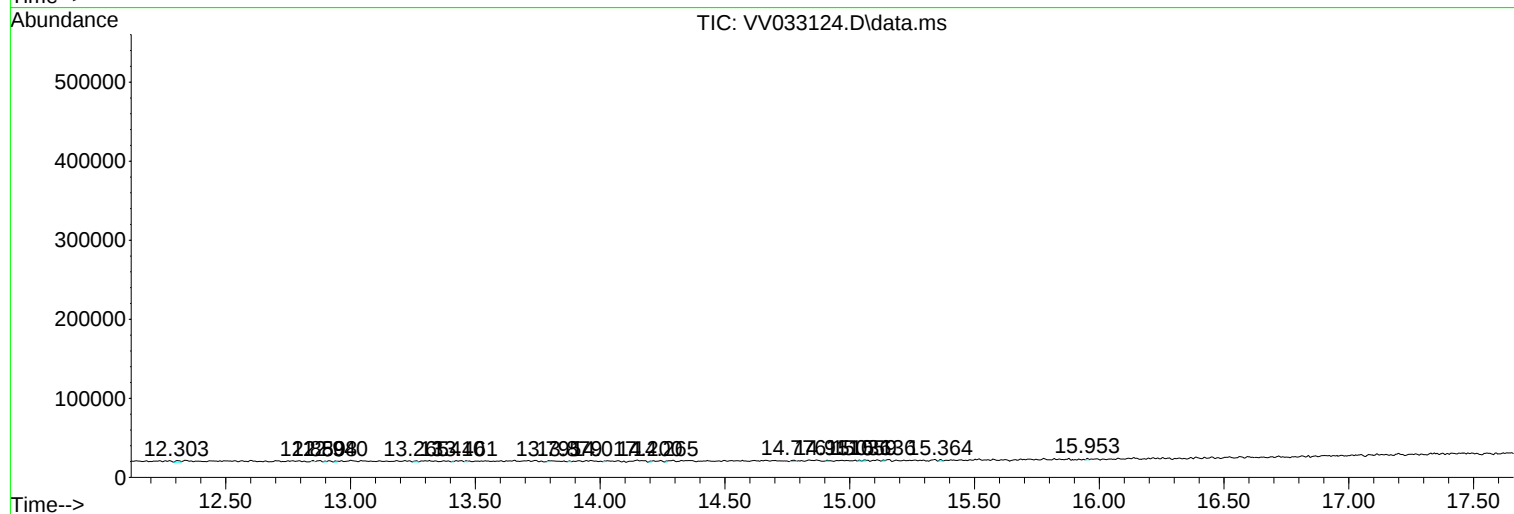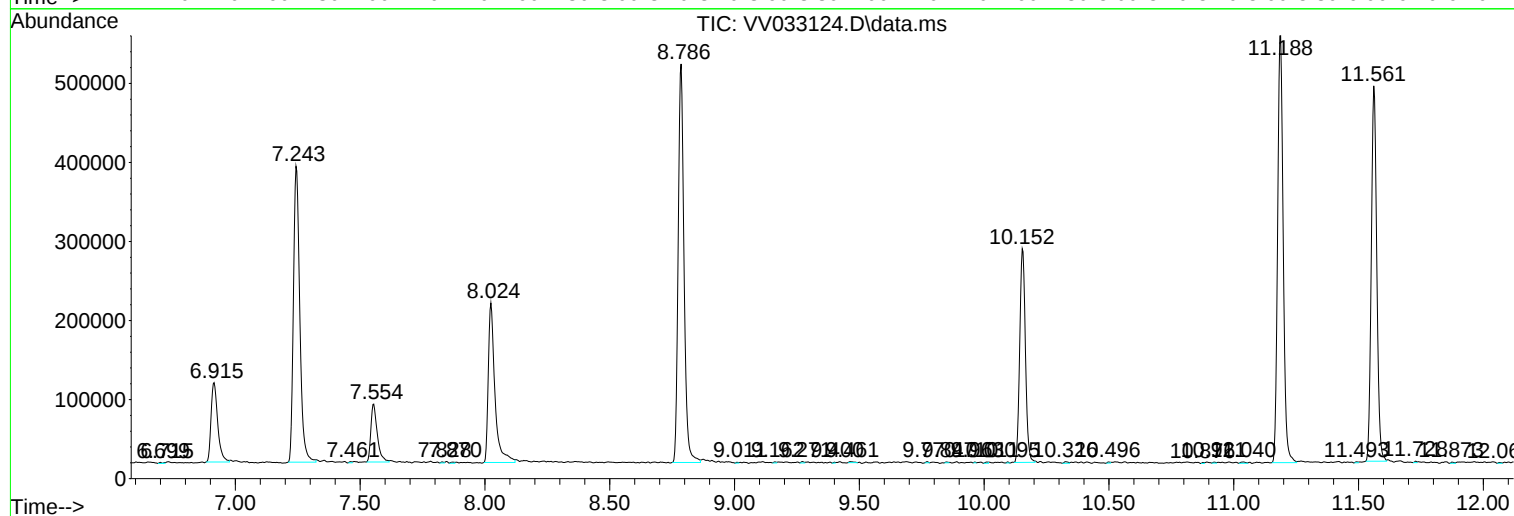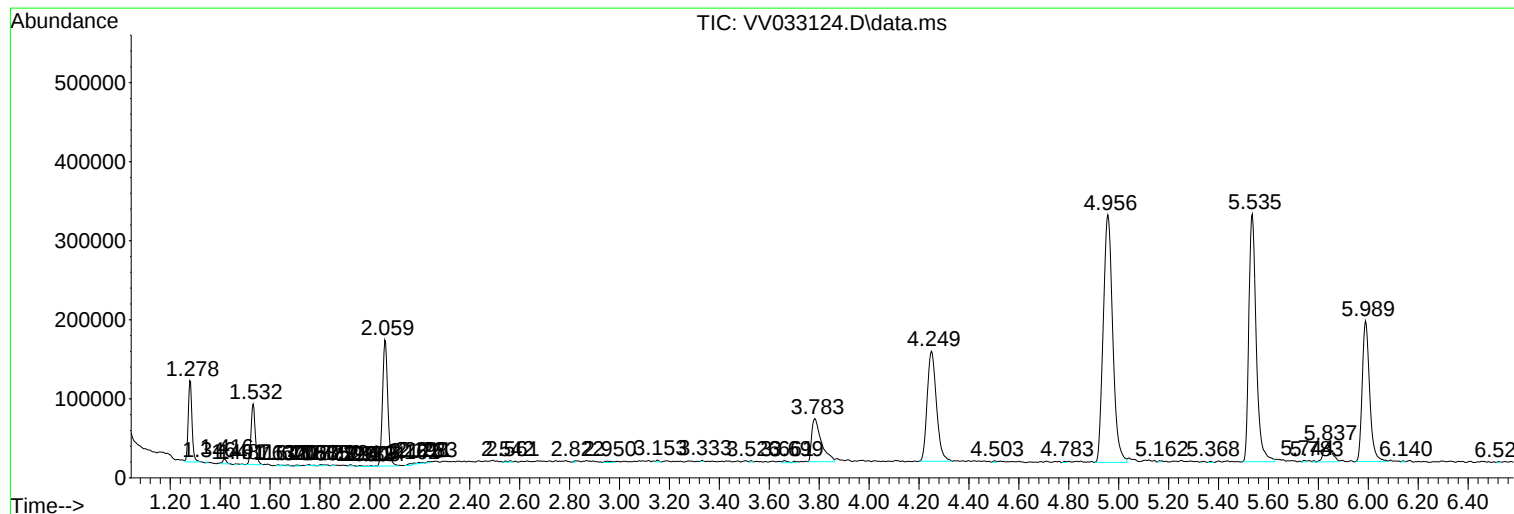

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033124.D
Acq On : 06 Dec 2023 18:13
Operator : SY/MD
Sample : 05644-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033124.D
Acq On : 06 Dec 2023 18:13
Operator : SY/MD
Sample : 05644-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G54

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------