

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033126.D
 Acq On : 06 Dec 2023 18:59
 Operator : SY/MD
 Sample : 05644-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	99543	102721	12.56%	1.479%
2	1.417	111	117	123	rBV3	4723	5424	0.66%	0.078%
3	1.487	135	139	141	rBV2	1548	1247	0.15%	0.018%
4	1.532	146	153	169	rVB	77966	93468	11.43%	1.346%
5	1.632	179	184	192	rVB4	1227	1624	0.20%	0.023%
6	1.664	192	194	199	rVB	1309	996	0.12%	0.014%
7	1.700	199	205	210	rBV3	2002	2850	0.35%	0.041%
8	1.732	213	215	218	rBV2	993	687	0.08%	0.010%
9	1.786	229	232	233	rBV	357	147	0.02%	0.002%
10	1.802	233	237	238	rVV	919	553	0.07%	0.008%
11	1.812	238	240	242	rVV2	1018	588	0.07%	0.008%
12	1.828	242	245	247	rVV3	1171	789	0.10%	0.011%
13	1.844	247	250	253	rVV2	890	692	0.08%	0.010%
14	1.864	253	256	259	rVV2	1120	998	0.12%	0.014%
15	1.883	259	262	265	rVV2	1763	1282	0.16%	0.018%
16	1.902	266	268	270	rVV2	913	479	0.06%	0.007%
17	1.928	273	276	279	rVB2	1447	968	0.12%	0.014%
18	1.944	279	281	284	rBV3	581	333	0.04%	0.005%
19	1.960	284	286	294	rVB2	1250	1274	0.16%	0.018%
20	2.005	294	300	304	rBV	1345	1701	0.21%	0.024%
21	2.024	304	306	307	rBV	146	52	0.01%	0.001%
22	2.060	307	317	328	rBV	155737	227109	27.76%	3.270%
23	2.111	328	333	342	rVB3	6317	9344	1.14%	0.135%
24	2.220	361	367	374	rBV2	5426	8573	1.05%	0.123%
25	2.323	397	399	401	rBV3	1266	746	0.09%	0.011%
26	2.397	419	422	425	rVB	1360	924	0.11%	0.013%
27	2.835	554	558	564	rBV	1542	2147	0.26%	0.031%
28	3.510	765	768	772	rBV	1763	1599	0.20%	0.023%
29	3.613	796	800	803	rBV	1703	1437	0.18%	0.021%
30	3.783	844	853	875	rBV	52229	136606	16.70%	1.967%
31	4.050	934	936	938	rBV	1477	947	0.12%	0.014%
32	4.249	983	998	1024	rBV	136988	355169	43.42%	5.114%
33	4.616	1110	1112	1115	rBV	990	517	0.06%	0.007%
34	4.957	1202	1218	1251	rBV2	304565	814290	99.55%	11.724%
35	5.298	1321	1324	1326	rBV	1618	1002	0.12%	0.014%
36	5.423	1360	1363	1368	rBV2	2037	1966	0.24%	0.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033126.D
 Acq On : 06 Dec 2023 18:59
 Operator : SY/MD
 Sample : 05644-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G57

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1426	rBV	306069	631132	77.16%	9.087%
38	5.838	1482	1492	1508	rVB7	15765	37827	4.62%	0.545%
39	5.989	1527	1539	1559	rBV	171902	350922	42.90%	5.053%
40	6.285	1628	1631	1638	rVB	2691	2854	0.35%	0.041%
41	6.314	1638	1640	1641	rBV	996	482	0.06%	0.007%
42	6.732	1768	1770	1775	rVB	1374	910	0.11%	0.013%
43	6.915	1816	1827	1845	rBV2	100051	186307	22.78%	2.683%
44	7.243	1918	1929	1951	rBV	369747	664312	81.21%	9.565%
45	7.555	2016	2026	2050	rBV	72488	137284	16.78%	1.977%
46	7.751	2083	2087	2091	rBV	1778	1601	0.20%	0.023%
47	7.918	2136	2139	2142	rBV	1882	1055	0.13%	0.015%
48	8.024	2163	2172	2199	rBV2	181482	340934	41.68%	4.909%
49	8.664	2368	2371	2374	rBV	1341	1022	0.12%	0.015%
50	8.686	2375	2378	2381	rVB	2104	1444	0.18%	0.021%
51	8.786	2398	2409	2434	rBV	484716	808882	98.89%	11.647%
52	9.156	2521	2524	2526	rBV	1813	1143	0.14%	0.016%
53	9.220	2542	2544	2548	rBV	1396	809	0.10%	0.012%
54	9.432	2606	2610	2612	rBV2	1442	1385	0.17%	0.020%
55	9.799	2721	2724	2726	rBV	1804	1183	0.14%	0.017%
56	9.834	2732	2735	2741	rBV2	1293	1620	0.20%	0.023%
57	10.153	2824	2834	2858	rVB	269171	426348	52.12%	6.139%
58	10.239	2858	2861	2864	rBV	2027	1462	0.18%	0.021%
59	10.493	2938	2940	2943	rBV	1187	604	0.07%	0.009%
60	10.789	3030	3032	3038	rVB	1606	1453	0.18%	0.021%
61	10.902	3064	3067	3073	rBV2	1461	1038	0.13%	0.015%
62	11.108	3127	3131	3132	rBV	1495	1062	0.13%	0.015%
63	11.185	3145	3155	3173	rBV	540678	817997	100.00%	11.778%
64	11.432	3229	3232	3234	rBV	1428	787	0.10%	0.011%
65	11.561	3261	3272	3289	rBV	459757	715746	87.50%	10.306%
66	11.857	3360	3364	3368	rBV2	1676	1566	0.19%	0.023%
67	12.104	3438	3441	3445	rBV	1410	1179	0.14%	0.017%
68	12.181	3462	3465	3468	rBV	2003	1436	0.18%	0.021%
69	12.326	3507	3510	3513	rBV	1962	1191	0.15%	0.017%
70	12.458	3548	3551	3556	rBV	1626	1403	0.17%	0.020%
71	13.802	3966	3969	3973	rVB	1694	1070	0.13%	0.015%
72	14.349	4131	4139	4148	rVB9	6246	10887	1.33%	0.157%
73	14.953	4325	4327	4330	rBV	1506	866	0.11%	0.012%
74	15.062	4357	4361	4365	rBV	2196	2111	0.26%	0.030%
75	15.098	4370	4372	4376	rVB	1674	1190	0.15%	0.017%
76	15.419	4470	4472	4477	rVB	1637	1473	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033126.D
Acq On : 06 Dec 2023 18:59
Operator : SY/MD
Sample : 05644-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G57

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis




Sum of corrected areas: 6945226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033126.D
Acq On : 06 Dec 2023 18:59
Operator : SY/MD
Sample : 05644-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

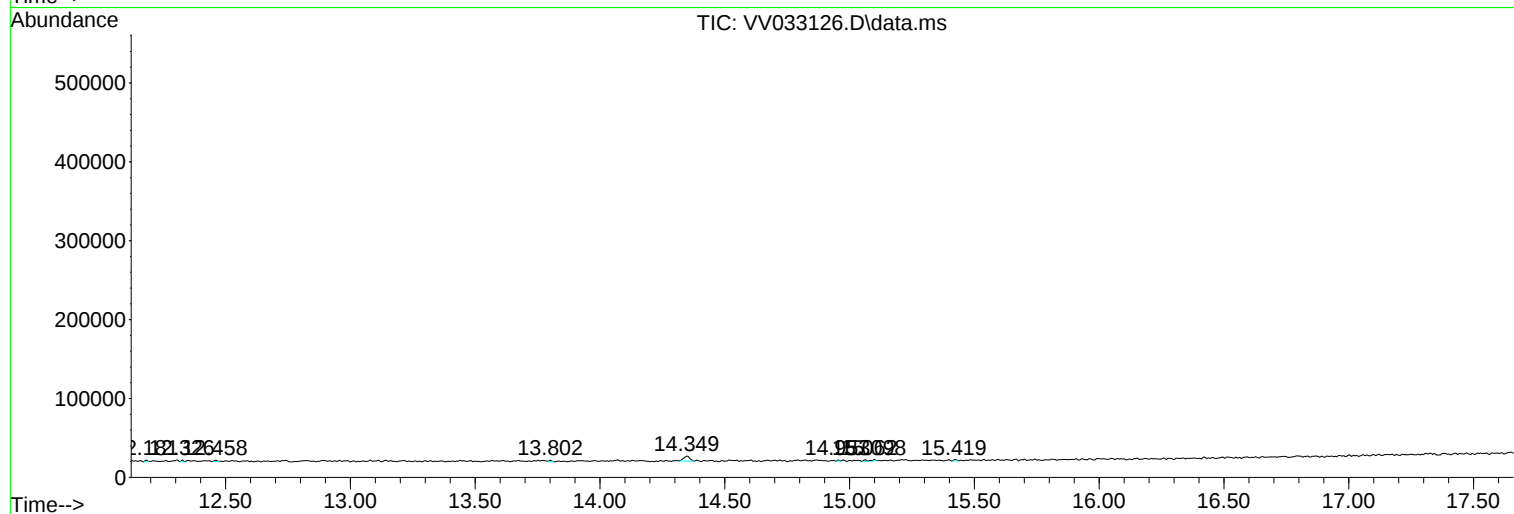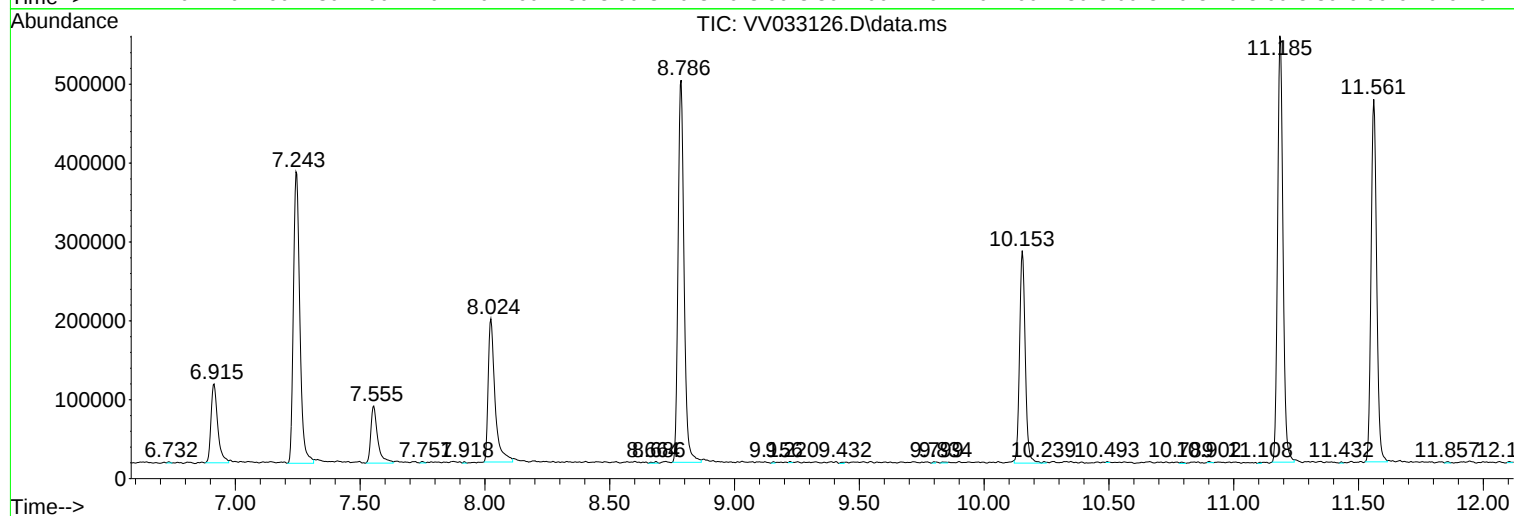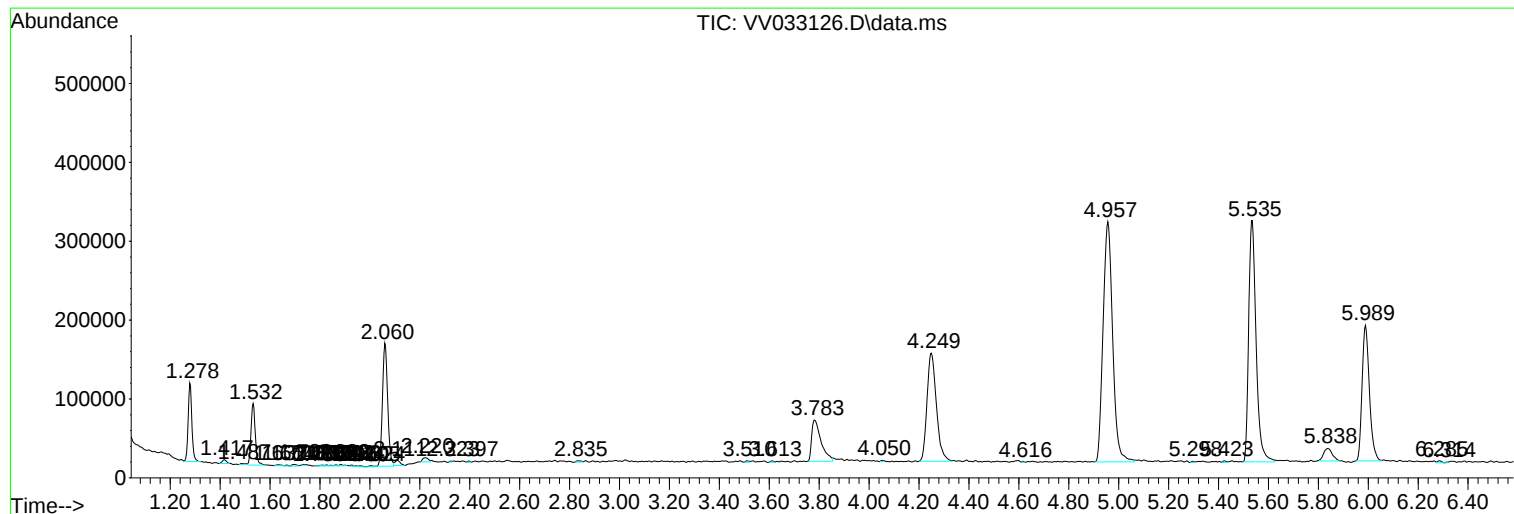

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033126.D
Acq On : 06 Dec 2023 18:59
Operator : SY/MD
Sample : 05644-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033126.D
Acq On : 06 Dec 2023 18:59
Operator : SY/MD
Sample : 05644-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G57

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------