

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033127.D
 Acq On : 06 Dec 2023 19:22
 Operator : SY/MD
 Sample : 05644-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	98714	109751	13.06%	1.569%
2	1.342	92	94	100	rVB2	1701	1374	0.16%	0.020%
3	1.416	111	117	126	rVB2	6985	10155	1.21%	0.145%
4	1.455	126	129	132	rBV2	1263	695	0.08%	0.010%
5	1.532	145	153	171	rVB	73116	90699	10.80%	1.297%
6	1.625	180	182	185	rVB2	746	403	0.05%	0.006%
7	1.651	188	190	193	rVB	1080	653	0.08%	0.009%
8	1.674	193	197	202	rBV2	1448	1343	0.16%	0.019%
9	1.696	202	204	206	rBV2	446	150	0.02%	0.002%
10	1.709	206	208	210	rVB	772	322	0.04%	0.005%
11	1.741	213	218	223	rVB	1289	1359	0.16%	0.019%
12	1.770	223	227	232	rVB3	1138	1006	0.12%	0.014%
13	1.818	236	242	243	rBV2	991	833	0.10%	0.012%
14	1.828	243	245	248	rBV3	389	202	0.02%	0.003%
15	1.844	248	250	253	rVB2	858	451	0.05%	0.006%
16	1.860	253	255	256	rVB2	351	127	0.02%	0.002%
17	1.876	256	260	263	rBV	1373	1156	0.14%	0.017%
18	1.924	269	275	280	rVB2	1315	1683	0.20%	0.024%
19	1.947	280	282	285	rBV	281	147	0.02%	0.002%
20	1.969	285	289	294	rVB3	1388	1252	0.15%	0.018%
21	2.002	294	299	303	rBV	1453	1709	0.20%	0.024%
22	2.059	304	317	331	rBV	154678	225942	26.90%	3.230%
23	2.114	331	334	339	rVB3	1831	1394	0.17%	0.020%
24	2.182	339	355	356	rBV3	4025	8150	0.97%	0.117%
25	2.211	362	364	365	rBV	1125	548	0.07%	0.008%
26	2.326	397	400	402	rBV	1331	815	0.10%	0.012%
27	2.580	476	479	485	rBV2	2065	1792	0.21%	0.026%
28	2.867	565	568	574	rBV	1990	2090	0.25%	0.030%
29	3.130	644	650	653	rBV2	1589	1808	0.22%	0.026%
30	3.246	683	686	690	rBV	1414	1143	0.14%	0.016%
31	3.442	744	747	751	rBV	1404	1181	0.14%	0.017%
32	3.484	758	760	763	rBV	1233	614	0.07%	0.009%
33	3.635	804	807	809	rBV	1402	846	0.10%	0.012%
34	3.780	844	852	874	rBV	51574	135374	16.11%	1.936%
35	4.249	984	998	1020	rBV	137397	348331	41.46%	4.980%
36	4.503	1074	1077	1081	rBV	1346	945	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033127.D
 Acq On : 06 Dec 2023 19:22
 Operator : SY/MD
 Sample : 05644-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.571	1095	1098	1100	rBV	1503	1050	0.12%	0.015%
38	4.625	1112	1115	1118	rBV	1803	1423	0.17%	0.020%
39	4.899	1197	1200	1202	rBV	2302	1549	0.18%	0.022%
40	4.956	1202	1218	1243	rVV2	306904	819949	97.60%	11.723%
41	5.137	1271	1274	1275	rBV	1119	680	0.08%	0.010%
42	5.239	1303	1306	1308	rBV	1050	664	0.08%	0.009%
43	5.429	1363	1365	1368	rBV2	1176	631	0.08%	0.009%
44	5.448	1368	1371	1375	rVB	1457	932	0.11%	0.013%
45	5.535	1386	1398	1419	rBV	316346	647575	77.09%	9.259%
46	5.825	1480	1488	1502	rBV7	8604	21272	2.53%	0.304%
47	5.944	1522	1525	1527	rBV	1814	952	0.11%	0.014%
48	5.989	1527	1539	1560	rVV	172519	359716	42.82%	5.143%
49	6.275	1626	1628	1635	rVB	2029	1394	0.17%	0.020%
50	6.365	1653	1656	1660	rBV2	1109	977	0.12%	0.014%
51	6.387	1661	1663	1665	rBV	1011	655	0.08%	0.009%
52	6.558	1713	1716	1722	rBV	1310	1299	0.15%	0.019%
53	6.699	1758	1760	1765	rVB	2314	1715	0.20%	0.025%
54	6.863	1806	1811	1814	rBV2	1716	1765	0.21%	0.025%
55	6.915	1817	1827	1848	rVV	99831	187465	22.32%	2.680%
56	7.091	1880	1882	1884	rBV2	1041	580	0.07%	0.008%
57	7.188	1910	1912	1918	rBV	1431	1209	0.14%	0.017%
58	7.243	1918	1929	1951	rBV	367178	650705	77.46%	9.303%
59	7.554	2016	2026	2043	rBV2	71102	130975	15.59%	1.873%
60	7.776	2092	2095	2099	rBV	2307	2044	0.24%	0.029%
61	8.024	2163	2172	2197	rBV	189337	350632	41.74%	5.013%
62	8.349	2269	2273	2275	rBV3	2075	1815	0.22%	0.026%
63	8.786	2398	2409	2428	rBV	504163	823215	97.99%	11.770%
64	9.140	2516	2519	2521	rBV	1385	984	0.12%	0.014%
65	9.423	2604	2607	2610	rBV	1399	1247	0.15%	0.018%
66	9.593	2657	2660	2663	rVB	1204	713	0.08%	0.010%
67	9.879	2746	2749	2755	rVB	2661	2190	0.26%	0.031%
68	9.966	2773	2776	2780	rVB	1971	1470	0.17%	0.021%
69	9.988	2780	2783	2786	rBV	2406	1865	0.22%	0.027%
70	10.152	2823	2834	2853	rBV	264389	419904	49.98%	6.004%
71	10.406	2908	2913	2917	rBV	1809	1963	0.23%	0.028%
72	10.535	2950	2953	2955	rBV2	1465	1155	0.14%	0.017%
73	10.741	3014	3017	3020	rBV	1727	1371	0.16%	0.020%
74	10.840	3045	3048	3049	rBV	1242	775	0.09%	0.011%
75	10.931	3073	3076	3080	rVB	1334	1050	0.12%	0.015%
76	11.185	3145	3155	3172	rBV	538209	840069	100.00%	12.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033127.D
 Acq On : 06 Dec 2023 19:22
 Operator : SY/MD
 Sample : 05644-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.471	3237	3244	3251	rBV	1756	2641	0.31%	0.038%
78	11.561	3261	3272	3296	rBV	462926	720209	85.73%	10.297%
79	11.857	3362	3364	3366	rBV2	1153	672	0.08%	0.010%
80	11.969	3396	3399	3402	rBV	1579	978	0.12%	0.014%
81	12.094	3435	3438	3440	rBV	1549	1215	0.14%	0.017%
82	12.815	3658	3662	3666	rBV	1672	1966	0.23%	0.028%
83	12.995	3716	3718	3722	rBV	1081	751	0.09%	0.011%
84	13.133	3758	3761	3764	rBV	2039	1285	0.15%	0.018%
85	13.178	3770	3775	3778	rBV2	1863	1685	0.20%	0.024%
86	13.509	3875	3878	3881	rBV	1493	1166	0.14%	0.017%
87	13.676	3924	3930	3933	rBV2	1493	1969	0.23%	0.028%
88	13.750	3951	3953	3960	rVB	2012	2346	0.28%	0.034%
89	13.782	3960	3963	3965	rBV3	1506	1047	0.12%	0.015%
90	14.172	4081	4084	4085	rBV	1296	835	0.10%	0.012%
91	14.557	4201	4204	4206	rBV2	1551	983	0.12%	0.014%
92	14.869	4299	4301	4303	rBV2	1283	837	0.10%	0.012%
93	14.985	4335	4337	4339	rVB	1698	753	0.09%	0.011%
94	15.178	4394	4397	4403	rBV2	1769	1719	0.20%	0.025%
95	15.217	4407	4409	4412	rBV	1259	856	0.10%	0.012%
96	15.390	4460	4463	4466	rBV2	1891	1637	0.19%	0.023%
97	15.535	4505	4508	4512	rBV2	1578	1339	0.16%	0.019%
98	15.750	4572	4575	4579	rBV2	1823	1484	0.18%	0.021%
99	15.850	4603	4606	4610	rBV	2377	1795	0.21%	0.026%




Sum of corrected areas: 6994205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033127.D
Acq On : 06 Dec 2023 19:22
Operator : SY/MD
Sample : 05644-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

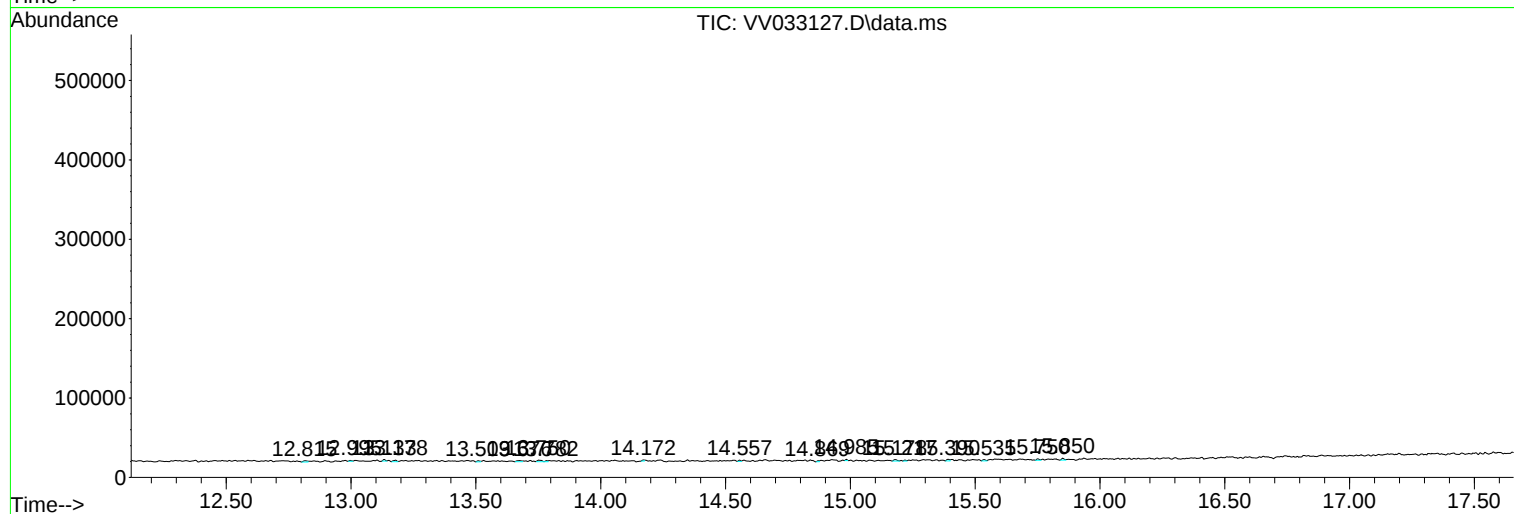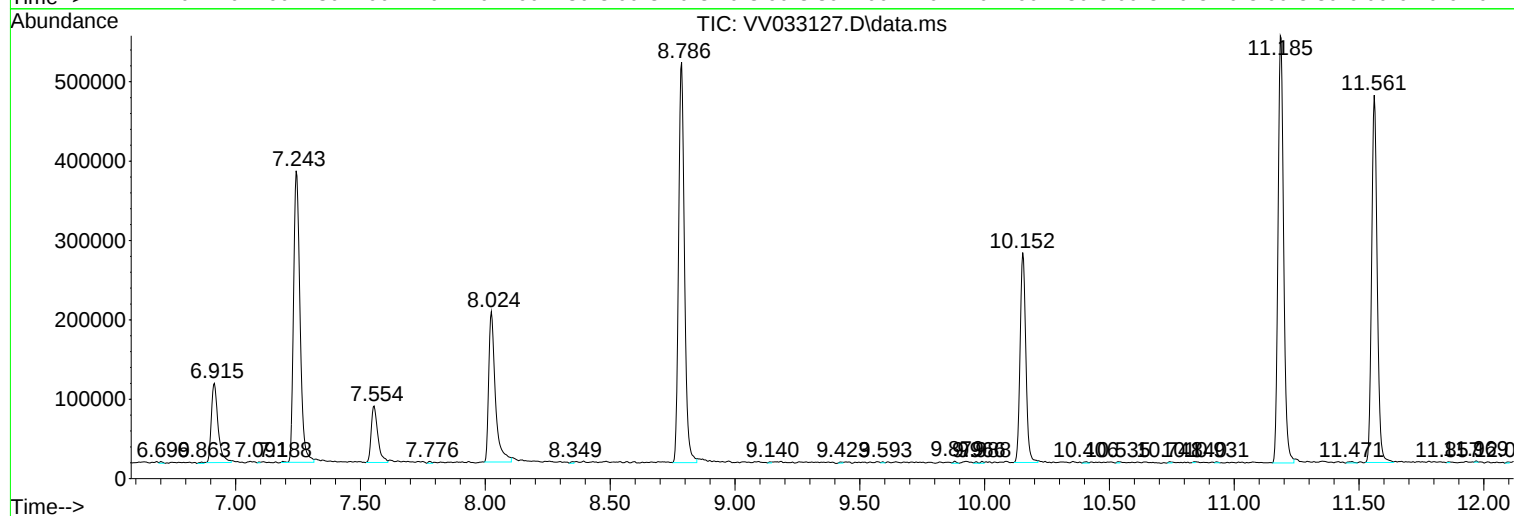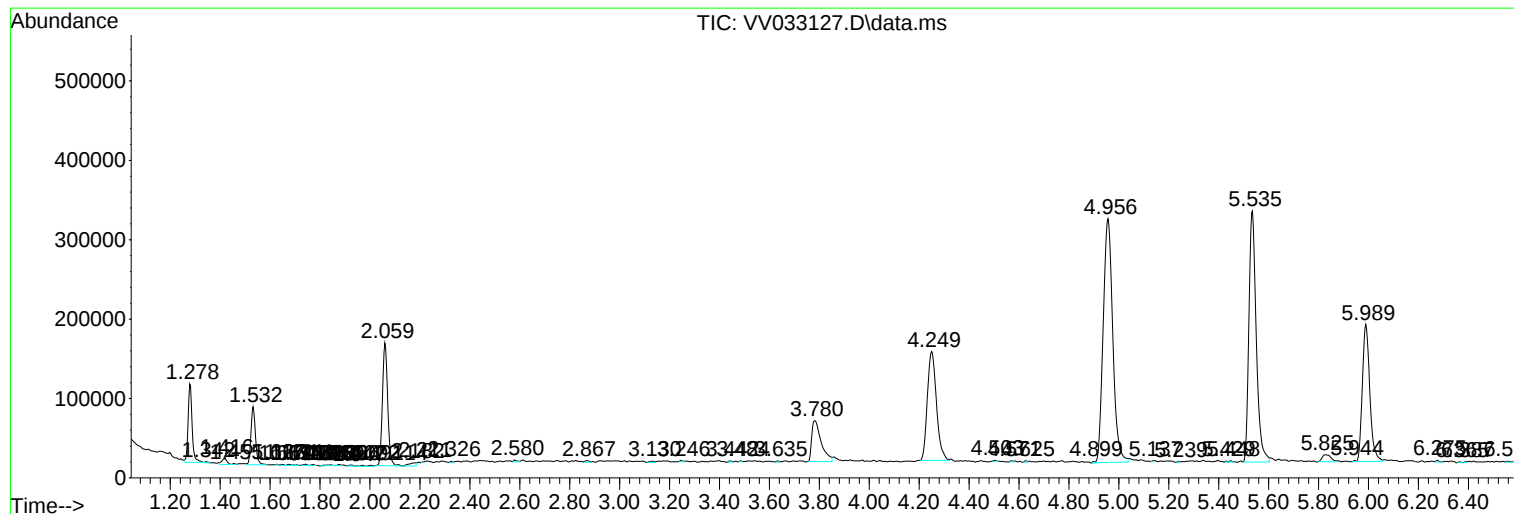

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033127.D
Acq On : 06 Dec 2023 19:22
Operator : SY/MD
Sample : 05644-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033127.D
Acq On : 06 Dec 2023 19:22
Operator : SY/MD
Sample : 05644-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G58

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------