

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033128.D
 Acq On : 06 Dec 2023 19:46
 Operator : SY/MD
 Sample : 05644-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	107560	108946	12.87%	1.503%
2	1.417	110	117	124	rVB2	6210	8244	0.97%	0.114%
3	1.462	129	131	134	rBV2	804	562	0.07%	0.008%
4	1.532	145	153	163	rBV	78067	91088	10.76%	1.256%
5	1.603	172	175	178	rBV3	659	363	0.04%	0.005%
6	1.619	178	180	183	rVB	1310	719	0.08%	0.010%
7	1.651	183	190	191	rBV2	851	796	0.09%	0.011%
8	1.677	195	198	200	rBV	514	298	0.04%	0.004%
9	1.773	225	228	231	rBV	943	531	0.06%	0.007%
10	1.838	241	248	255	rBV3	1349	1333	0.16%	0.018%
11	1.880	255	261	263	rBV2	1046	873	0.10%	0.012%
12	1.896	263	266	268	rBV	973	603	0.07%	0.008%
13	1.909	268	270	275	rVB3	1783	1153	0.14%	0.016%
14	1.944	277	281	286	rVB5	542	477	0.06%	0.007%
15	1.979	290	292	295	rVB2	618	340	0.04%	0.005%
16	2.011	299	302	305	rBV2	905	521	0.06%	0.007%
17	2.060	305	317	333	rBV	164331	242937	28.70%	3.351%
18	2.118	333	335	336	rBV2	776	417	0.05%	0.006%
19	2.127	336	338	339	rBV	679	347	0.04%	0.005%
20	2.140	339	342	343	rBV2	516	335	0.04%	0.005%
21	2.169	346	351	353	rBV	1383	1332	0.16%	0.018%
22	2.201	358	361	363	rVB2	1486	809	0.10%	0.011%
23	2.224	363	368	370	rBV2	1939	1834	0.22%	0.025%
24	2.281	382	386	387	rBV2	1626	1249	0.15%	0.017%
25	2.478	444	447	450	rBV	1846	1146	0.14%	0.016%
26	2.661	501	504	507	rBV2	1570	1249	0.15%	0.017%
27	2.892	573	576	578	rBV	1453	978	0.12%	0.013%
28	2.925	584	586	588	rBV	1007	539	0.06%	0.007%
29	2.941	588	591	593	rVV	1140	685	0.08%	0.009%
30	3.027	616	618	621	rVB	1214	595	0.07%	0.008%
31	3.169	660	662	663	rBV	931	425	0.05%	0.006%
32	3.227	677	680	684	rBV2	1314	1237	0.15%	0.017%
33	3.526	771	773	775	rBV	1238	784	0.09%	0.011%
34	3.712	828	831	834	rBV2	1065	800	0.09%	0.011%
35	3.728	834	836	838	rBV2	1083	699	0.08%	0.010%
36	3.780	844	852	870	rBV	55252	142766	16.87%	1.969%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120623\
 Data File : VW033128.D
 Acq On : 06 Dec 2023 19:46
 Operator : SY/MD
 Sample : 05644-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.249	984	998	1023	rBV2	144046	365635	43.20%	5.043%
38	4.870	1188	1191	1196	rVB2	1448	1131	0.13%	0.016%
39	4.957	1202	1218	1241	rBV2	315584	837053	98.90%	11.544%
40	5.137	1272	1274	1278	rBV2	1325	1055	0.12%	0.015%
41	5.204	1293	1295	1298	rVB	1935	957	0.11%	0.013%
42	5.223	1298	1301	1303	rBV	1808	1332	0.16%	0.018%
43	5.326	1329	1333	1337	rBV	1885	2174	0.26%	0.030%
44	5.461	1372	1375	1379	rBV	1476	1342	0.16%	0.019%
45	5.532	1386	1397	1422	rBV	315266	649962	76.80%	8.964%
46	5.834	1479	1491	1510	rBV7	56355	124558	14.72%	1.718%
47	5.989	1528	1539	1560	rBV2	179426	365325	43.17%	5.038%
48	6.291	1631	1633	1636	rVB	1684	926	0.11%	0.013%
49	6.915	1817	1827	1849	rBV	103957	195437	23.09%	2.695%
50	7.172	1904	1907	1911	rVB	1604	1169	0.14%	0.016%
51	7.243	1919	1929	1951	rBV	387080	672001	79.40%	9.268%
52	7.474	1999	2001	2004	rBV2	1290	715	0.08%	0.010%
53	7.494	2004	2007	2010	rVB	1608	1165	0.14%	0.016%
54	7.555	2016	2026	2044	rBV2	74564	134446	15.89%	1.854%
55	7.953	2146	2150	2154	rBV	1385	1169	0.14%	0.016%
56	7.985	2158	2160	2163	rBV	899	581	0.07%	0.008%
57	8.024	2163	2172	2199	rBV	199222	374286	44.22%	5.162%
58	8.153	2209	2212	2215	rVB	2068	1299	0.15%	0.018%
59	8.699	2379	2382	2388	rBV2	1676	2061	0.24%	0.028%
60	8.783	2397	2408	2427	rBV	499955	828656	97.91%	11.429%
61	8.886	2438	2440	2447	rVB	1900	1842	0.22%	0.025%
62	9.301	2566	2569	2572	rBV	957	726	0.09%	0.010%
63	9.593	2657	2660	2662	rBV2	1060	720	0.09%	0.010%
64	9.915	2757	2760	2763	rBV2	1162	868	0.10%	0.012%
65	10.040	2796	2799	2801	rBV	1495	926	0.11%	0.013%
66	10.153	2823	2834	2853	rBV	280989	437794	51.73%	6.038%
67	10.538	2951	2954	2957	rBV	1965	1297	0.15%	0.018%
68	10.590	2967	2970	2973	rBV	1727	1080	0.13%	0.015%
69	10.677	2994	2997	2999	rBV2	1397	734	0.09%	0.010%
70	10.767	3023	3025	3027	rBV	887	420	0.05%	0.006%
71	10.815	3038	3040	3043	rVB	1082	515	0.06%	0.007%
72	10.895	3062	3065	3069	rBV	1607	1303	0.15%	0.018%
73	10.982	3089	3092	3094	rBV	1315	956	0.11%	0.013%
74	11.111	3129	3132	3136	rBV	1311	1438	0.17%	0.020%
75	11.185	3144	3155	3177	rBV	540178	846345	100.00%	11.673%
76	11.339	3200	3203	3205	rBV2	1416	855	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
 Data File : VV033128.D
 Acq On : 06 Dec 2023 19:46
 Operator : SY/MD
 Sample : 05644-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.516	3256	3258	3261	rBV	1294	799	0.09%	0.011%
78	11.561	3261	3272	3289	rBV	471528	746310	88.18%	10.293%
79	11.712	3316	3319	3323	rVB	1760	1388	0.16%	0.019%
80	11.812	3347	3350	3352	rBV	1533	971	0.11%	0.013%
81	12.445	3545	3547	3551	rVB	1712	1025	0.12%	0.014%
82	12.908	3688	3691	3694	rBV	2160	1620	0.19%	0.022%
83	12.985	3712	3715	3718	rBV	1349	1043	0.12%	0.014%
84	13.185	3774	3777	3779	rBV3	1279	1012	0.12%	0.014%
85	13.233	3790	3792	3795	rBV2	1257	870	0.10%	0.012%
86	13.300	3809	3813	3816	rBV	1821	1779	0.21%	0.025%
87	13.432	3851	3854	3856	rBV	1130	845	0.10%	0.012%
88	13.612	3908	3910	3912	rBV	1399	596	0.07%	0.008%
89	13.625	3912	3914	3916	rBV2	899	409	0.05%	0.006%
90	13.722	3941	3944	3947	rBV	1259	800	0.09%	0.011%
91	14.059	4046	4049	4057	rVB	1527	1309	0.15%	0.018%
92	14.403	4153	4156	4159	rBV	1555	957	0.11%	0.013%
93	14.628	4224	4226	4229	rVB2	1047	506	0.06%	0.007%
94	14.995	4338	4340	4344	rBV	1363	1236	0.15%	0.017%
95	15.111	4374	4376	4380	rVB4	1742	1101	0.13%	0.015%
96	15.390	4461	4463	4466	rBV2	1233	871	0.10%	0.012%
97	15.641	4538	4541	4544	rBV	1836	1421	0.17%	0.020%
98	15.705	4558	4561	4563	rVB2	1965	1086	0.13%	0.015%
99	15.721	4564	4566	4570	rVB2	1872	1185	0.14%	0.016%
100	15.975	4642	4645	4649	rBV	1900	1343	0.16%	0.019%




Sum of corrected areas: 7250746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033128.D
Acq On : 06 Dec 2023 19:46
Operator : SY/MD
Sample : 05644-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

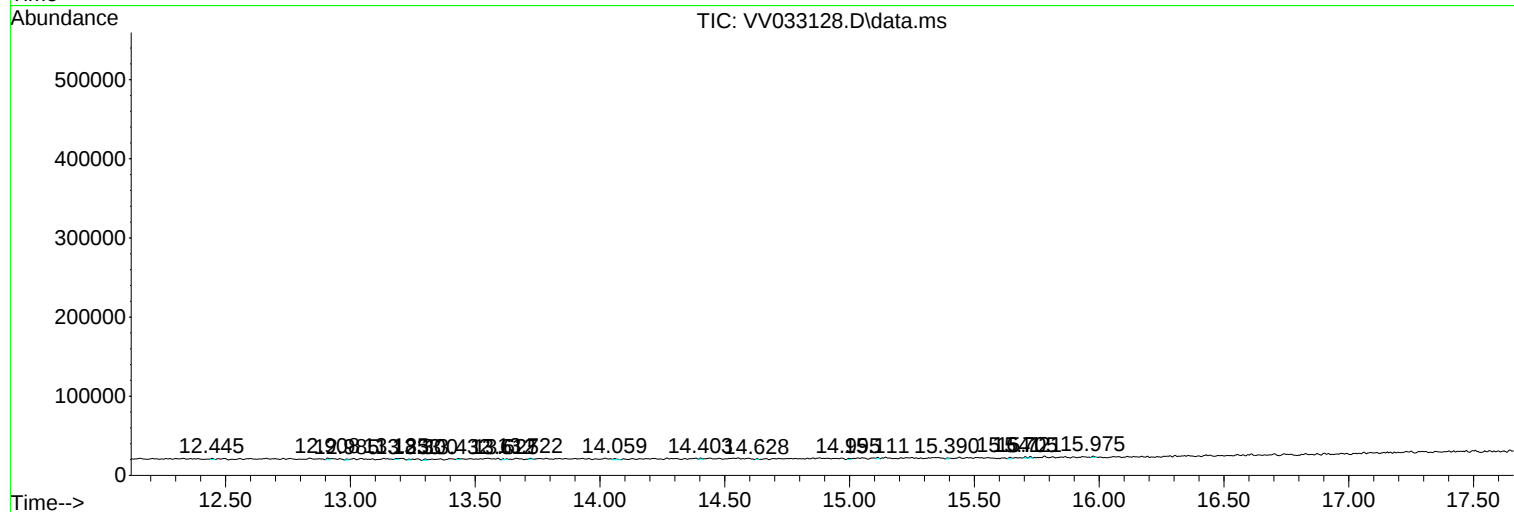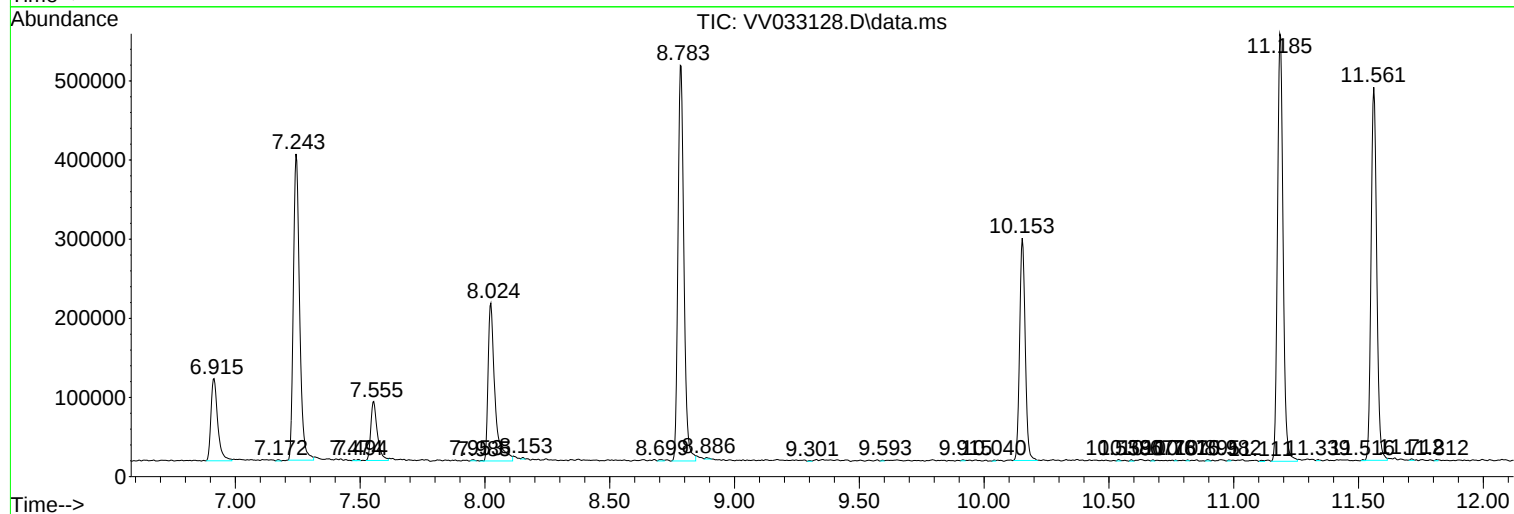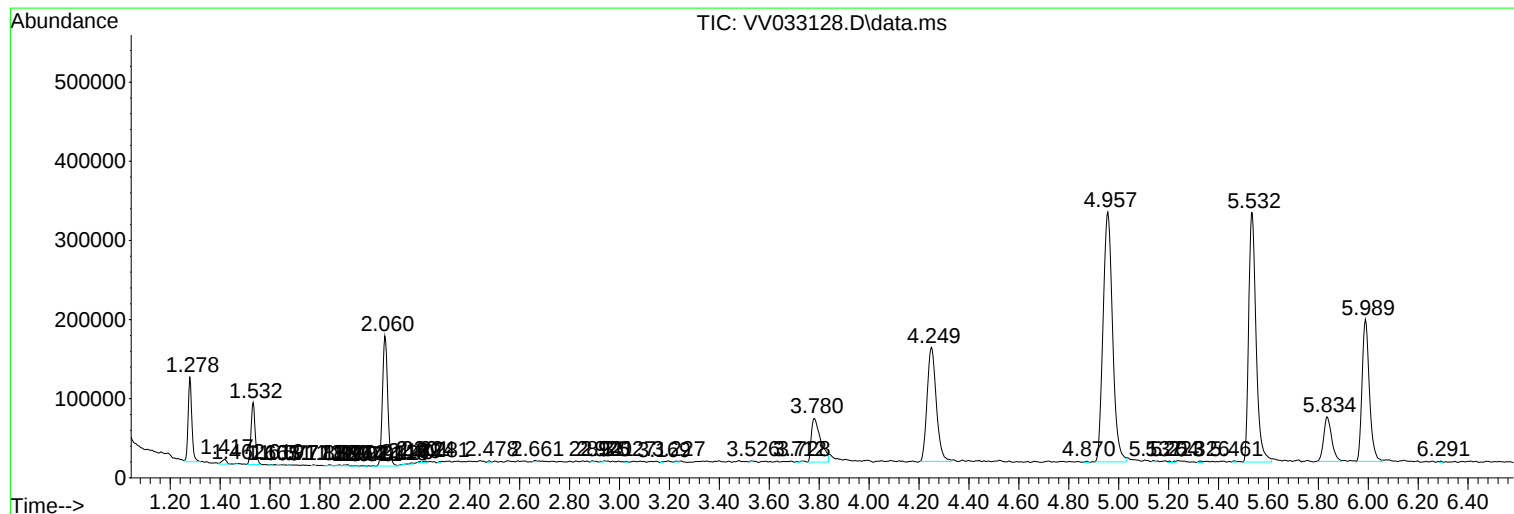

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033128.D
Acq On : 06 Dec 2023 19:46
Operator : SY/MD
Sample : 05644-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033128.D
Acq On : 06 Dec 2023 19:46
Operator : SY/MD
Sample : 05644-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------