
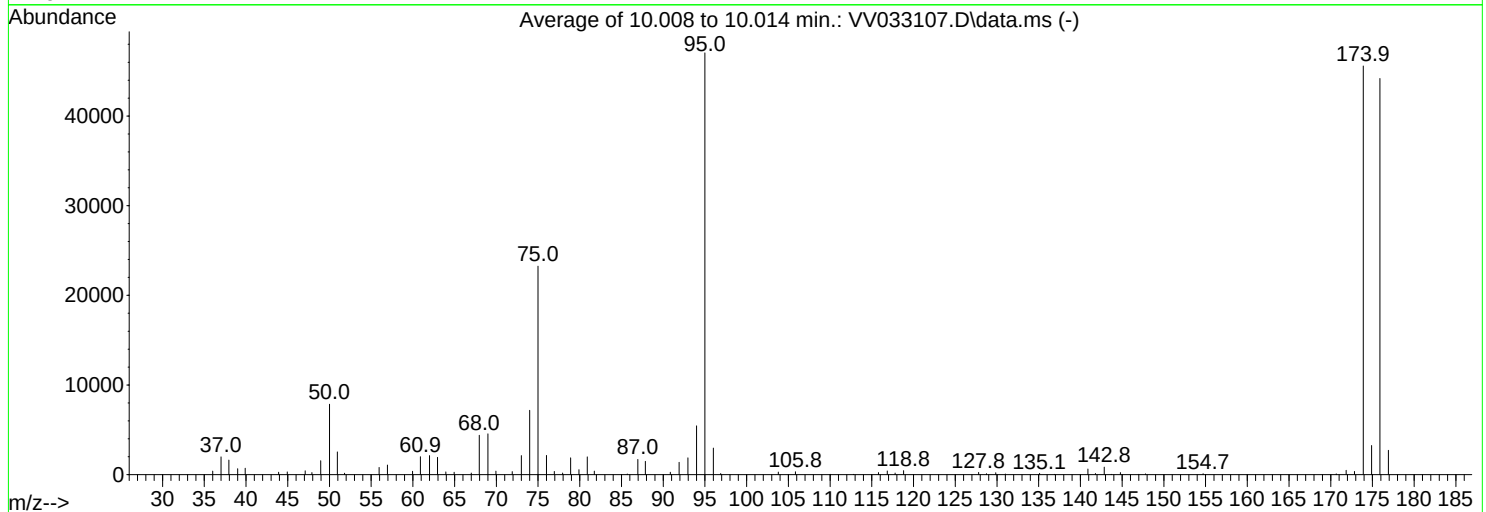


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120623\
Data File : VV033107.D
Acq On : 06 Dec 2023 09:18
Operator : SY/MD
Sample : BFB241
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB241

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Fri Dec 08 21:51:12 2023

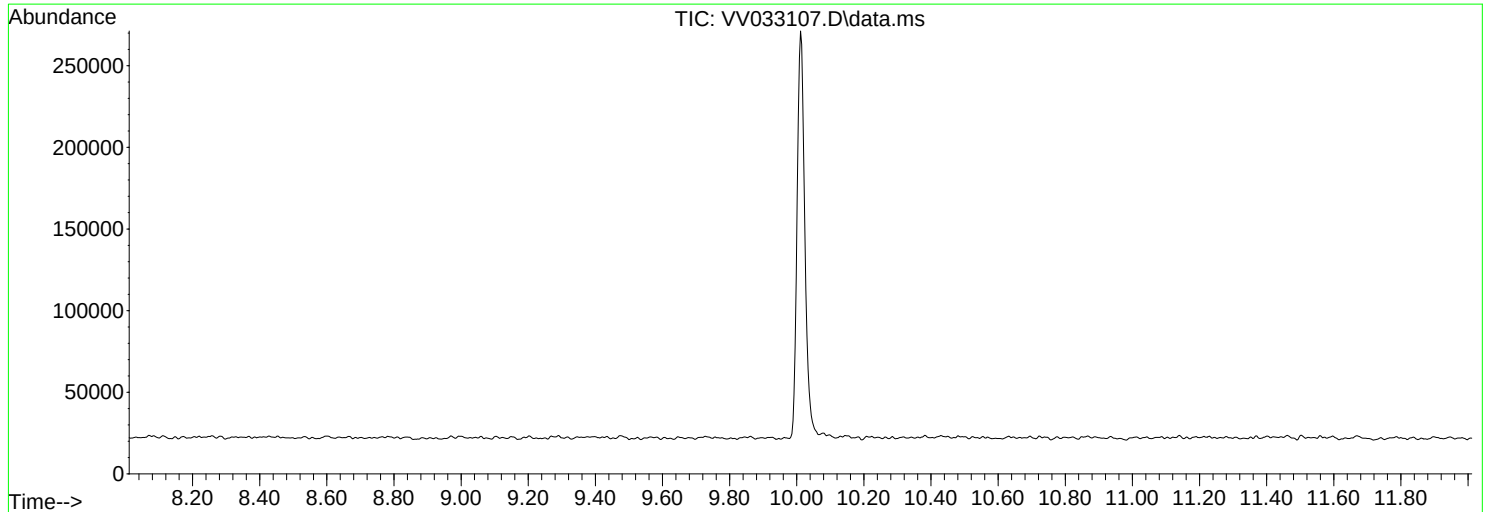

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	7857	PASS
75	95	30	80	49.4	23256	PASS
95	95	100	100	100.0	47048	PASS
96	95	5	9	6.3	2971	PASS
173	174	0.00	2	0.8	355	PASS
174	95	50	120	96.9	45581	PASS
175	174	5	9	7.1	3250	PASS
176	174	95	105	96.9	44184	PASS
177	176	5	10	6.1	2707	PASS

m/z	Abundance
39.10	110.0
39.90	21440.0
44.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	370.0
37.00	2128.0
38.00	1552.0
39.00	752.0
39.90	22032.0
43.90	444.0
45.00	290.0
47.10	390.0
47.90	237.0
49.00	1461.0
50.00	7663.0
50.90	2361.0
51.80	116.0
56.00	802.0
56.90	1099.0
60.00	414.0
60.90	2296.0
62.00	2188.0
62.90	1859.0
63.90	316.0
65.00	261.0
67.10	173.0
67.90	4443.0
69.00	4734.0
69.90	380.0
71.90	302.0
73.00	2210.0
74.00	6699.0
75.00	22984.0
76.00	2008.0
76.90	296.0
77.90	194.0
78.90	1874.0
79.90	583.0
80.90	1853.0
81.70	379.0
85.70	123.0
86.90	1781.0
87.80	1332.0
90.90	253.0
91.80	1327.0
93.00	1819.0
94.00	5163.0
95.00	46200.0
96.00	2981.0
96.90	117.0
103.80	234.0
105.80	346.0
115.80	219.0
116.80	395.0
117.80	162.0
118.80	444.0
127.80	209.0
128.70	105.0
129.80	171.0
135.10	102.0
136.90	127.0
140.90	614.0
141.80	139.0
142.90	761.0
144.80	205.0
147.00	100.0
171.80	433.0
173.90	43488.0
174.90	3118.0
175.90	41688.0
176.90	2627.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	392.0
37.00	2066.0
37.90	1681.0
39.00	818.0
39.90	22248.0
43.90	449.0
44.90	309.0
47.10	426.0
47.90	214.0
48.90	1615.0
50.00	8175.0
51.00	2654.0
51.80	173.0
56.00	859.0
57.00	1114.0
60.00	370.0
60.90	1995.0
62.00	2219.0
63.00	1995.0
63.90	329.0
65.00	284.0
67.00	178.0
67.90	4490.0
69.00	4743.0
70.00	412.0
71.90	368.0
73.00	2155.0
74.00	7405.0
75.00	24136.0
76.00	2256.0
76.90	341.0
77.90	179.0
78.90	1898.0
79.90	560.0
80.90	2054.0
81.80	372.0
85.70	118.0
87.00	1747.0
87.90	1517.0
90.80	278.0
91.90	1340.0
92.90	1848.0
94.00	5624.0
95.00	48728.0
96.00	3057.0
96.90	136.0
103.80	280.0
105.80	334.0
115.80	247.0
116.90	433.0
117.80	175.0
118.80	471.0
127.80	266.0
128.80	117.0
129.90	211.0
131.00	103.0
135.10	154.0
140.90	678.0
141.80	115.0
142.90	886.0
143.70	103.0
144.80	249.0
147.80	131.0
154.70	145.0
170.60	126.0
171.90	512.0
172.90	579.0
173.90	46976.0
174.90	3351.0
175.90	45544.0
176.90	2772.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	400.0
37.00	1727.0
37.90	1634.0
39.00	756.0
39.90	22176.0
43.90	426.0
44.90	328.0
47.10	456.0
47.90	240.0
49.00	1571.0
50.00	7732.0
51.00	2597.0
51.80	180.0
55.90	760.0
57.00	1004.0
59.80	372.0
60.90	1696.0
62.00	1976.0
63.00	1939.0
64.00	288.0
64.90	285.0
66.90	203.0
68.00	4239.0
69.00	4201.0
70.00	412.0
71.90	373.0
73.00	1982.0
74.00	7399.0
75.00	22648.0
76.00	2169.0
77.00	424.0
78.00	166.0
78.90	1837.0
79.90	516.0
80.90	2033.0
81.80	411.0
87.00	1565.0
87.90	1623.0
90.90	260.0
92.00	1449.0
92.90	1956.0
94.00	5560.0
95.00	46216.0
96.00	2876.0
96.90	101.0
103.80	319.0
105.90	287.0
110.00	102.0
112.80	127.0
115.80	232.0
116.90	387.0
117.80	185.0
118.80	409.0
127.80	262.0
128.80	128.0
129.90	255.0
131.00	115.0
135.10	168.0
140.90	613.0
141.80	102.0
142.80	898.0
144.80	260.0
147.80	163.0
154.70	162.0
170.70	141.0
171.90	493.0
172.80	486.0
173.90	46280.0
174.90	3280.0
175.90	45320.0
176.90	2722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241