

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120718\
 Data File : VV008882.D
 Acq On : 07 Dec 2018 17:58
 Operator : SY/MD
 Sample : J6263-05
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0TP2

Quant Time: Dec 08 01:07:42 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 07 22:19:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	104646	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	98904	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	43744	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	24836	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.59	69	19330	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.14	63	45374	4.22	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.40%
20) 2-Butanone-d5	3.96	46	72826	52.84	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.68%
24) Chloroform-d	4.41	84	61786	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.09	65	32209	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.10	84	123731	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.12	67	36021	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.36	98	110249	4.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.00%
43) trans-1,3-Dichloropropene-	7.67	79	13087	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.14	63	50946	46.66	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.32%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	22592	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	40607	5.04	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.80%


Target Compounds					Ovalue
13) Acetone	2.22	43	10153	13.233 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120718\
Data File : VV008882.D
Acq On : 07 Dec 2018 17:58
Operator : SY/MD
Sample : J6263-05
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0TP2

Quant Time: Dec 08 01:07:42 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 07 22:19:33 2018
Response via : Initial Calibration

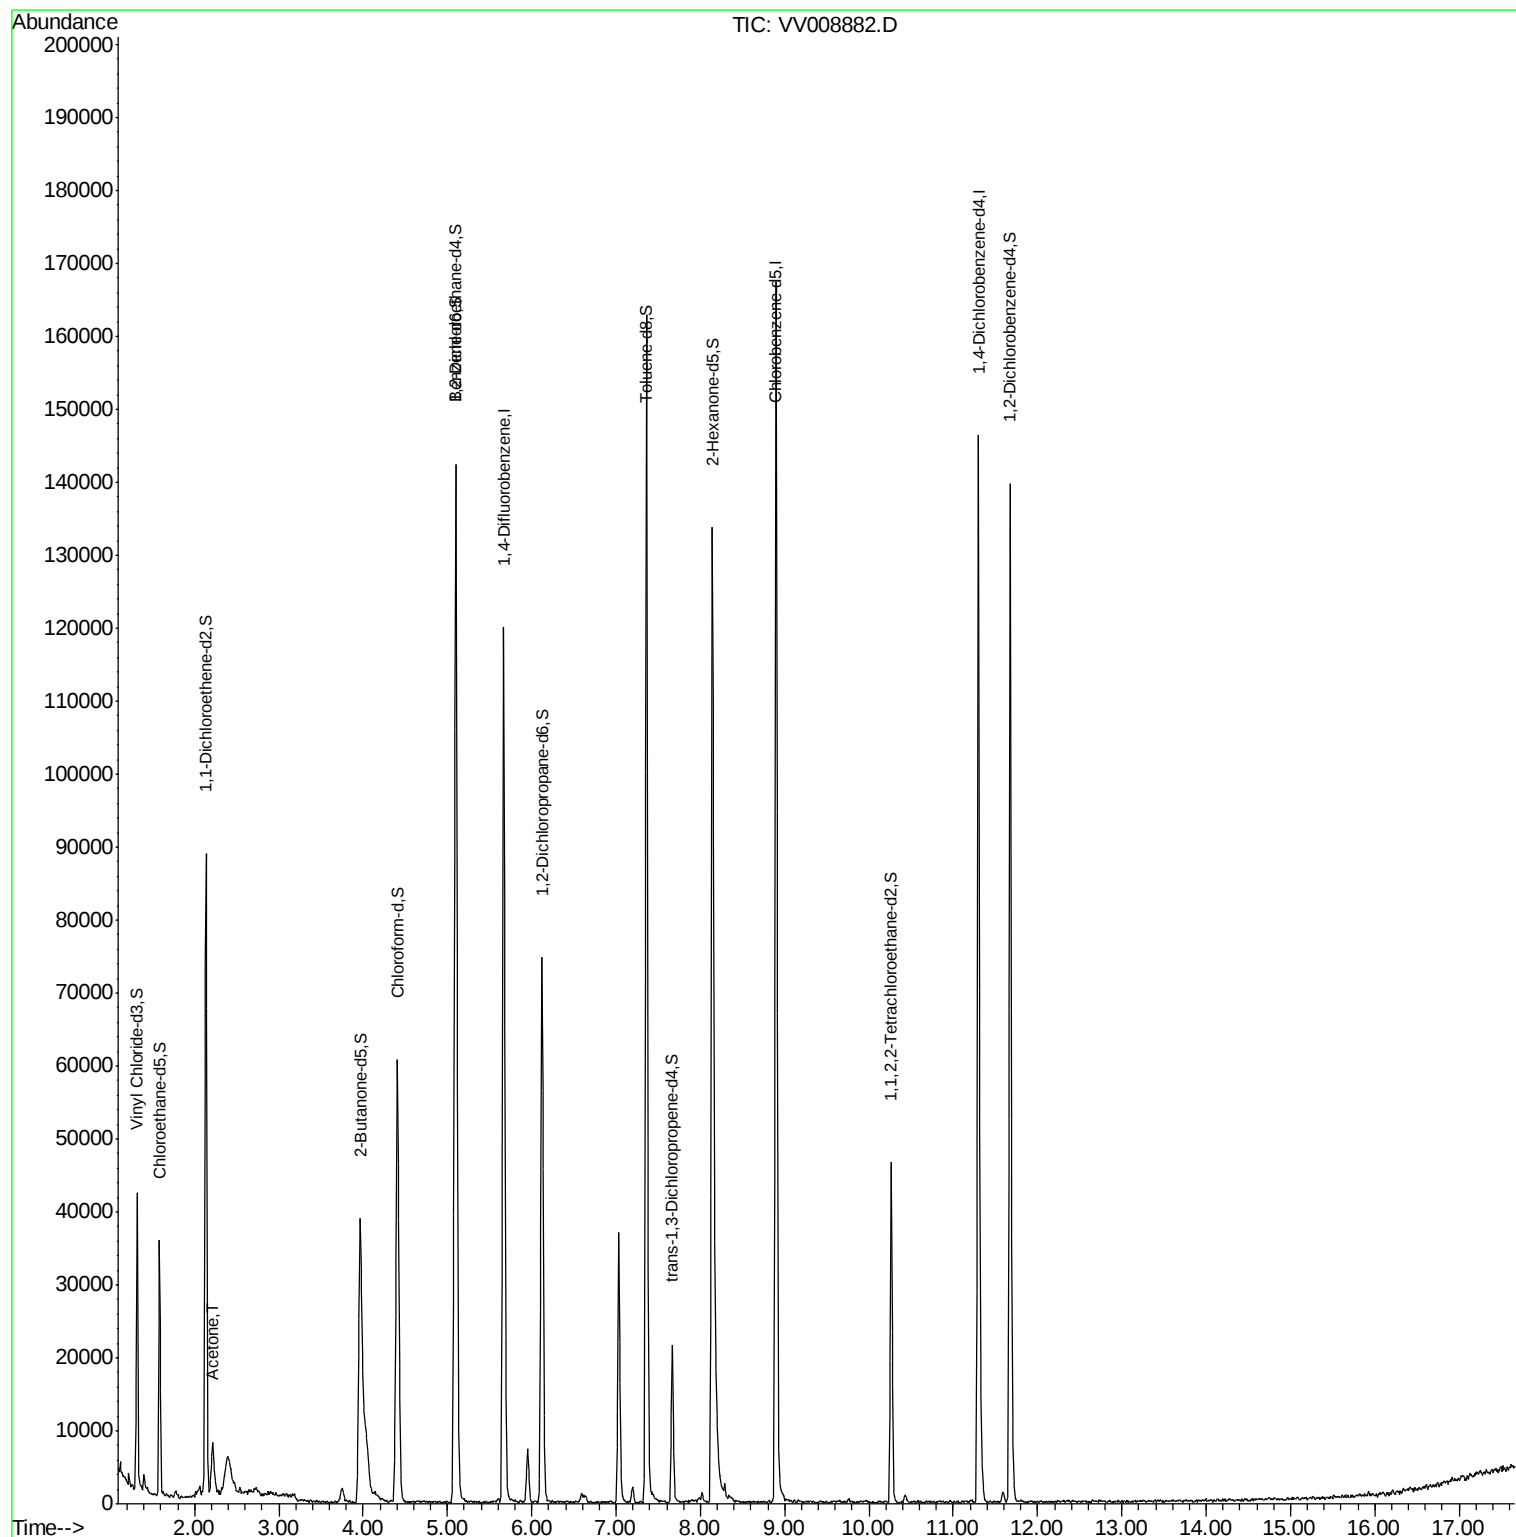

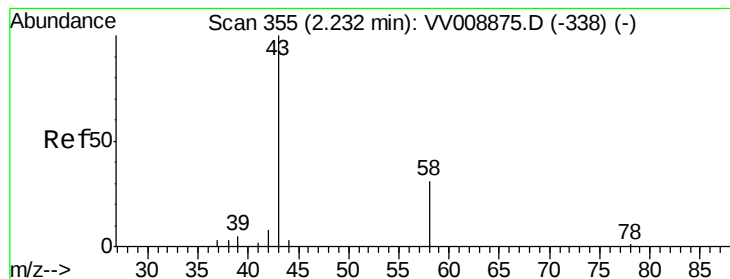

#13
 Acetone
 Concen: 13.233 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. -0.02 min
 Lab File: VV008882.D
 Acq: 07 Dec 2018 17:58

Instrument :
 MSVOA_V
 ClientSampleId :
 C0TP2

Tot Ion	Ion	Ratio	Lower	Upper
43	100			
58	29.4	0.0	52.4	

