


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120718\
Data File : VV008874.D
Acq On : 07 Dec 2018 12:02
Operator : SY/MD
Sample : BFB56
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR120518WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Dec 07 22:19:33 2018

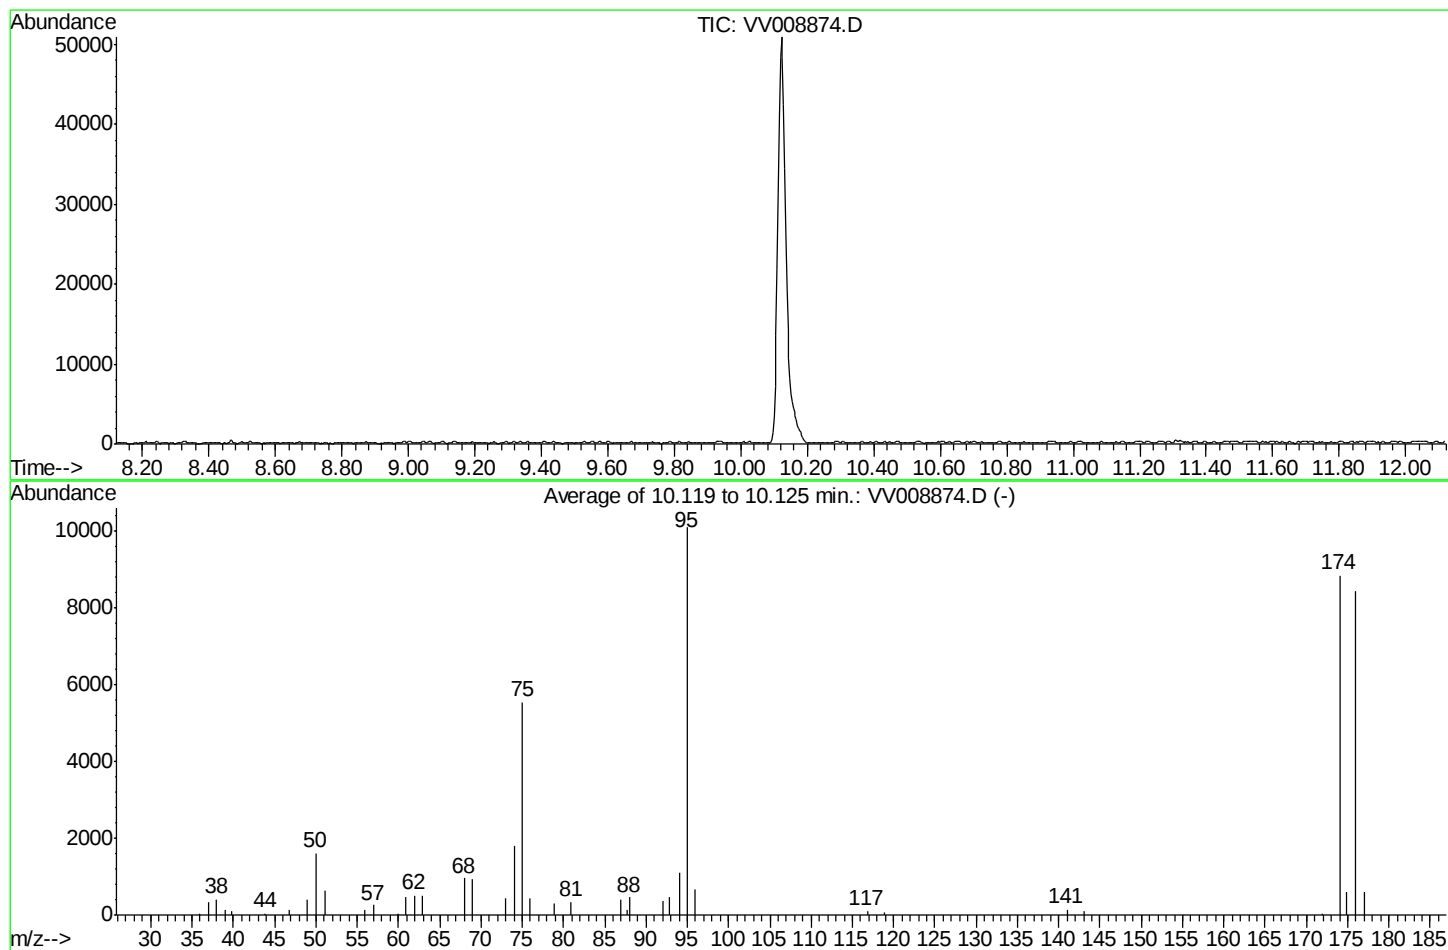

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	1617	PASS
75	95	30	80	55.0	5552	PASS
95	95	100	100	100.0	10100	PASS
96	95	5	9	6.5	654	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.6	8844	PASS
175	174	5	9	6.7	593	PASS
176	174	95	101	95.4	8433	PASS
177	176	5	9	7.0	593	PASS

m/z	Abundance
35.90	110.0
36.90	337.0
38.00	433.0
38.90	152.0
39.80	116.0
43.80	201.0
46.80	130.0
49.00	411.0
50.00	1650.0
51.00	653.0
55.90	145.0
57.00	211.0
60.80	483.0
61.90	503.0
62.90	510.0
68.00	971.0
69.00	864.0
72.90	426.0
74.00	1870.0
75.00	5470.0
76.00	409.0
78.90	320.0
80.90	368.0
87.00	399.0
88.00	344.0
92.00	342.0
92.90	422.0
94.00	1159.0
95.00	9984.0
96.00	666.0
116.80	112.0
118.80	106.0
141.00	139.0
143.00	127.0
174.00	8619.0
174.90	645.0
176.00	7986.0
177.00	539.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
43.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
37.00	318.0
38.00	345.0
39.00	146.0
39.90	115.0
43.90	151.0
46.80	103.0
49.00	368.0
50.00	1548.0
51.10	629.0
55.80	122.0
57.00	322.0
59.90	129.0
60.90	459.0
62.00	490.0
63.00	460.0
68.00	925.0
69.00	955.0
73.00	421.0
74.00	1700.0
75.10	5385.0
76.00	457.0
78.90	266.0
80.90	325.0
86.90	374.0
87.70	360.0
88.10	353.0
92.00	383.0
92.90	465.0
94.00	1009.0
95.00	9896.0
96.00	641.0
116.80	102.0
141.00	144.0
143.00	107.0
174.00	8796.0
174.90	512.0
176.00	8621.0
176.90	626.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.90	332.0
38.00	425.0
38.90	144.0
39.90	121.0
43.80	167.0
46.80	141.0
49.00	461.0
50.00	1655.0
51.00	638.0
55.90	159.0
57.00	263.0
60.90	466.0
61.90	529.0
63.00	507.0
68.00	968.0
69.00	950.0
73.00	433.0
74.00	1857.0
75.00	5801.0
76.00	445.0
78.90	311.0
80.90	361.0
86.90	393.0
87.80	327.0
88.10	363.0
92.00	410.0
92.90	471.0
94.00	1088.0
95.00	10421.0
96.00	655.0
116.80	121.0
118.80	103.0
141.00	165.0
143.00	116.0
171.90	115.0
174.00	9118.0
174.90	623.0
176.00	8694.0
177.00	615.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56