

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120720\
 Data File : VV019494.D
 Acq On : 07 Dec 2020 16:20
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	82	rVB	181103	177910	11.78%	1.650%
2	1.576	144	151	161	rVB	168606	189979	12.58%	1.762%
3	2.123	312	321	344	rVB	355452	544549	36.06%	5.051%
4	2.608	468	472	473	rBV3	832	509	0.03%	0.005%
5	2.730	507	510	512	rBV3	444	286	0.02%	0.003%
6	2.766	518	521	523	rBV	896	691	0.05%	0.006%
7	2.849	545	547	550	rVB3	724	429	0.03%	0.004%
8	2.904	560	564	565	rBV2	835	584	0.04%	0.005%
9	2.987	586	590	591	rBV2	751	477	0.03%	0.004%
10	3.103	624	626	628	rBV3	561	336	0.02%	0.003%
11	3.155	640	642	644	rBV3	800	269	0.02%	0.002%
12	3.216	657	661	663	rVB2	871	491	0.03%	0.005%
13	3.296	681	686	689	rBV3	567	468	0.03%	0.004%
14	3.322	690	694	696	rVV4	613	542	0.04%	0.005%
15	3.344	699	701	704	rVB	775	289	0.02%	0.003%
16	3.377	709	711	716	rVV4	917	595	0.04%	0.006%
17	3.505	747	751	752	rBV3	507	327	0.02%	0.003%
18	3.592	773	778	780	rBV4	554	481	0.03%	0.004%
19	3.640	791	793	797	rVB2	768	339	0.02%	0.003%
20	3.688	806	808	810	rBV2	564	243	0.02%	0.002%
21	3.714	813	816	818	rBV2	595	466	0.03%	0.004%
22	3.769	830	833	835	rBV3	541	411	0.03%	0.004%
23	3.901	864	874	906	rBV	96590	278766	18.46%	2.586%
24	4.373	1003	1021	1051	rBV	239763	597204	39.55%	5.540%
25	4.608	1090	1094	1096	rBV4	802	704	0.05%	0.007%
26	4.743	1135	1136	1138	rBV3	788	297	0.02%	0.003%
27	4.817	1155	1159	1162	rBV4	798	636	0.04%	0.006%
28	4.910	1186	1188	1192	rBV4	656	522	0.03%	0.005%
29	5.068	1218	1237	1263	rBV2	585789	1509910	100.00%	14.006%
30	5.444	1352	1354	1355	rBV2	1000	388	0.03%	0.004%
31	5.544	1379	1385	1387	rBV5	854	816	0.05%	0.008%
32	5.579	1393	1396	1397	rBV2	770	398	0.03%	0.004%
33	5.637	1402	1414	1440	rBV	425905	859117	56.90%	7.969%
34	5.846	1477	1479	1482	rBV2	1050	555	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120720\
 Data File : VV019494.D
 Acq On : 07 Dec 2020 16:20
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
 Title : VOC Analysis

35	5.878	1487	1489	1490	rBV2	735	363	0.02%	0.003%
36	5.926	1493	1504	1526	rVV3	40150	86913	5.76%	0.806%
37	6.090	1542	1555	1585	rBV	342797	703292	46.58%	6.524%
38	6.396	1647	1650	1652	rVB3	817	333	0.02%	0.003%
39	6.425	1657	1659	1661	rVB2	975	367	0.02%	0.003%
40	6.444	1661	1665	1667	rBV2	545	447	0.03%	0.004%
41	6.511	1683	1686	1688	rBV3	653	478	0.03%	0.004%
42	6.598	1710	1713	1715	rBV2	765	601	0.04%	0.006%
43	6.727	1750	1753	1754	rBV	512	347	0.02%	0.003%
44	6.891	1802	1804	1806	rVB2	536	259	0.02%	0.002%
45	7.007	1825	1840	1864	rBV	179238	338989	22.45%	3.145%
46	7.335	1930	1942	1972	rBV	642777	1119544	74.15%	10.385%
47	7.585	2018	2020	2024	rVB5	935	462	0.03%	0.004%
48	7.640	2028	2037	2059	rVV	131236	227541	15.07%	2.111%
49	7.942	2128	2131	2134	rBV3	1043	607	0.04%	0.006%
50	8.058	2162	2167	2171	rBV5	1061	1126	0.07%	0.010%
51	8.106	2172	2182	2219	rBV2	265885	557002	36.89%	5.167%
52	8.605	2335	2337	2341	rBV3	552	236	0.02%	0.002%
53	8.730	2373	2376	2378	rBV3	1078	722	0.05%	0.007%
54	8.872	2408	2420	2440	rBV	660778	1064106	70.47%	9.871%
55	9.106	2491	2493	2495	rBV3	1078	621	0.04%	0.006%
56	9.354	2568	2570	2576	rBV4	684	509	0.03%	0.005%
57	9.563	2633	2635	2636	rBV2	640	253	0.02%	0.002%
58	9.852	2722	2725	2727	rBV3	830	595	0.04%	0.006%
59	9.875	2730	2732	2736	rVB3	924	533	0.04%	0.005%
60	9.916	2741	2745	2747	rBV2	805	657	0.04%	0.006%
61	10.019	2776	2777	2779	rBV2	562	241	0.02%	0.002%
62	10.235	2830	2844	2862	rBV	355287	561542	37.19%	5.209%
63	10.363	2882	2884	2887	rVB2	861	385	0.03%	0.004%
64	10.399	2892	2895	2896	rBV2	611	319	0.02%	0.003%
65	10.444	2906	2909	2910	rBV2	1048	490	0.03%	0.005%
66	10.482	2917	2921	2925	rVB5	959	984	0.07%	0.009%
67	10.518	2925	2932	2934	rBV5	1029	1074	0.07%	0.010%
68	10.531	2934	2936	2939	rBV3	1062	685	0.05%	0.006%
69	10.646	2970	2972	2976	rBV3	457	243	0.02%	0.002%
70	10.675	2978	2981	2985	rBV2	989	663	0.04%	0.006%
71	10.746	3000	3003	3005	rBV2	1444	774	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120720\
 Data File : VV019494.D
 Acq On : 07 Dec 2020 16:20
 Operator : SY/MD
 Sample : VV1207MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
 Title : VOC Analysis

72	10.797	3011	3019	3022	rBV7	820	1111	0.07%	0.010%
73	10.842	3031	3033	3037	rBV3	691	554	0.04%	0.005%
74	10.897	3048	3050	3054	rVB3	645	395	0.03%	0.004%
75	10.933	3057	3061	3063	rBV4	1167	869	0.06%	0.008%
76	11.010	3083	3085	3091	rBV7	976	717	0.05%	0.007%
77	11.154	3127	3130	3133	rBV2	851	687	0.05%	0.006%
78	11.270	3154	3166	3188	rBV	610270	946113	62.66%	8.776%
79	11.386	3197	3202	3203	rBV4	1067	883	0.06%	0.008%
80	11.521	3239	3244	3245	rBV3	691	576	0.04%	0.005%
81	11.643	3271	3282	3305	rBV	611354	970652	64.29%	9.004%
82	11.875	3352	3354	3356	rBV3	654	327	0.02%	0.003%
83	11.907	3360	3364	3365	rBV3	765	569	0.04%	0.005%
84	12.048	3407	3408	3414	rVB4	914	713	0.05%	0.007%
85	12.100	3421	3424	3426	rBV2	595	387	0.03%	0.004%
86	12.148	3437	3439	3441	rBV3	650	292	0.02%	0.003%
87	12.482	3540	3543	3545	rBV2	517	377	0.02%	0.003%
88	12.646	3592	3594	3597	rBV3	858	703	0.05%	0.007%
89	12.768	3630	3632	3635	rBV2	616	307	0.02%	0.003%
90	12.878	3663	3666	3668	rBV2	916	666	0.04%	0.006%
91	13.251	3781	3782	3784	rBV	504	262	0.02%	0.002%
92	13.289	3787	3794	3802	rVV10	2805	4601	0.30%	0.043%
93	13.321	3802	3804	3807	rBV2	923	600	0.04%	0.006%
94	13.614	3892	3895	3896	rBV3	669	298	0.02%	0.003%
95	13.910	3985	3987	3988	rBV2	624	241	0.02%	0.002%
96	14.016	4018	4020	4024	rBV3	1010	633	0.04%	0.006%
97	14.402	4138	4140	4142	rBV3	904	493	0.03%	0.005%
98	14.588	4196	4198	4202	rBV2	1217	552	0.04%	0.005%
99	14.691	4228	4230	4233	rBV3	702	465	0.03%	0.004%
100	15.087	4350	4353	4357	rBV4	979	806	0.05%	0.007%


Sum of corrected areas: 10780136

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120720\
Data File : VV019494.D
Acq On : 07 Dec 2020 16:20
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.0µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

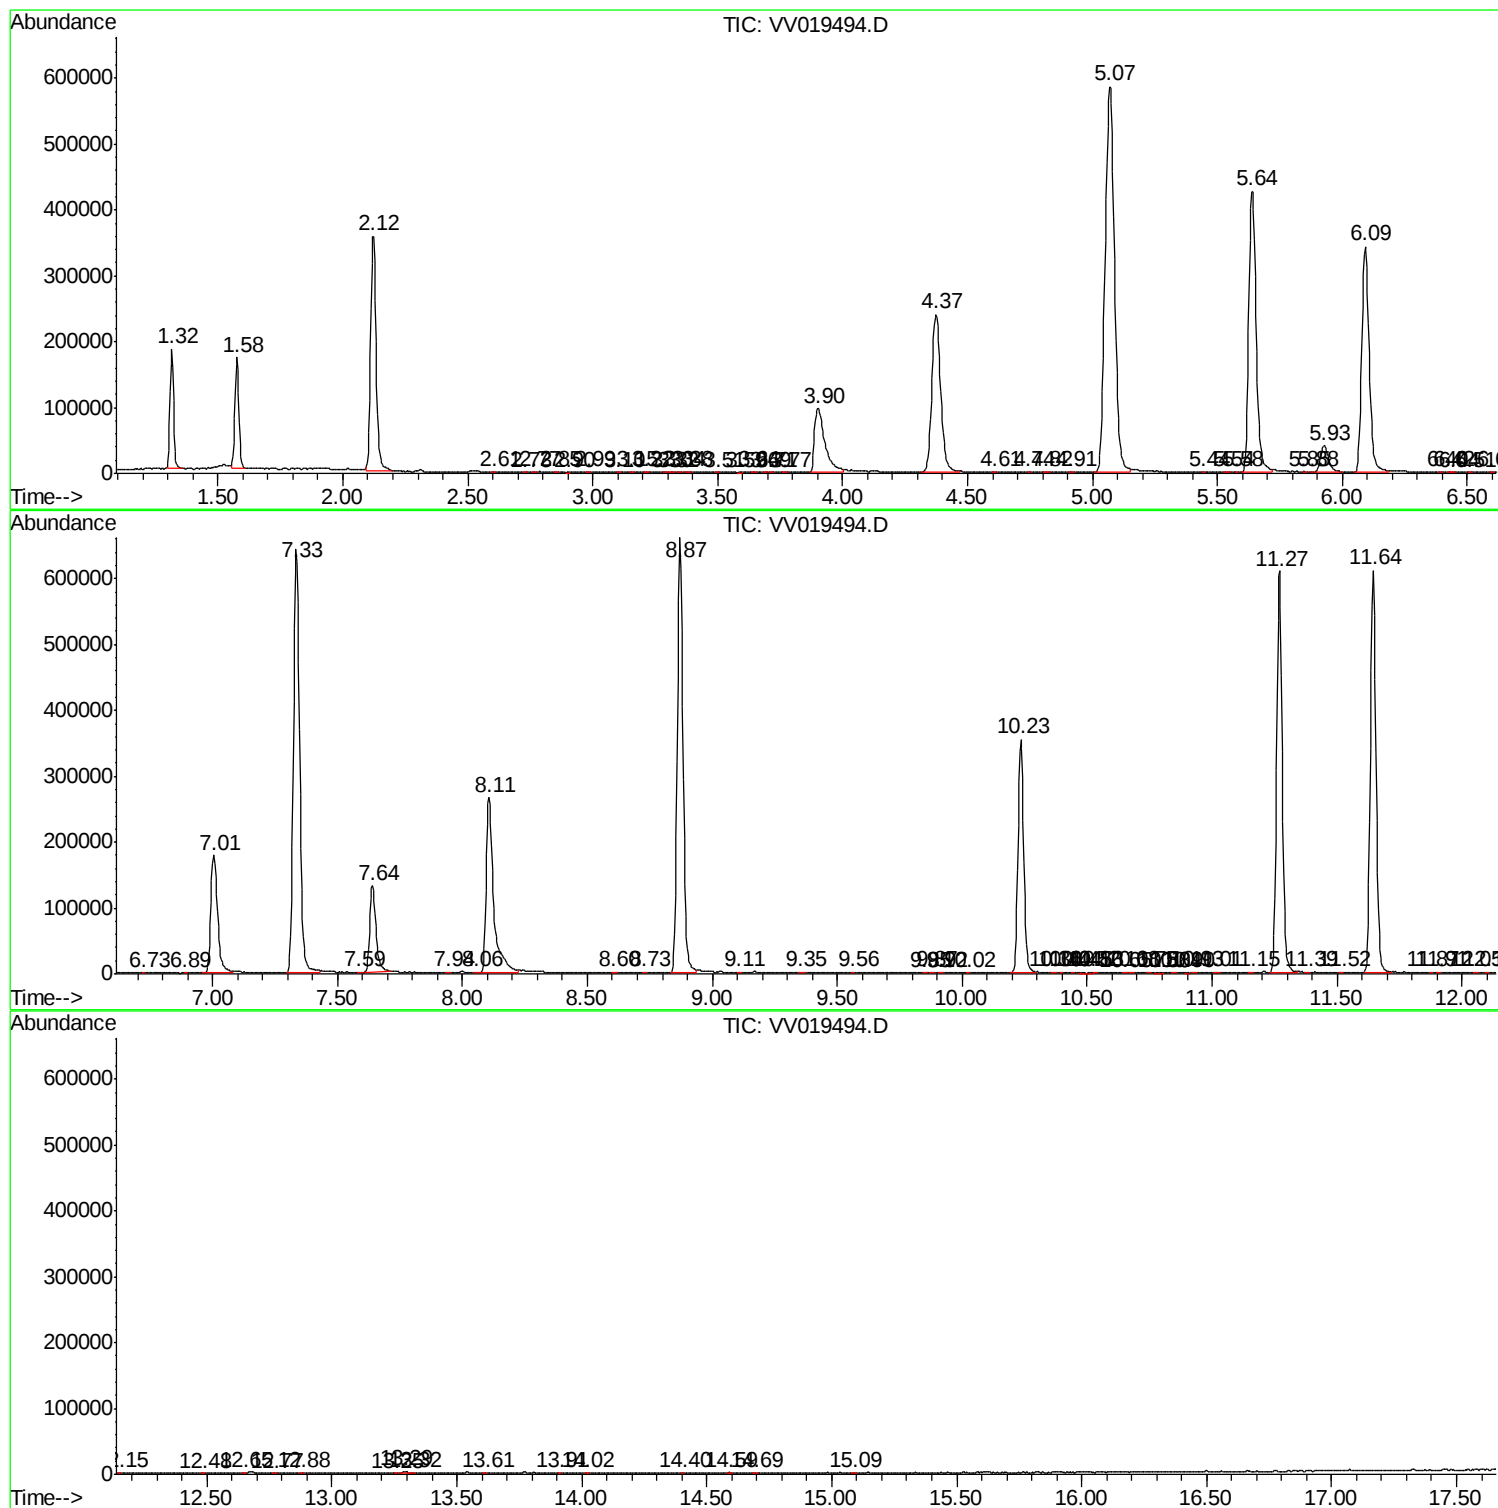

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120720\
Data File : VV019494.D
Acq On : 07 Dec 2020 16:20
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120720\
Data File : VV019494.D
Acq On : 07 Dec 2020 16:20
Operator : SY/MD
Sample : VV1207MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK96

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc