


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120720\
 Data File : VV019484.D
 Acq On : 07 Dec 2020 09:25
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120720WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 08 03:05:02 2020

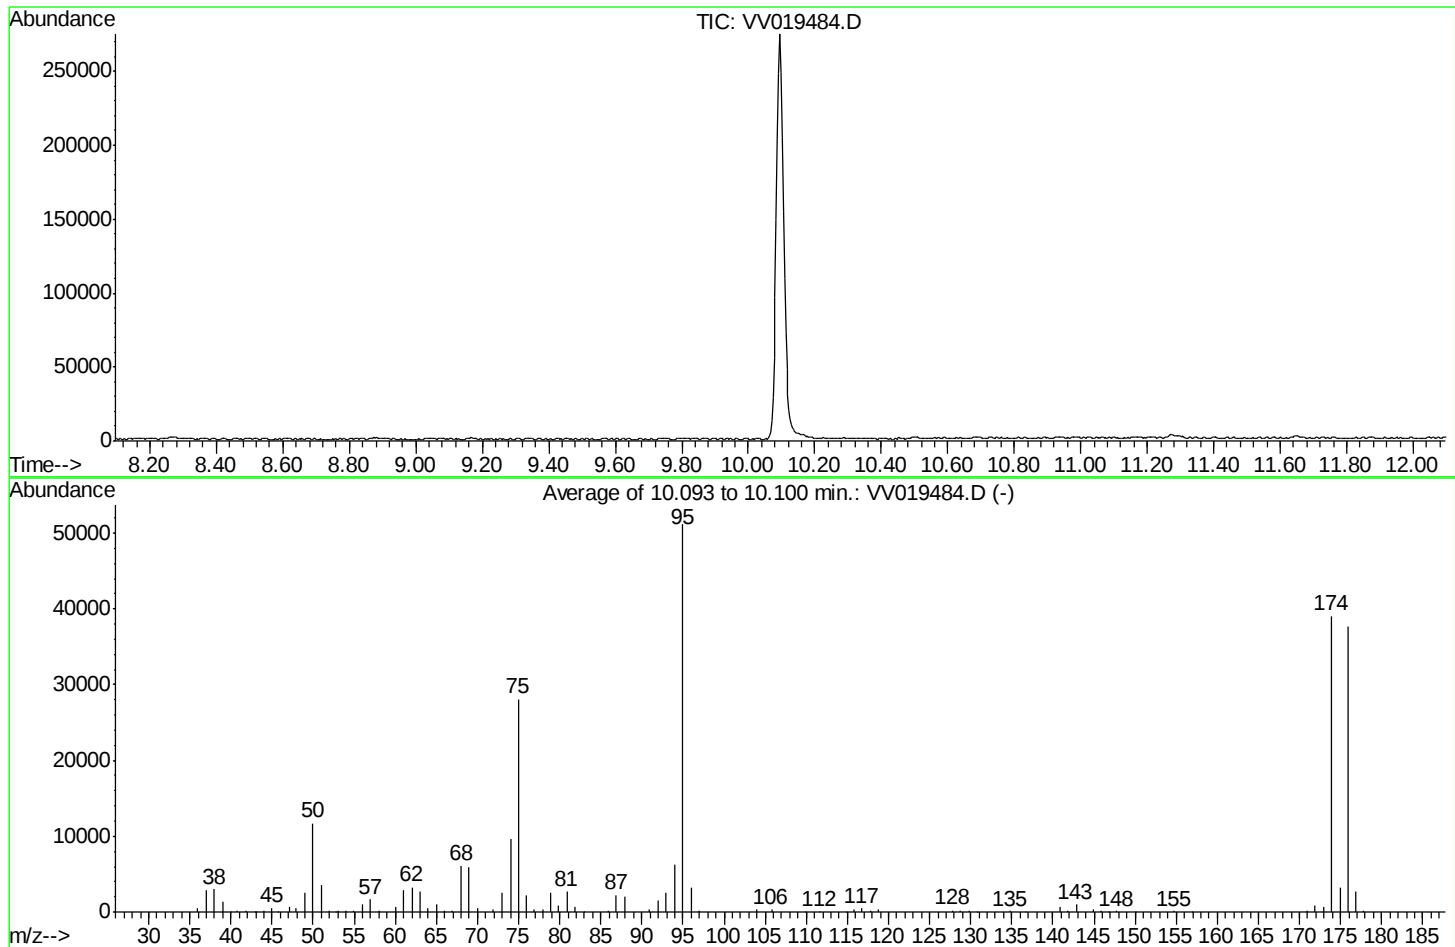

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	11729	PASS
75	95	30	80	55.0	28120	PASS
95	95	100	100	100.0	51154	PASS
96	95	5	9	6.2	3173	PASS
173	174	0.00	2	1.9	730	PASS
174	95	50	120	76.4	39058	PASS
175	174	5	9	8.1	3163	PASS
176	174	95	101	96.5	37690	PASS
177	176	5	9	7.3	2733	PASS

m/z	Abundance
36.00	566.0
37.00	3196.0
38.00	3237.0
39.00	1565.0
39.90	312.0
40.90	123.0
41.90	147.0
42.90	144.0
44.00	789.0
45.00	465.0
45.90	230.0
47.00	780.0
47.90	381.0
49.00	2552.0
50.00	12109.0
51.00	3769.0
52.00	215.0
52.90	191.0
54.00	115.0
54.90	269.0
56.00	935.0
57.00	1772.0
58.00	165.0
60.00	726.0
61.00	3029.0
62.00	3393.0
63.00	2743.0
64.00	530.0
65.00	1034.0
65.90	173.0
66.90	264.0
68.00	6341.0
69.00	6152.0
70.00	517.0
71.90	345.0
72.90	2669.0
74.00	9635.0
75.00	29200.0
76.00	2307.0
76.90	332.0
77.90	310.0
78.90	2505.0
79.90	947.0
80.90	2642.0
81.90	751.0
83.00	121.0
86.00	162.0
86.90	2407.0
87.90	2079.0
91.00	352.0
92.00	1649.0
93.00	2637.0
94.00	6570.0
95.00	52912.0
96.00	3211.0
96.90	121.0
103.90	264.0
105.80	318.0
109.90	132.0
115.80	323.0
116.80	506.0
117.80	238.0
118.80	385.0
127.80	251.0
128.80	109.0
129.80	206.0
130.80	137.0
134.80	158.0
136.60	136.0
140.80	705.0
141.80	106.0
142.90	931.0
144.80	476.0
145.80	115.0
147.70	130.0
150.00	121.0
154.80	169.0
156.90	118.0
170.80	190.0
171.90	762.0
172.90	750.0
173.90	39880.0
174.90	3107.0
175.90	38136.0
176.90	2899.0
177.70	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	539.0
37.00	3134.0
38.00	3154.0
39.00	1443.0
39.90	285.0
40.80	129.0
41.90	141.0
42.90	124.0
44.00	842.0
45.00	524.0
45.90	181.0
47.00	693.0
47.90	458.0
49.00	2522.0
50.00	12107.0
51.00	3611.0
52.00	200.0
53.00	160.0
54.00	123.0
54.90	221.0
56.00	982.0
56.90	1637.0
58.00	164.0
60.00	741.0
61.00	2998.0
62.00	3331.0
63.00	2791.0
63.90	511.0
65.00	1048.0
65.90	176.0
67.00	230.0
68.00	6366.0
69.00	6146.0
70.00	520.0
71.90	324.0
72.90	2607.0
74.00	9934.0
75.00	29096.0
76.00	2226.0
76.90	288.0
78.00	345.0
78.90	2525.0
79.90	801.0
80.90	2731.0
81.90	748.0
82.90	117.0
86.00	150.0
86.90	2302.0
88.00	2053.0
91.00	358.0
92.00	1671.0
93.00	2512.0
94.00	6468.0
95.00	53008.0
96.00	3237.0
96.90	131.0
103.90	262.0
105.80	280.0
111.70	103.0
114.80	108.0
115.90	313.0
116.80	469.0
117.80	259.0
118.80	397.0
127.90	271.0
128.80	119.0
129.80	220.0
130.80	115.0
134.80	146.0
136.70	114.0
140.80	751.0
141.80	135.0
142.90	956.0
144.90	404.0
145.80	129.0
146.80	107.0
147.80	131.0
154.80	146.0
170.90	183.0
171.90	847.0
172.90	756.0
173.90	40376.0
174.90	3314.0
175.90	39032.0
176.90	2868.0
177.70	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
35.20	108.0
35.90	477.0
37.00	2870.0
38.00	2692.0
39.00	1310.0
39.80	297.0
40.70	140.0
41.90	115.0
43.10	106.0
44.00	816.0
45.00	538.0
45.90	137.0
47.10	567.0
48.00	506.0
49.00	2347.0
50.00	10972.0
51.00	3215.0
52.00	180.0
52.70	116.0
53.10	149.0
53.90	112.0
54.90	208.0
55.90	924.0
56.90	1459.0
58.00	132.0
60.00	614.0
61.00	2746.0
62.00	2946.0
63.00	2520.0
63.90	481.0
65.00	941.0
65.90	149.0
67.00	161.0
68.00	5767.0
69.00	5517.0
70.00	474.0
71.80	275.0
73.00	2269.0
74.00	9188.0
75.00	26064.0
76.00	2018.0
76.90	259.0
78.00	277.0
79.00	2367.0
79.90	644.0
80.90	2538.0
81.90	666.0
85.90	131.0
86.90	1948.0
88.00	1928.0
90.90	308.0
92.00	1472.0
92.90	2286.0
94.00	5904.0
95.00	47544.0
96.00	3072.0
97.00	129.0
103.90	267.0
105.80	253.0
111.60	111.0
114.90	115.0
115.90	268.0
116.80	433.0
117.80	260.0
118.80	391.0
127.90	245.0
128.70	112.0
129.80	216.0
134.90	117.0
140.80	662.0
141.80	137.0
142.90	921.0
144.90	339.0
145.80	111.0
146.90	106.0
147.90	167.0
154.70	137.0
170.90	164.0
171.80	796.0
172.90	685.0
173.90	36920.0
174.90	3070.0
175.90	35904.0
176.90	2432.0
177.80	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

Scan 2788 (10.055 min): VV019484.D
BFB62

m/z	Abundance
35.30	103.0
36.80	122.0
38.80	102.0
40.00	254.0
41.10	134.0
43.90	560.0
45.70	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62