

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120721\
 Data File : VW023828.D
 Acq On : 07 Dec 2021 17:20
 Operator : SY/MD
 Sample : M4879-01DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 08 01:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	174054	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	164774	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	90404	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36031	2.522	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	50.400%
7) Chloroethane-d5	1.568	69	31991	2.848	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	57.000%#
11) 1,1-Dichloroethene-d2	2.108	63	53765	2.135	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	42.800%#
20) 2-Butanone-d5	3.892	46	95547	55.625	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.260%
24) Chloroform-d	4.346	84	86767	3.487	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.800%#
26) 1,2-Dichloroethane-d4	5.031	65	42033	3.616	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.400%
32) Benzene-d6	5.050	84	167806	3.739	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	74.800%
36) 1,2-Dichloropropane-d6	6.069	67	49803	3.958	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.200%
41) Toluene-d8	7.313	98	155527	3.708	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.200%
43) trans-1,3-Dichloroprop...	7.622	79	19158	3.777	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.600%
46) 2-Hexanone-d5	8.088	63	80156	47.564	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.120%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	35032	3.869	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	77.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	64365	4.027	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	80.600%
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	1245	0.087	ug/L	97
5) Vinyl chloride	1.314	62	1593	0.106	ug/L #	35
6) Bromomethane	1.523	94	611	0.071	ug/L	94
8) Chloroethane	1.593	64	916	0.096	ug/L #	54
12) 1,1-Dichloroethene	2.114	96	1062	0.091	ug/L #	1
14) Carbon disulfide	2.294	76	2353	0.060	ug/L #	94
16) Methylene chloride	2.507	84	11222	0.674	ug/L	95
17) Methyl tert-butyl Ether	2.767	73	4993	0.209	ug/L #	1
18) trans-1,2-Dichloroethene	2.764	96	1394	0.105	ug/L	96
19) 1,1-Dichloroethane	3.195	63	1155	0.052	ug/L #	86
22) cis-1,2-Dichloroethene	3.908	96	29839	2.342	ug/L	100
30) Cyclohexane	4.677	56	8817	0.491	ug/L	95
33) Benzene	5.101	78	40143	0.855	ug/L	100
34) Trichloroethene	5.915	95	20042	1.593	ug/L	95
35) Methylcyclohexane	6.130	83	6982	0.356	ug/L	93
37) 1,2-Dichloropropane	6.185	63	852	0.076	ug/L #	84
38) Bromodichloromethane	6.519	83	1112	0.073	ug/L #	80
42) Toluene	7.394	91	13272	0.261	ug/L	99
45) 1,1,2-Trichloroethane	7.844	97	569	0.074	ug/L #	71

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
 Data File : VV023828.D
 Acq On : 07 Dec 2021 17:20
 Operator : SY/MD
 Sample : M4879-01DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 08 01:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


47) Tetrachloroethene	7.973	164	61510	5.370	ug/L	98
49) Dibromochloromethane	7.973	129	54628	5.156	ug/L #	11
50) 1,2-Dibromoethane	8.362	107	416	0.055	ug/L #	95
52) Ethylbenzene	9.014	91	24527	0.461	ug/L	98
53) m,p-xylene	9.140	106	18003	0.849	ug/L	98
54) o-xylene	9.548	106	3448	0.171	ug/L	87
55) Styrene	9.574	104	2050	0.060	ug/L #	77
60) Isopropylbenzene	9.934	105	7214	0.134	ug/L #	96
61) 1,2,3-Trichloropropane	10.281	75	415	0.065	ug/L #	6
62) 1,3,5-Trimethylbenzene	10.538	105	26929	0.600	ug/L	100
63) 1,2,4-Trimethylbenzene	10.915	105	110117	2.479	ug/L	99
64) 1,3-Dichlorobenzene	11.185	146	2009	0.073	ug/L	89
65) 1,4-Dichlorobenzene	11.278	146	1910	0.069	ug/L	97
67) 1,2-Dichlorobenzene	11.644	146	1879	0.074	ug/L #	88
68) 1,2-Dibromo-3-chloropr...	12.419	75	97	0.076	ug/L #	1
70) 1,2,4-trichlorobenzene	13.265	180	1127	0.067	ug/L #	66
71) Naphthalene	13.503	128	16191	0.720	ug/L	98
72) 1,2,3-Trichlorobenzene	13.744	180	1019	0.070	ug/L #	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023828.D
Acq On : 07 Dec 2021 17:20
Operator : SY/MD
Sample : M4879-01DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 08 01:16:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration




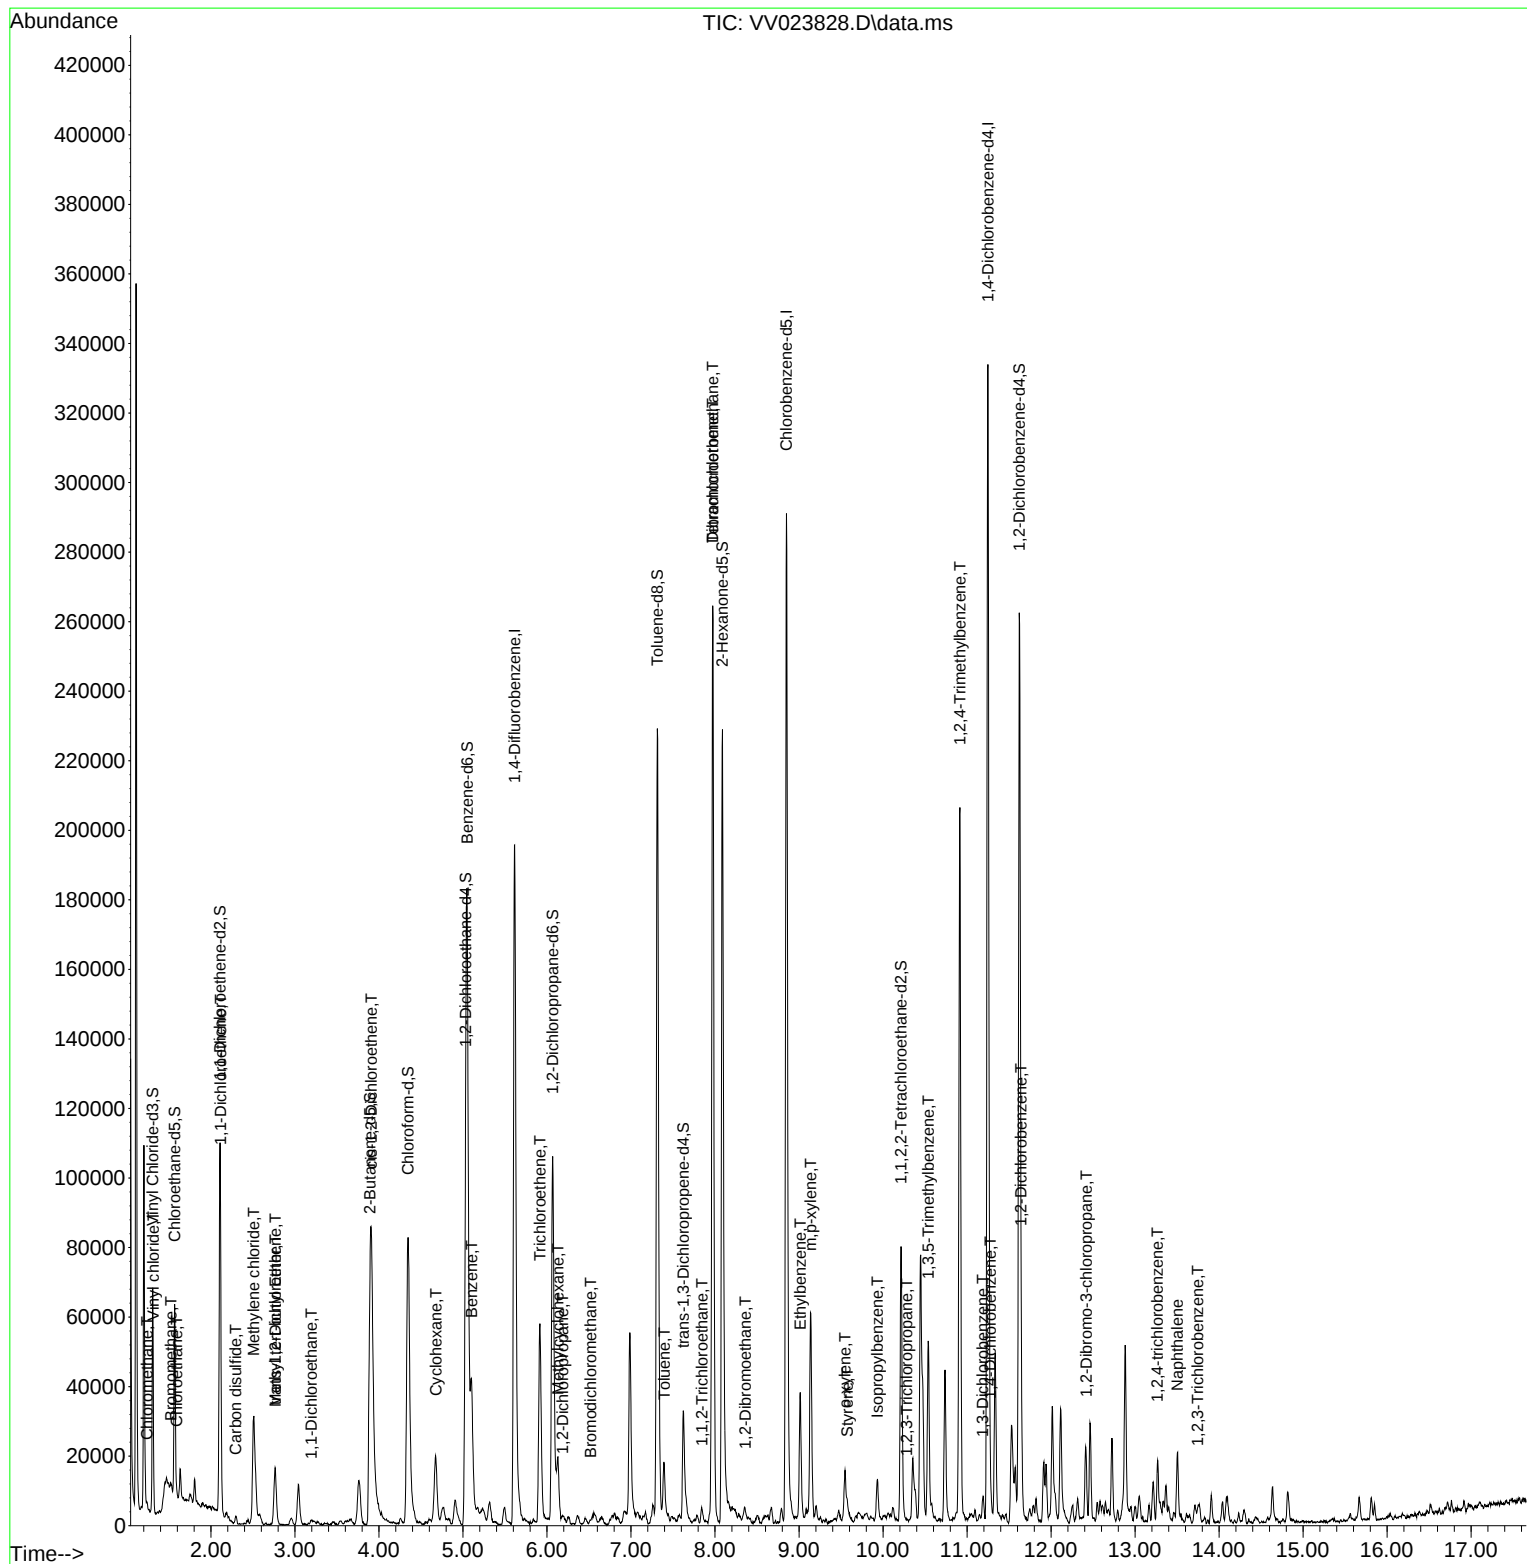


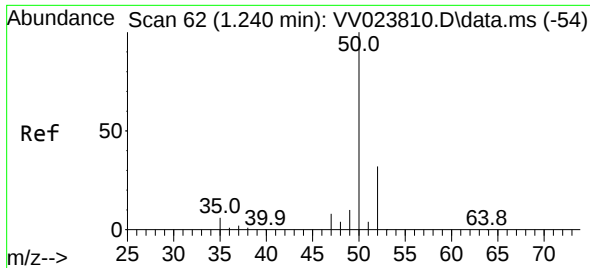

#3
Chloromethane
Concen: 0.087 ug/L
RT: 1.240 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 50 Resp: 1245
Ion Ratio Lower Upper
50 100
52 30.1 22.0 41.0

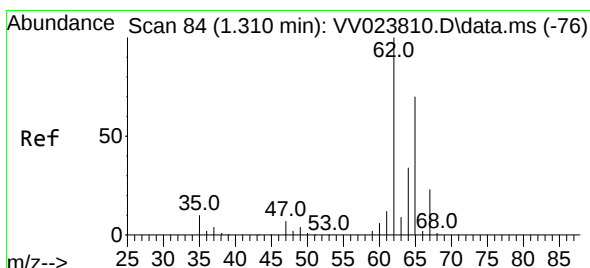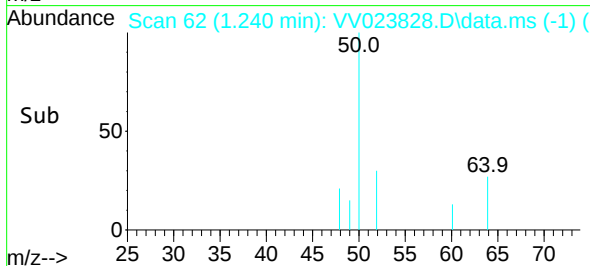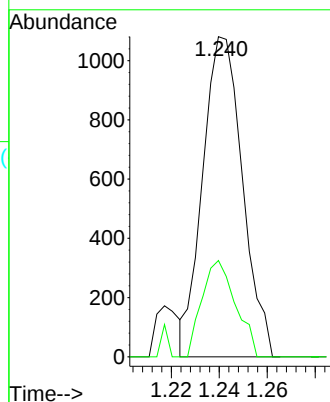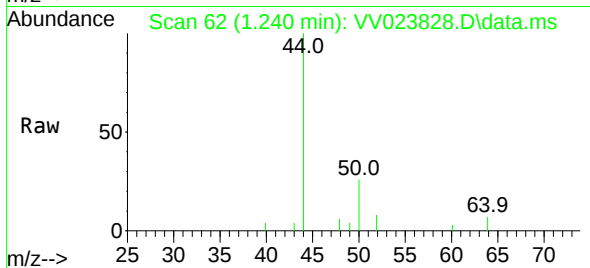

#5
Vinyl chloride
Concen: 0.106 ug/L
RT: 1.314 min Scan# 85
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20


Tgt Ion: 62 Resp: 1593
Ion Ratio Lower Upper
62 100
64 68.1 22.4 41.6#

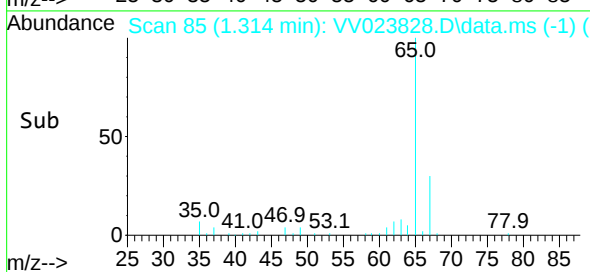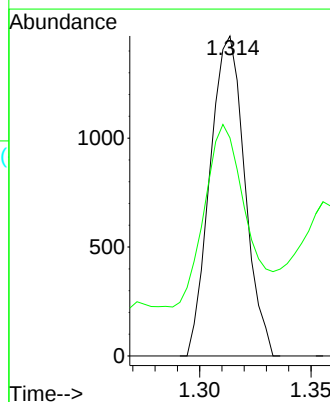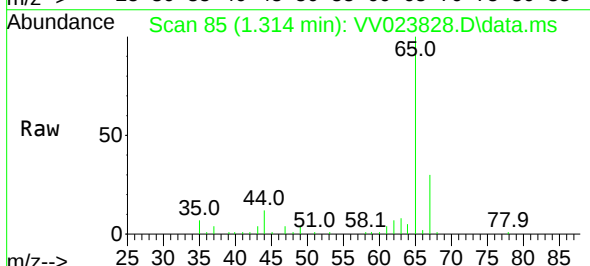






#6
Bromomethane
Concen: 0.071 ug/L
RT: 1.523 min Scan# 11
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



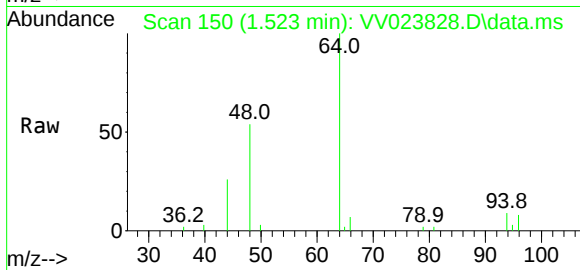



Tgt Ion: 94 Resp: 611
Ion Ratio Lower Upper
94 100
96 88.5 66.2 123.0

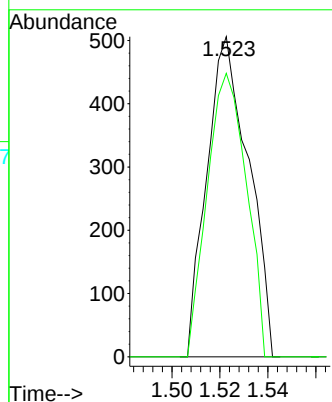

#8
Chloroethane
Concen: 0.096 ug/L
RT: 1.593 min Scan# 172
Delta R.T. 0.010 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 64 Resp: 916
Ion Ratio Lower Upper
64 100
66 5.6 21.4 39.8#




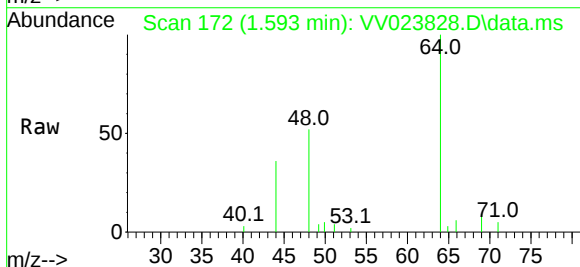




#12
1,1-Dichloroethene
Concen: 0.091 ug/L
RT: 2.114 min Scan# 311
Delta R.T. -0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 96 Resp: 1062
Ion Ratio Lower Upper
96 100
61 709.7 116.1 215.5#
63 4861.7 79.4 147.4#

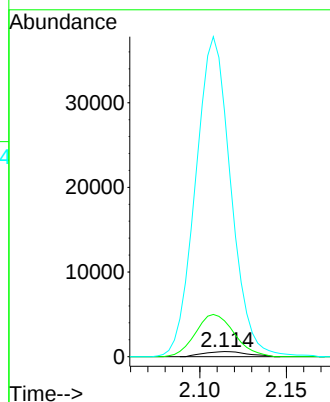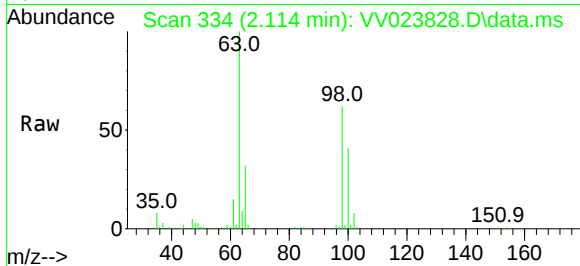

#14
Carbon disulfide
Concen: 0.060 ug/L
RT: 2.294 min Scan# 390
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20


Tgt Ion: 76 Resp: 2353
Ion Ratio Lower Upper
76 100
78 11.4 7.5 11.3#

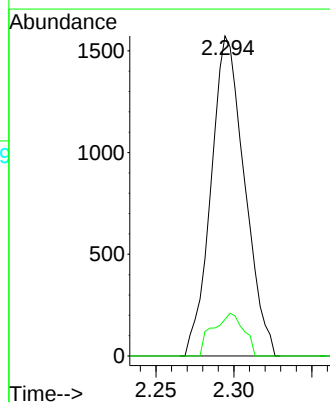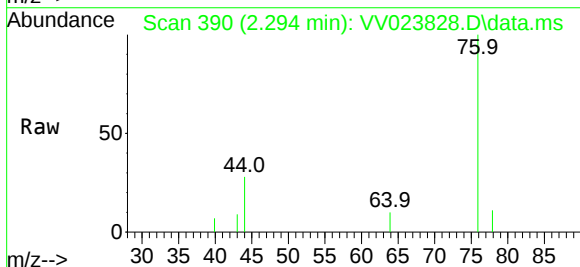






#16
Methylene chloride
Concen: 0.674 ug/L
RT: 2.507 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



Tgt Ion: 84 Resp: 11222




Ion	Ratio	Lower	Upper
84	100		
86	70.3	42.6	79.0
49	115.4	79.7	147.9

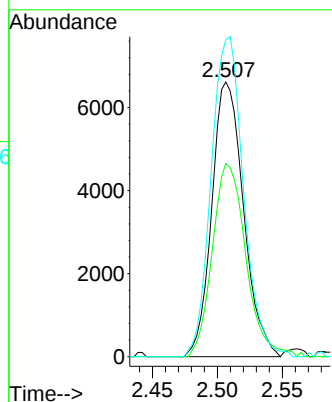


#17
Methyl tert-butyl Ether
Concen: 0.209 ug/L
RT: 2.767 min Scan# 537
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 73 Resp: 4993


Ion	Ratio	Lower	Upper
73	100		
43	45.6	15.5	23.3#
57	122.9	17.1	25.7#

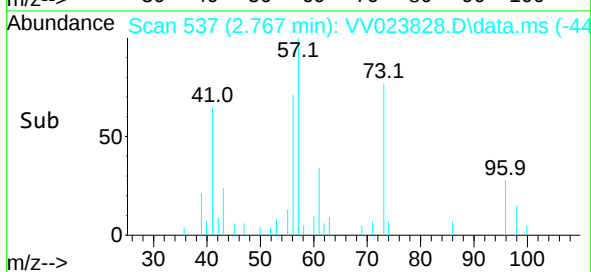






#18
trans-1,2-Dichloroethene
Concen: 0.105 ug/L
RT: 2.764 min Scan# 51
Delta R.T. 0.006 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :

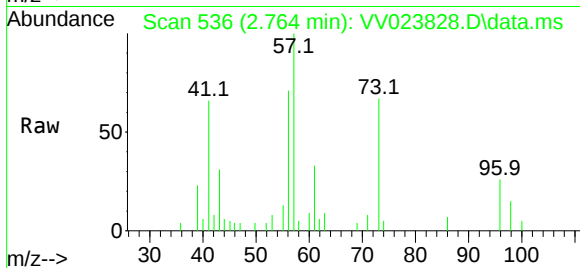

Tgt Ion: 96 Resp: 1394




Ion	Ratio	Lower	Upper
96	100		
61	127.3	88.2	163.8
98	55.9	44.9	83.5




#19
1,1-Dichloroethane
Concen: 0.052 ug/L
RT: 3.195 min Scan# 670
Delta R.T. 0.010 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 63 Resp: 1155

Ion	Ratio	Lower	Upper
63	100		
65	29.9	22.3	41.3
83	0.0	10.7	19.9

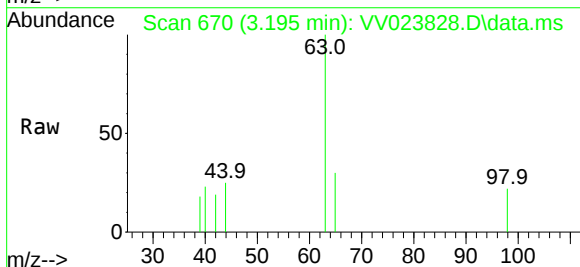



#22

cis-1,2-Dichloroethene

Concen: 2.342 ug/L

RT: 3.908 min Scan# 892

Delta R.T. 0.000 min


Lab File: VV023828.D

Acq: 07 Dec 2021 17:20

Instrument :

MSVOA_V

ClientSampleId :

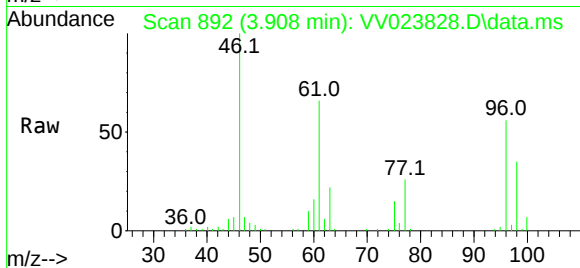




Tgt Ion: 96 Resp: 29839

Ion Ratio Lower Upper

96 100

61 119.2 83.4 154.8

68 0.0 0.0 0.0

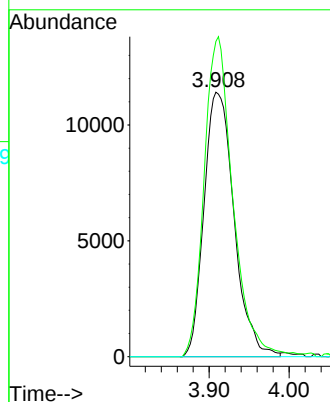

#30

Cyclohexane

Concen: 0.491 ug/L

RT: 4.677 min Scan# 1131

Delta R.T. 0.003 min

Lab File: VV023828.D

Acq: 07 Dec 2021 17:20




Tgt Ion: 56 Resp: 8817


Ion Ratio Lower Upper

56 100

69 33.8 24.8 37.2

84 90.2 75.9 113.9


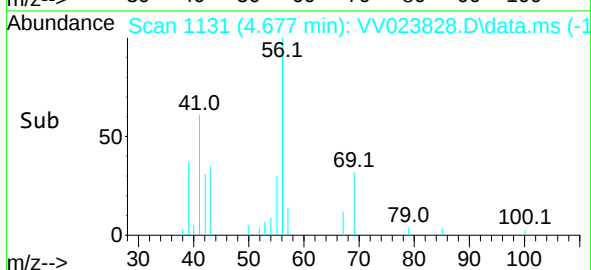
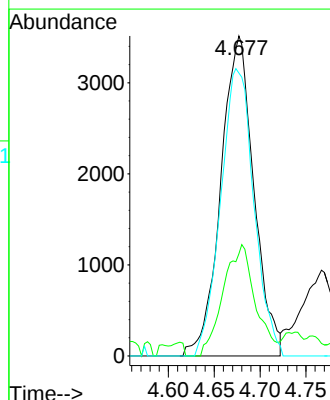
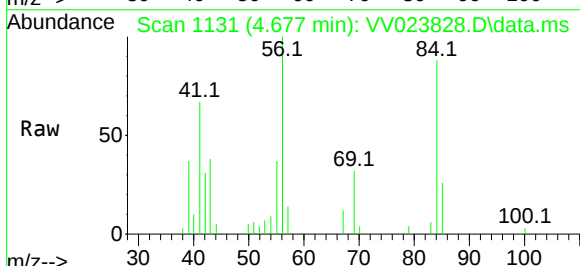


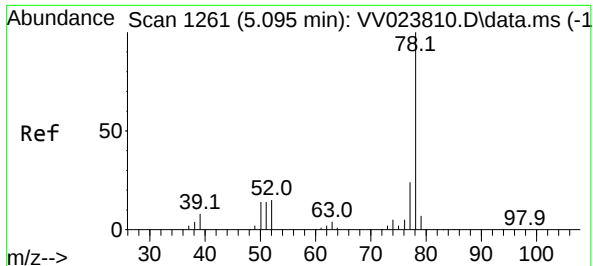

#33
Benzene
Concen: 0.855 ug/L
RT: 5.101 min Scan# 1263
Delta R.T. 0.006 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :




Tgt Ion: 78 Resp: 40143

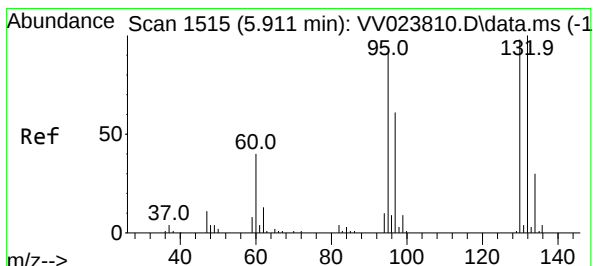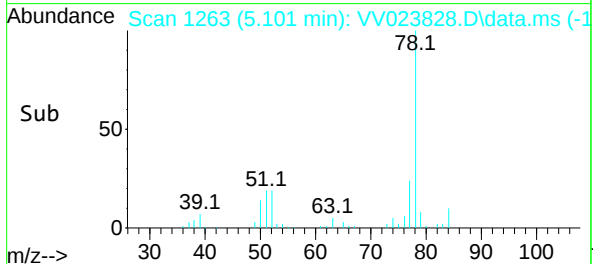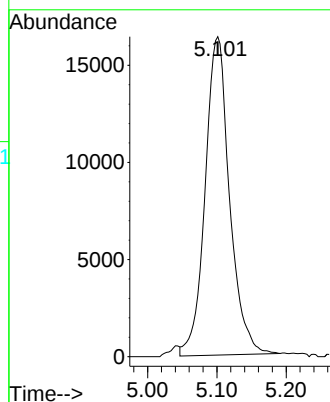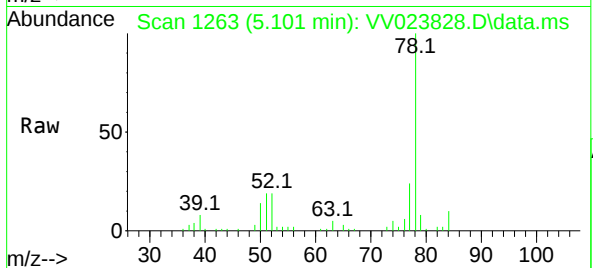


#34
Trichloroethene
Concen: 1.593 ug/L
RT: 5.915 min Scan# 1516
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 95 Resp: 20042

Ion	Ratio	Lower	Upper
95	100		
97	65.8	45.2	84.0
132	114.9	76.1	141.3
130	115.1	75.4	140.0


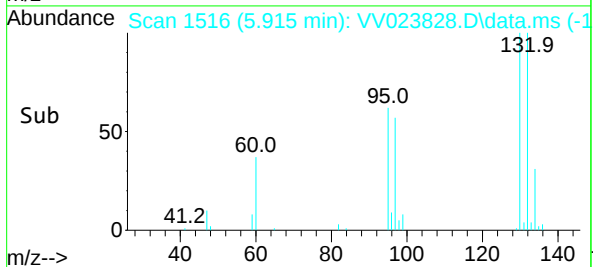
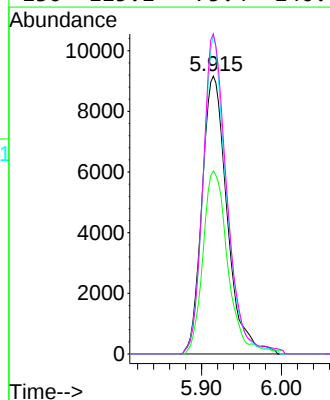
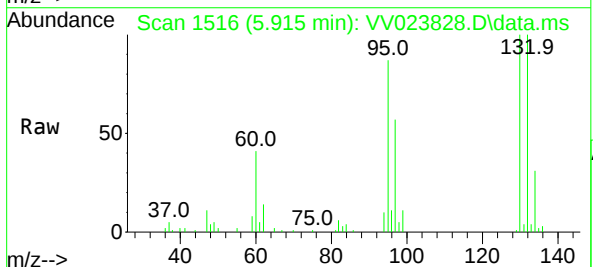




#35
Methylcyclohexane
Concen: 0.356 ug/L
RT: 6.130 min Scan# 11
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 83 Resp: 6982
Ion Ratio Lower Upper
83 100
55 84.0 60.2 90.2
98 50.4 41.0 61.4

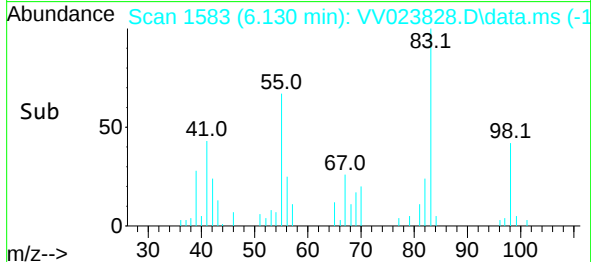

#37
1,2-Dichloropropane
Concen: 0.076 ug/L
RT: 6.185 min Scan# 1600
Delta R.T. 0.016 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20


Tgt Ion: 63 Resp: 852
Ion Ratio Lower Upper
63 100
112 0.0 4.3 6.5#

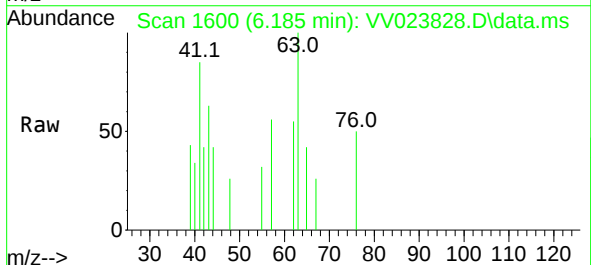






#38
Bromodichloromethane
Concen: 0.073 ug/L
RT: 6.519 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



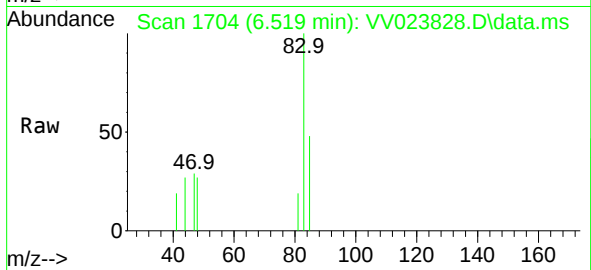



Tgt Ion: 83 Resp: 1112
Ion Ratio Lower Upper
83 100
85 48.3 44.0 81.8
127 0.0 8.6 12.8#

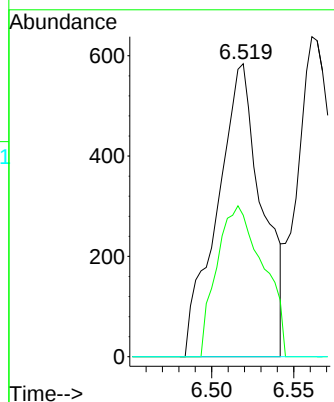

#42
Toluene
Concen: 0.261 ug/L
RT: 7.394 min Scan# 1976
Delta R.T. 0.010 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 91 Resp: 13272
Ion Ratio Lower Upper
91 100
92 58.7 41.5 77.1

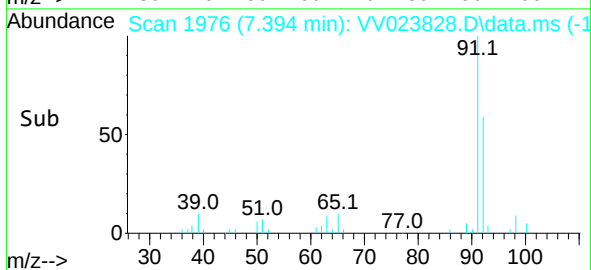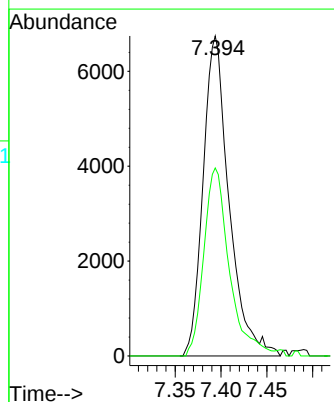



#45

1,1,2-Trichloroethane

Concen: 0.074 ug/L

RT: 7.844 min Scan# 2114

Delta R.T. 0.006 min

Lab File: VV023828.D

Acq: 07 Dec 2021 17:20

Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion: 97 Resp: 569





Ion Ratio Lower Upper

97 100

99 53.1 43.1 80.1

83 121.8 57.9 107.5#

85 35.4 38.0 70.6#

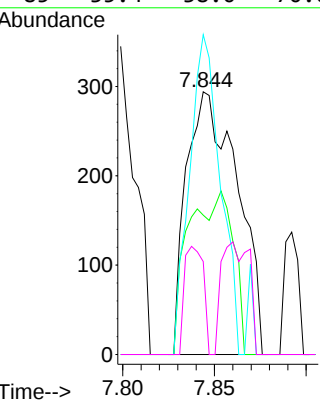

#47

Tetrachloroethene

Concen: 5.370 ug/L

RT: 7.973 min Scan# 2156

Delta R.T. 0.000 min

Lab File: VV023828.D

Acq: 07 Dec 2021 17:20

Tgt Ion: 164 Resp: 61510




Ion Ratio Lower Upper


164 100

129 92.4 62.6 116.2

131 88.7 61.0 113.4


166 123.0 87.3 162.1

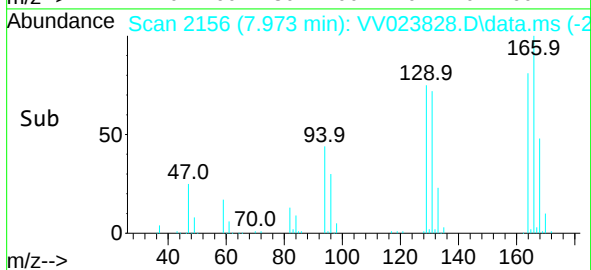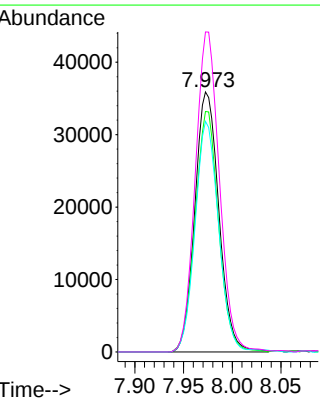



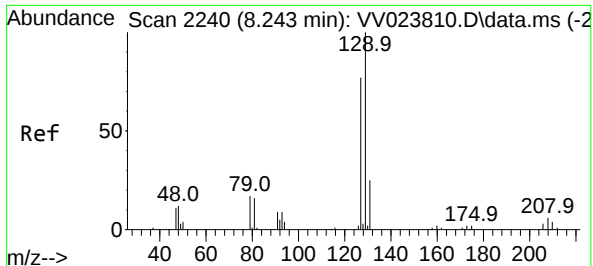


#49
Dibromochloromethane
Concen: 5.156 ug/L
RT: 7.973 min Scan# 2156
Delta R.T. -0.270 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



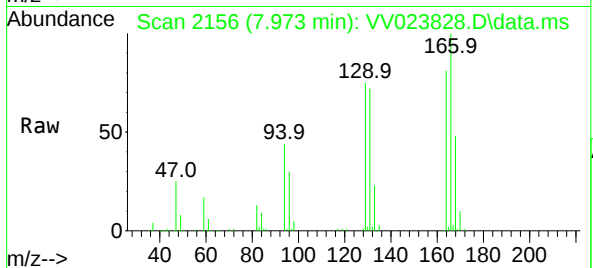



Tgt Ion:129 Resp: 54628
Ion Ratio Lower Upper
129 100
127 0.0 53.5 99.3#

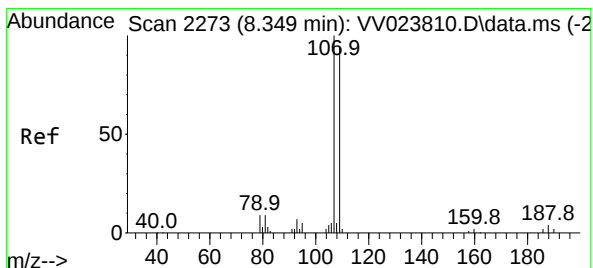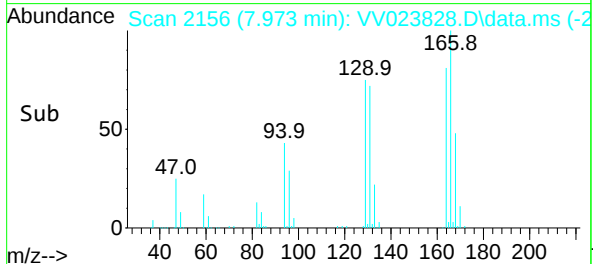

#50
1,2-Dibromoethane
Concen: 0.055 ug/L
RT: 8.362 min Scan# 2277
Delta R.T. 0.013 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion:107 Resp: 416
Ion Ratio Lower Upper
107 100
109 85.2 62.5 116.1
188 0.0 3.4 5.2#


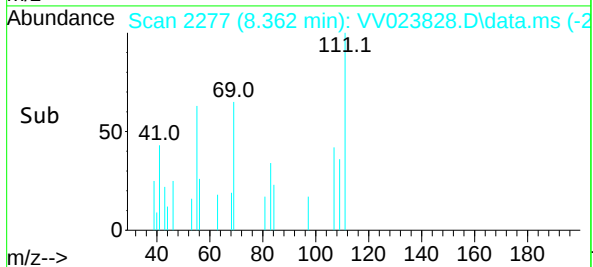

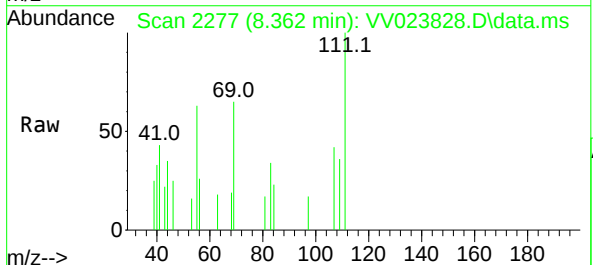




#52
Ethylbenzene
Concen: 0.461 ug/L
RT: 9.014 min Scan# 2479
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 91 Resp: 24527
Ion Ratio Lower Upper
91 100
106 32.8 22.0 41.0

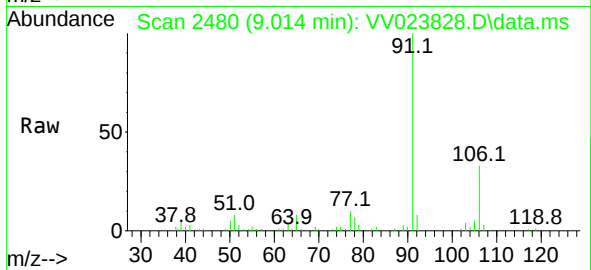

#53
m,p-xylene
Concen: 0.849 ug/L
RT: 9.140 min Scan# 2519
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 106 Resp: 18003
Ion Ratio Lower Upper
106 100
91 196.3 139.5 259.1









#54
o-xylene
Concen: 0.171 ug/L
RT: 9.548 min Scan# 2644
Delta R.T. 0.006 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:106 Resp: 3448
Ion Ratio Lower Upper
106 100
91 191.5 147.9 274.7



#55
Styrene
Concen: 0.060 ug/L
RT: 9.574 min Scan# 2654
Delta R.T. 0.016 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20


Tgt Ion:104 Resp: 2050
Ion Ratio Lower Upper
104 100
78 59.5 31.0 57.6#

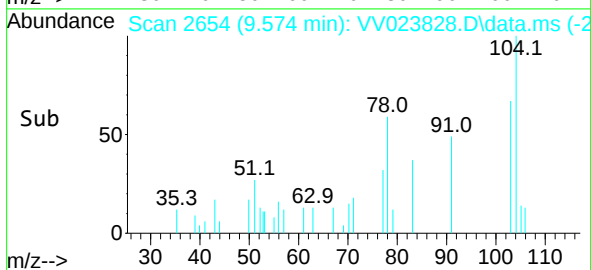






#60
Isopropylbenzene
Concen: 0.134 ug/L
RT: 9.934 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



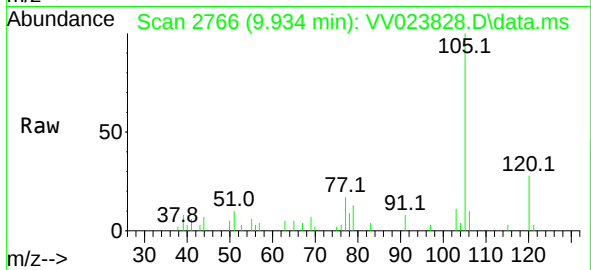



Tgt Ion:105 Resp: 7214
Ion Ratio Lower Upper
105 100
120 27.2 21.4 32.0
77 19.6 12.2 18.4#



#61
1,2,3-Trichloropropane
Concen: 0.065 ug/L
RT: 10.281 min Scan# 2874
Delta R.T. 0.010 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion: 75 Resp: 415
Ion Ratio Lower Upper
75 100
77 123.1 26.4 39.6#
110 15.2 34.2 51.2#









#62
 1,3,5-Trimethylbenzene
 Concen: 0.600 ug/L
 RT: 10.538 min Scan# 2954
 Delta R.T. 0.000 min
 Lab File: VV023828.D
 Acq: 07 Dec 2021 17:20




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion:105 Resp: 26929
 Ion Ratio Lower Upper
 105 100
 120 49.9 40.1 60.1

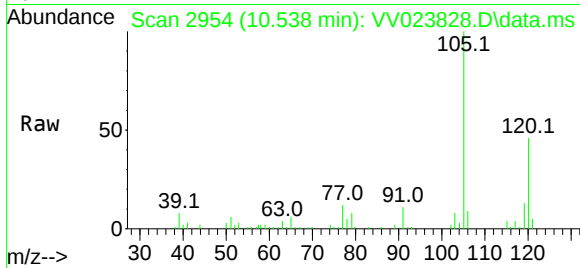

#63
 1,2,4-Trimethylbenzene
 Concen: 2.479 ug/L
 RT: 10.915 min Scan# 3071
 Delta R.T. 0.003 min
 Lab File: VV023828.D
 Acq: 07 Dec 2021 17:20


Tgt Ion:105 Resp: 110117
 Ion Ratio Lower Upper
 105 100
 120 46.7 36.7 55.1

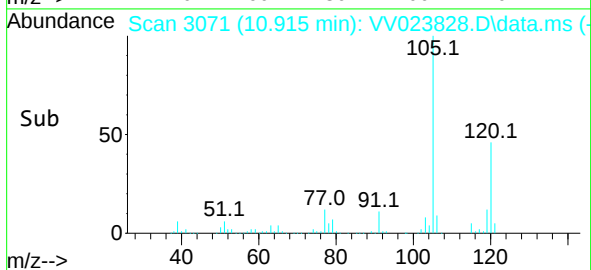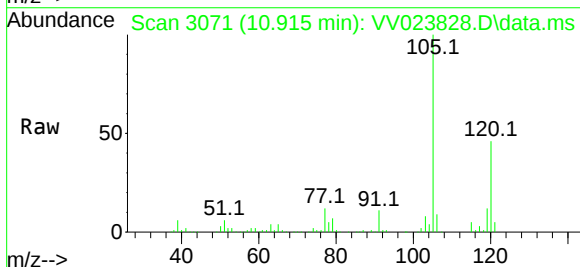






#64
1,3-Dichlorobenzene
Concen: 0.073 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.006 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Instrument :
MSVOA_V
ClientSampleId :



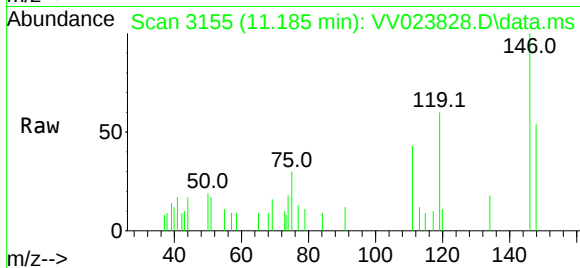



Tgt Ion:146 Resp: 2009
Ion Ratio Lower Upper
146 100
111 42.9 26.3 48.9
148 54.5 44.4 82.5



#65
1,4-Dichlorobenzene
Concen: 0.069 ug/L
RT: 11.278 min Scan# 3184
Delta R.T. 0.006 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20

Tgt Ion:146 Resp: 1910
Ion Ratio Lower Upper
146 100
111 39.7 25.6 47.6
148 65.9 44.8 83.2




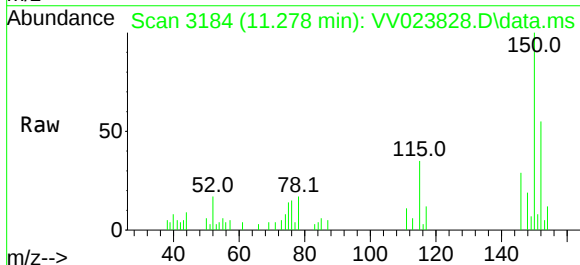




#67
 1,2-Dichlorobenzene
 Concen: 0.074 ug/L
 RT: 11.644 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV023828.D
 Acq: 07 Dec 2021 17:20




Instrument :
 MSVOA_V
 ClientSampleId :


Tgt Ion:146 Resp: 1879
 Ion Ratio Lower Upper
 146 100
 111 39.2 31.9 47.9
 148 48.0 50.5 75.7#

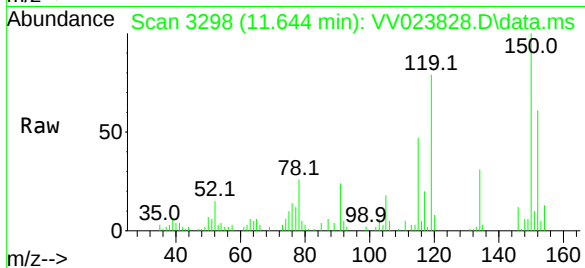

#68
 1,2-Dibromo-3-chloropropane
 Concen: 0.076 ug/L
 RT: 12.419 min Scan# 3539
 Delta R.T. -0.006 min
 Lab File: VV023828.D
 Acq: 07 Dec 2021 17:20

Tgt Ion: 75 Resp: 97
 Ion Ratio Lower Upper
 75 100
 155 0.0 71.7 107.5#
 157 0.0 103.3 154.9#


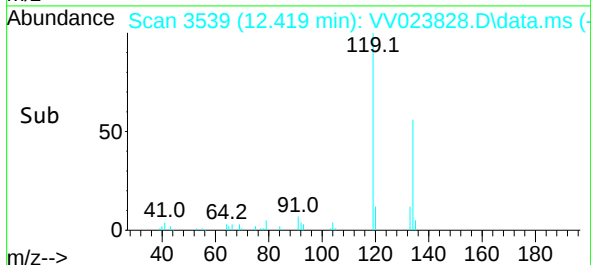
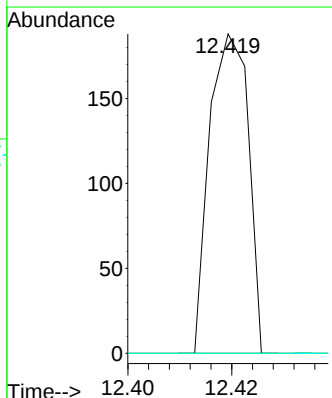
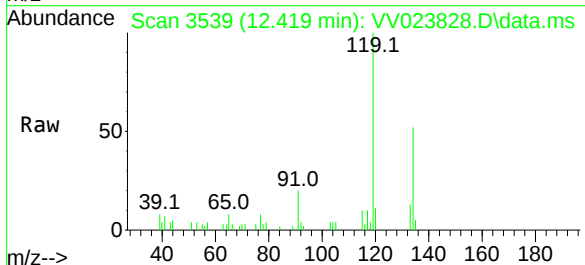




#70
1,2,4-trichlorobenzene
Concen: 0.067 ug/L
RT: 13.265 min Scan# 3802
Delta R.T. 0.003 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:180 Resp: 1127
Ion Ratio Lower Upper
180 100
182 78.4 74.4 111.6
145 79.3 23.3 34.9#

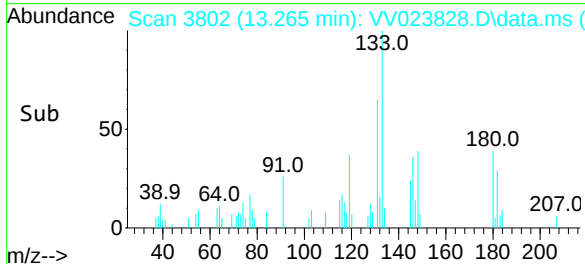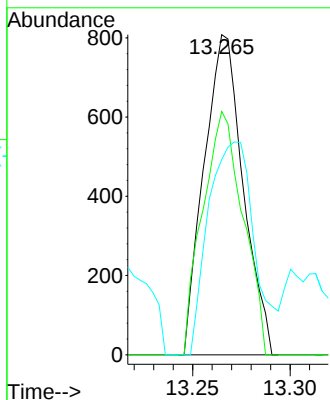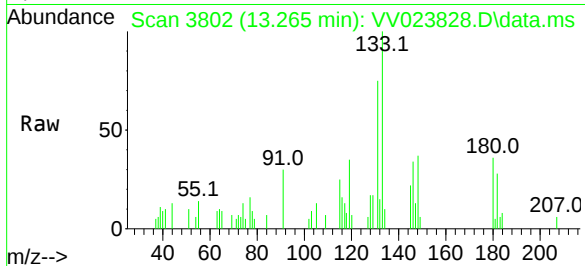

#71
Naphthalene
Concen: 0.720 ug/L
RT: 13.503 min Scan# 3876
Delta R.T. 0.000 min
Lab File: VV023828.D
Acq: 07 Dec 2021 17:20


Tgt Ion:128 Resp: 16191
Ion Ratio Lower Upper
128 100
129 10.7 9.0 13.4
127 11.6 10.2 15.4

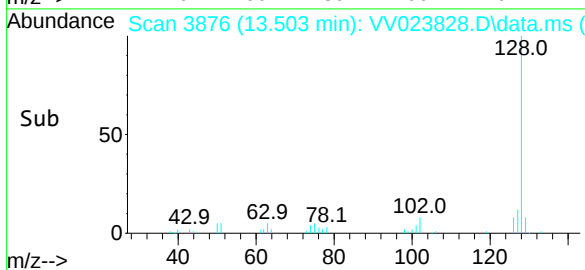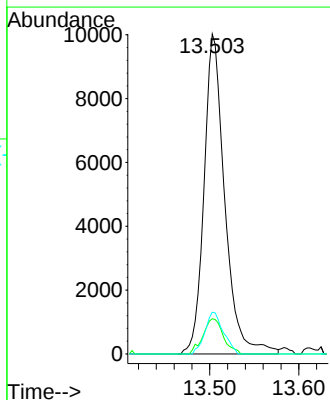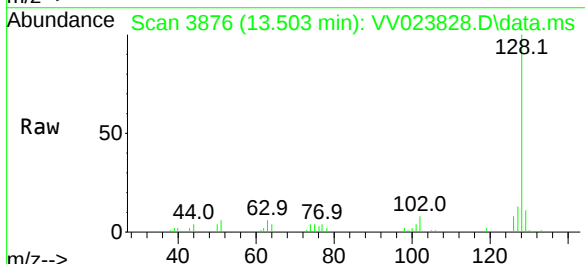



#72
 1,2,3-Trichlorobenzene
 Concen: 0.070 ug/L
 RT: 13.744 min Scan# 3951
 Delta R.T. 0.000 min
 Lab File: VV023828.D
 Acq: 07 Dec 2021 17:20

Instrument :
 MSVOA_V
 ClientSampleId :

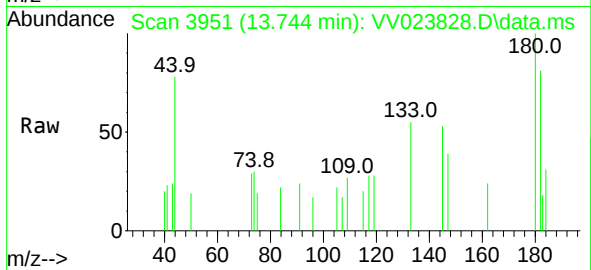

Tgt Ion:180 Resp: 1019
 Ion Ratio Lower Upper
 180 100
 182 92.1 76.8 115.2
 145 47.5 25.8 38.6#

