

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120721\
 Data File : VW023827.D
 Acq On : 07 Dec 2021 16:51
 Operator : SY/MD
 Sample : M4879-03 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

Quant Time: Dec 08 01:16:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144636	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	136120	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	71553	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	33250	2.800	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	56.000%
7) Chloroethane-d5	1.568	69	29668	3.179	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	63.600%#
11) 1,1-Dichloroethene-d2	2.108	63	51081	2.441	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.800%#
20) 2-Butanone-d5	3.912	46	87451	61.267	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.540%
24) Chloroform-d	4.349	84	87439	4.229	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%
26) 1,2-Dichloroethane-d4	5.034	65	42468	4.397	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
32) Benzene-d6	5.050	84	166667	4.495	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
36) 1,2-Dichloropropane-d6	6.072	67	49086	4.722	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.400%
41) Toluene-d8	7.317	98	155237	4.481	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	7.625	79	19807	4.727	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.600%
46) 2-Hexanone-d5	8.092	63	88025	63.228	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	126.460%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37615	5.028	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	64857	5.127	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.600%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.510	84	4665	0.337	ug/L	95
22) cis-1,2-Dichloroethene	3.918	96	1064	0.101	ug/L	84
34) Trichloroethene	5.924	95	1366	0.131	ug/L	86
42) Toluene	7.400	91	4514	0.107	ug/L	92
47) Tetrachloroethene	7.976	164	117624	12.431	ug/L	98
52) Ethylbenzene	9.018	91	6055	0.138	ug/L	98
53) m,p-xylene	9.143	106	3188	0.182	ug/L	89
54) o-xylene	9.548	106	1213	0.073	ug/L	91
60) Isopropylbenzene	9.940	105	2315	0.054	ug/L #	94
62) 1,3,5-Trimethylbenzene	10.538	105	4852	0.136	ug/L	94
63) 1,2,4-Trimethylbenzene	10.915	105	14986	0.426	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023827.D
Acq On : 07 Dec 2021 16:51
Operator : SY/MD
Sample : M4879-03 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G30

Quant Time: Dec 08 01:16:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration




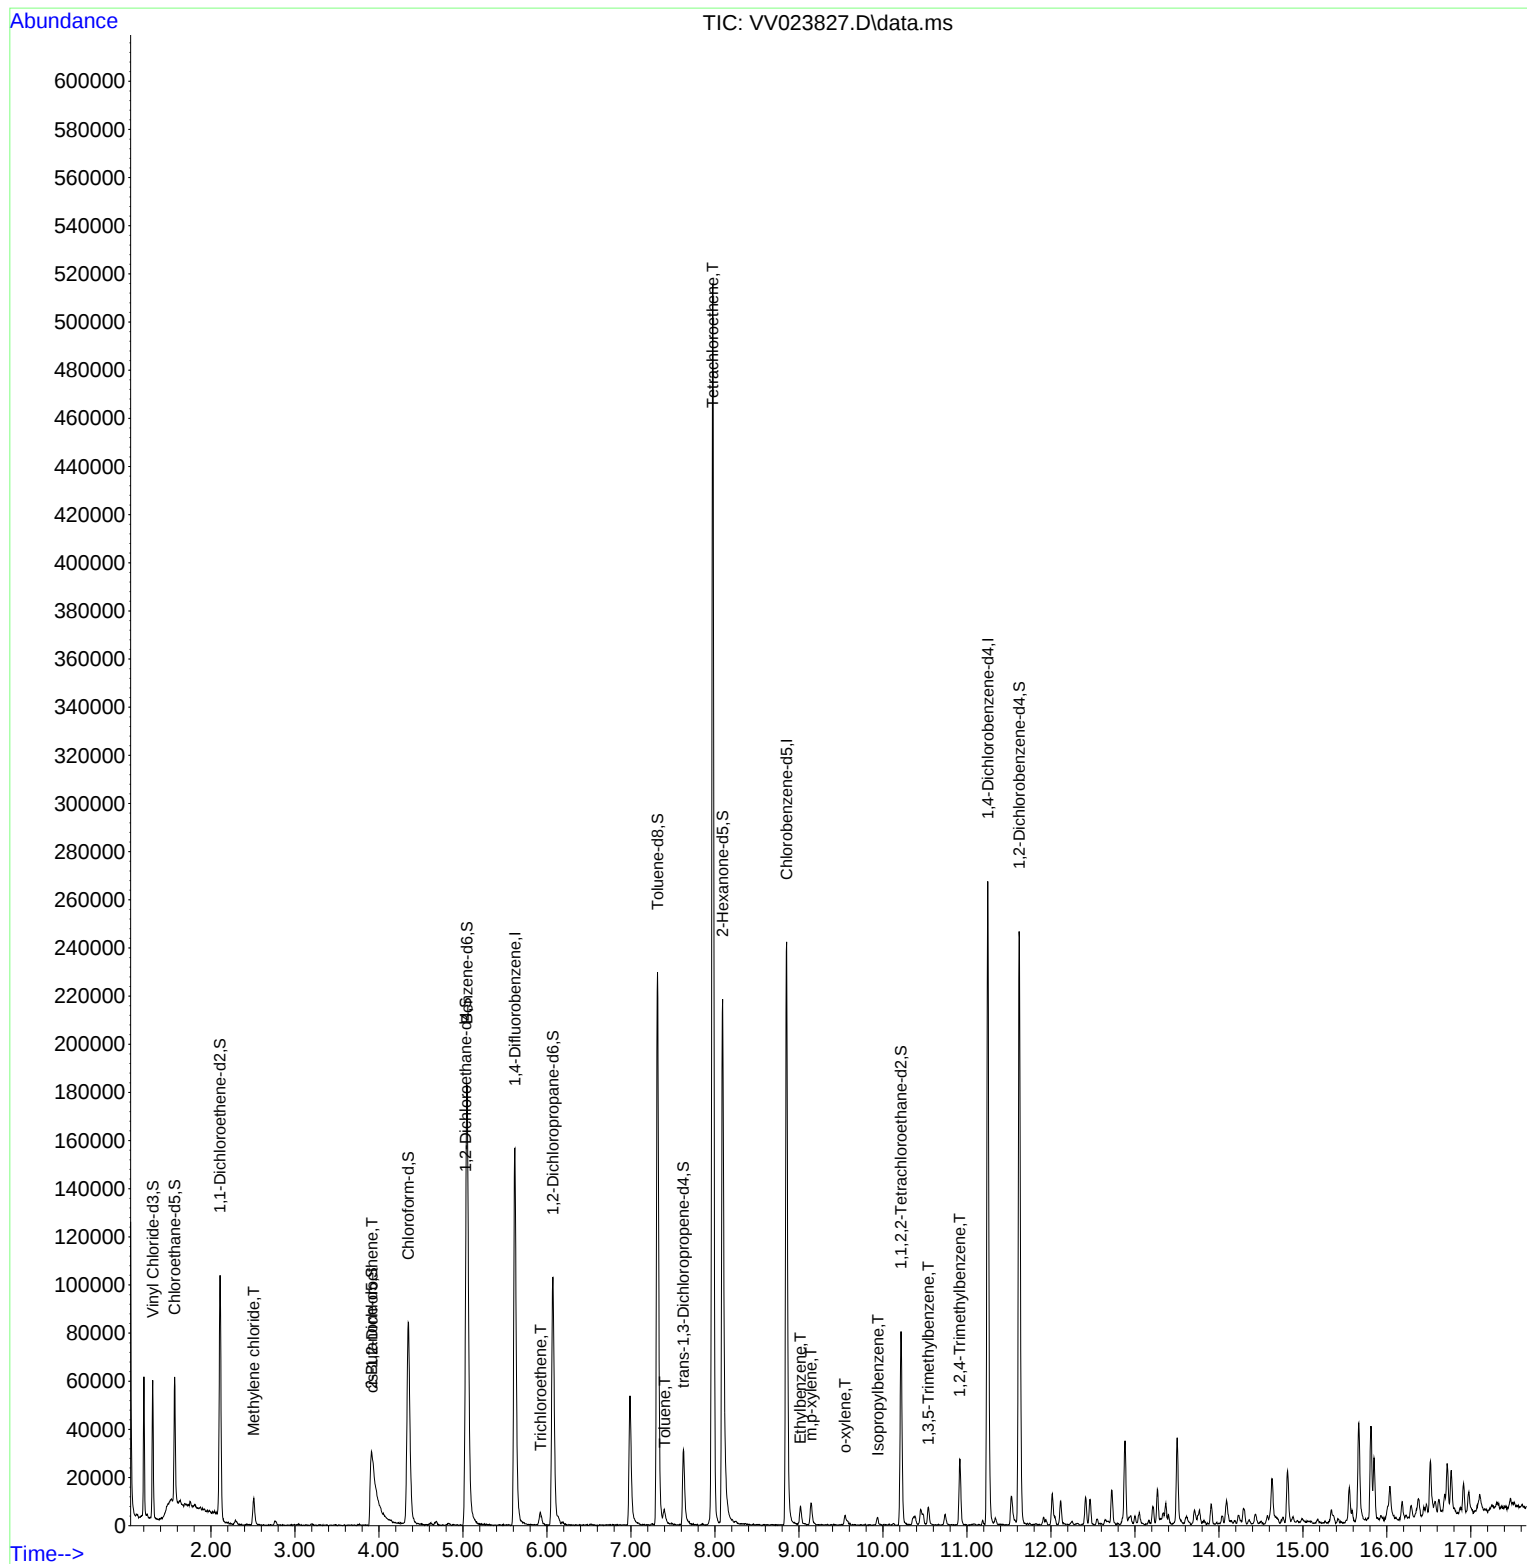


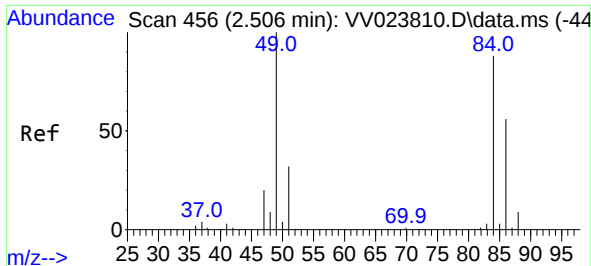

#16
Methylene chloride
Concen: 0.337 ug/L
RT: 2.510 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV023827.D
Acq: 07 Dec 2021 16:51




Instrument :
MSVOA_V
ClientSampleId :
C0G30


Tgt Ion: 84 Resp: 4665
Ion Ratio Lower Upper
84 100
86 63.5 42.6 79.0
49 107.2 79.7 147.9

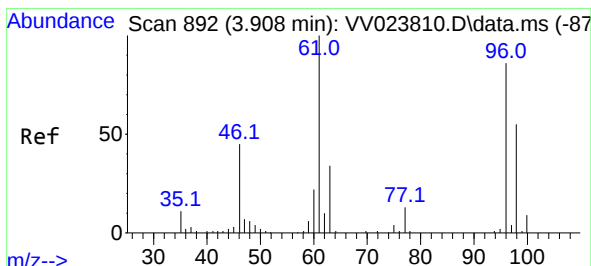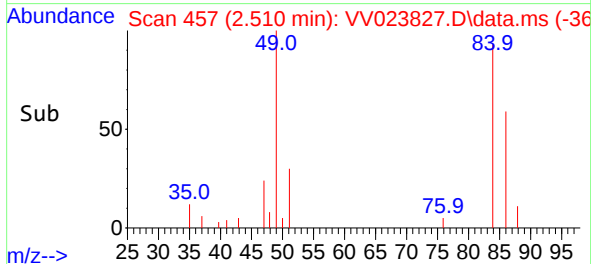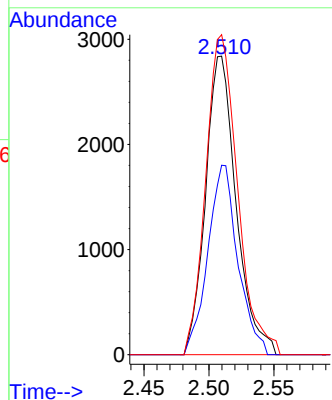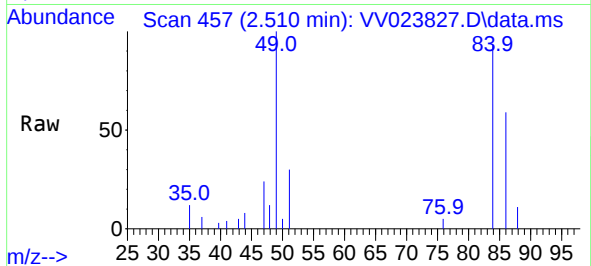

#22
cis-1,2-Dichloroethene
Concen: 0.101 ug/L
RT: 3.918 min Scan# 895
Delta R.T. 0.010 min
Lab File: VV023827.D
Acq: 07 Dec 2021 16:51

Tgt Ion: 96 Resp: 1064
Ion Ratio Lower Upper
96 100
61 101.7 83.4 154.8
68 0.0 0.0 0.0

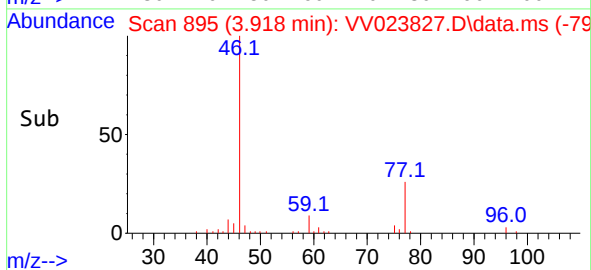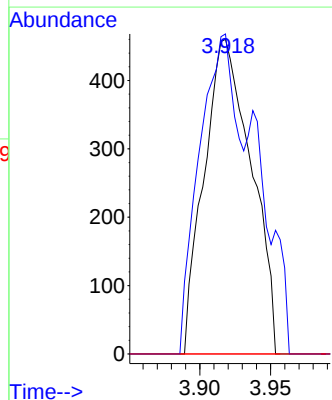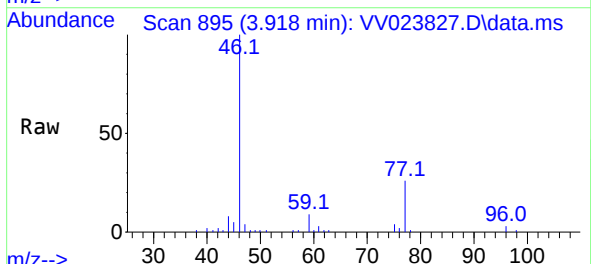




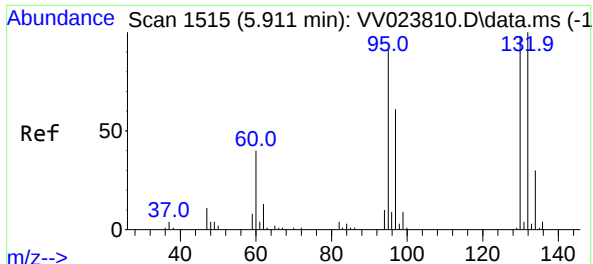


#34
 Trichloroethene
 Concen: 0.131 ug/L
 RT: 5.924 min Scan# 11
 Delta R.T. 0.013 min
 Lab File: VV023827.D
 Acq: 07 Dec 2021 16:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

Tgt Ion: 95 Resp: 1366




Ion	Ratio	Lower	Upper
95	100		
97	72.5	45.2	84.0
132	98.2	76.1	141.3
130	86.2	75.4	140.0

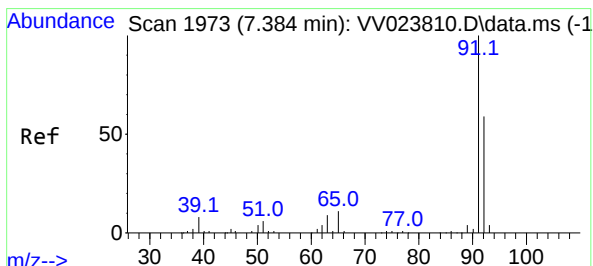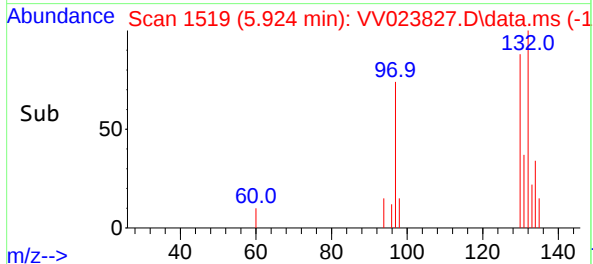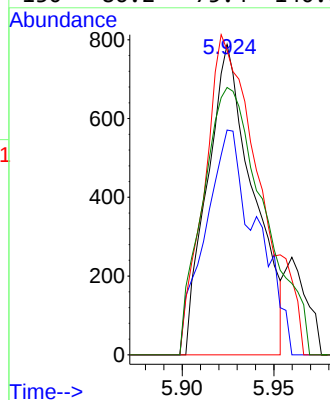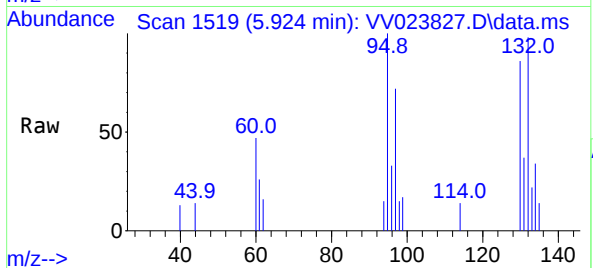


#42
 Toluene
 Concen: 0.107 ug/L
 RT: 7.400 min Scan# 1978
 Delta R.T. 0.016 min
 Lab File: VV023827.D
 Acq: 07 Dec 2021 16:51

Tgt Ion: 91 Resp: 4514

Ion	Ratio	Lower	Upper
91	100		
92	53.3	41.5	77.1

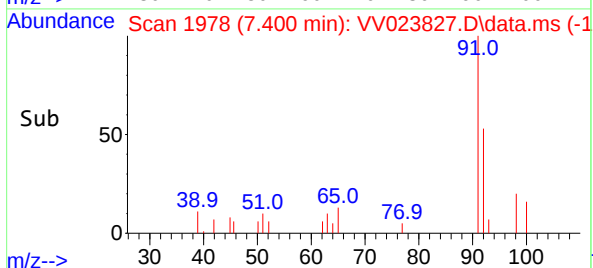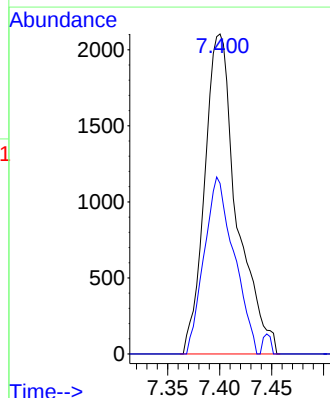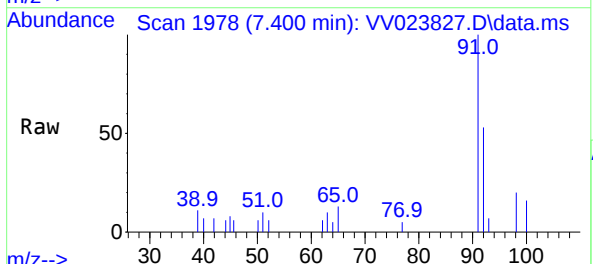

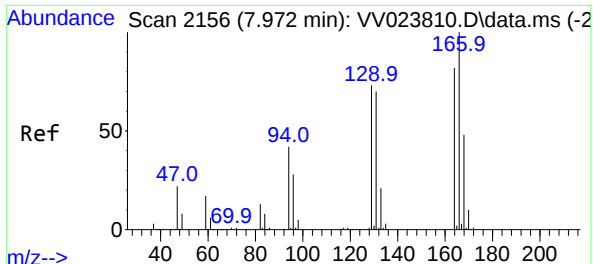

#47

Tetrachloroethene

Concen: 12.431 ug/L

RT: 7.976 min Scan# 2156

Delta R.T. 0.003 min

Lab File: VV023827.D

Acq: 07 Dec 2021 16:51

Instrument :

MSVOA_V

ClientSampleId :

C0G30

Tgt Ion:164 Resp: 117624


Ion Ratio Lower Upper

164 100




129 90.7 62.6 116.2

131 89.4 61.0 113.4

166 126.3 87.3 162.1

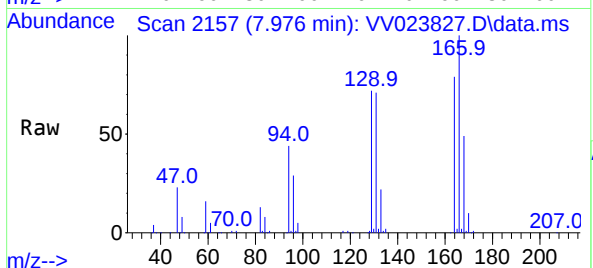

Abundance

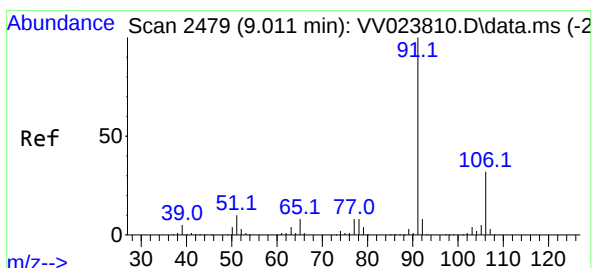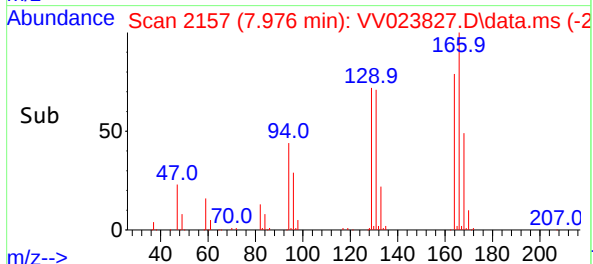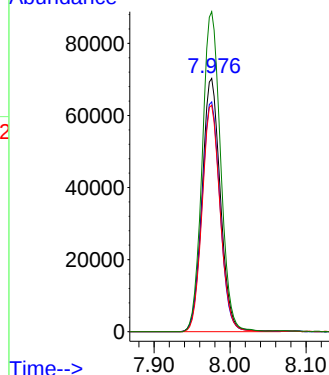

#52

Ethylbenzene

Concen: 0.138 ug/L

RT: 9.018 min Scan# 2481

Delta R.T. 0.007 min

Lab File: VV023827.D


Acq: 07 Dec 2021 16:51

Tgt Ion: 91 Resp: 6055



Ion Ratio Lower Upper


91 100

106 32.4 22.0 41.0

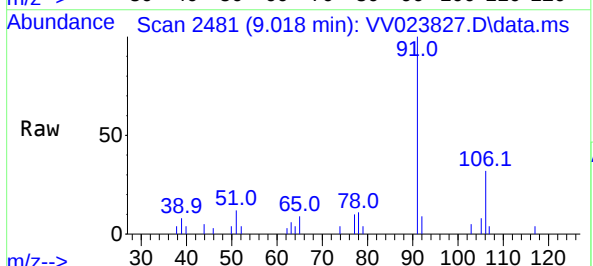

Abundance

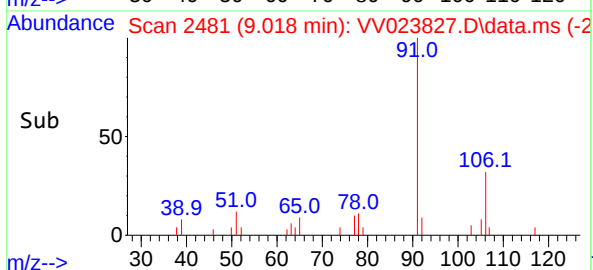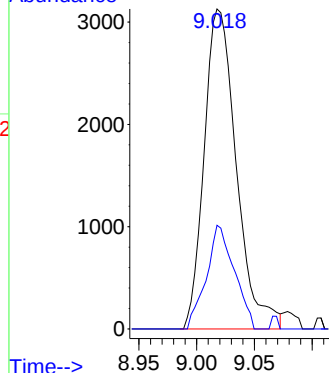

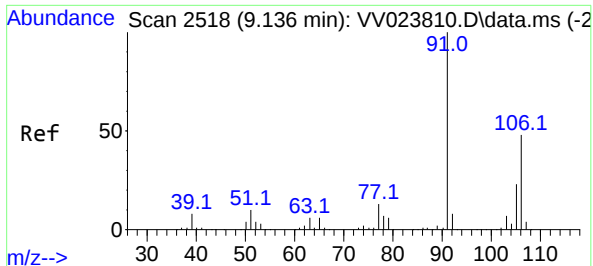

#53

m,p-xylene

Concen: 0.182 ug/L

RT: 9.143 min Scan# 2

Delta R.T. 0.007 min

Lab File: VV023827.D

Acq: 07 Dec 2021 16:51

Instrument :

MSVOA_V

ClientSampleId :





C0G30

Tgt Ion:106 Resp: 3188

Ion Ratio Lower Upper

106 100

91 182.2 139.5 259.1

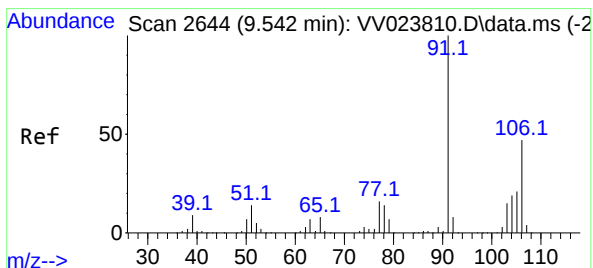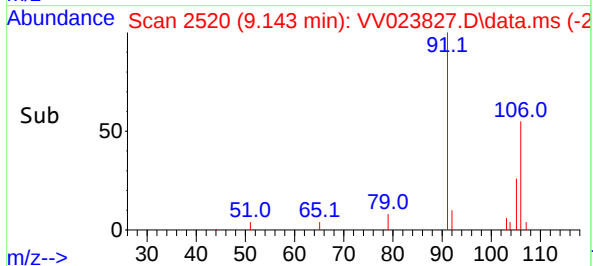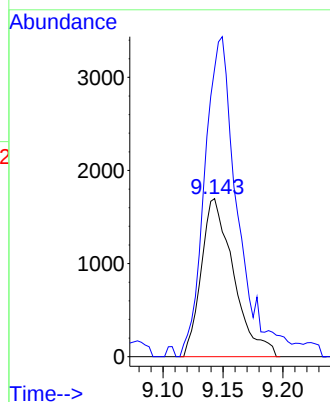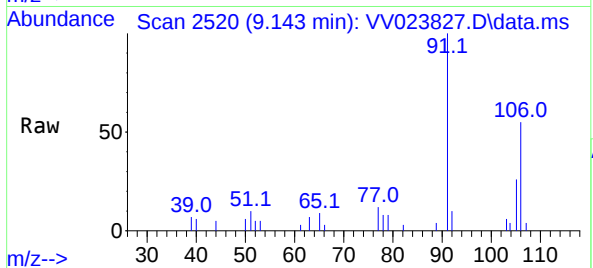

#54

o-xylene

Concen: 0.073 ug/L

RT: 9.548 min Scan# 2646

Delta R.T. 0.007 min

Lab File: VV023827.D




Acq: 07 Dec 2021 16:51


Tgt Ion:106 Resp: 1213

Ion Ratio Lower Upper

106 100

91 196.6 147.9 274.7


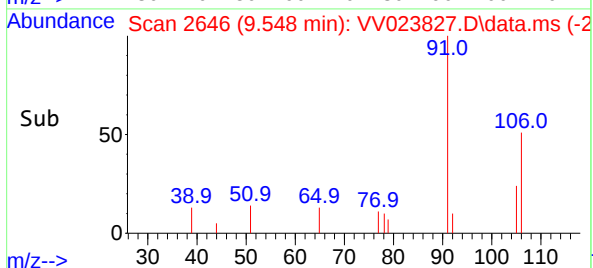
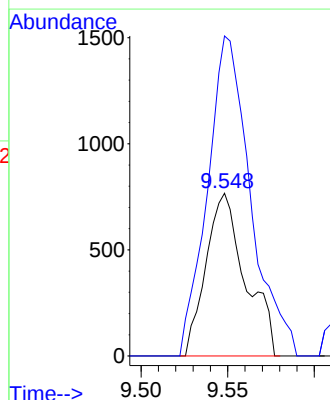
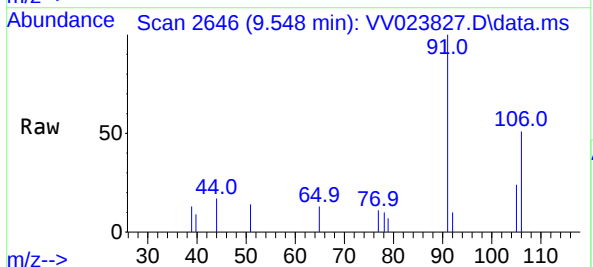


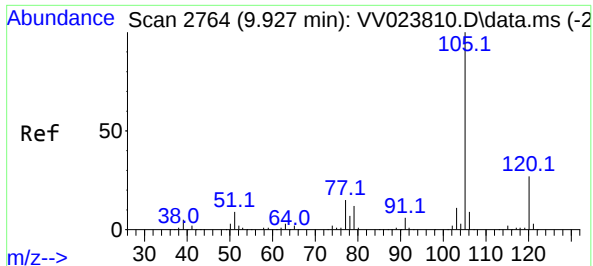

#60
Isopropylbenzene
Concen: 0.054 ug/L
RT: 9.940 min Scan# 21
Delta R.T. 0.010 min
Lab File: VV023827.D
Acq: 07 Dec 2021 16:51




Instrument :
MSVOA_V
ClientSampleId :
C0G30


Tgt Ion:105 Resp: 2315
Ion Ratio Lower Upper
105 100
120 29.6 21.4 32.0
77 12.2 12.2 18.4#

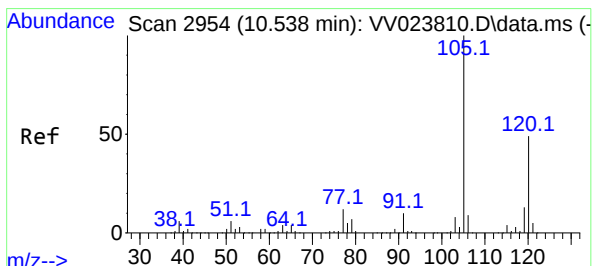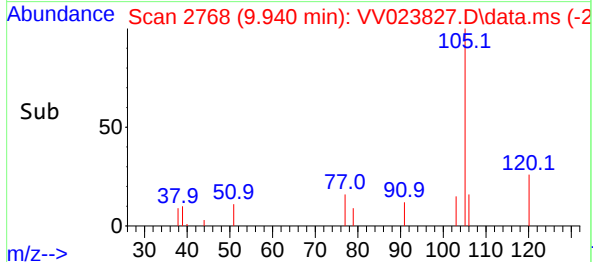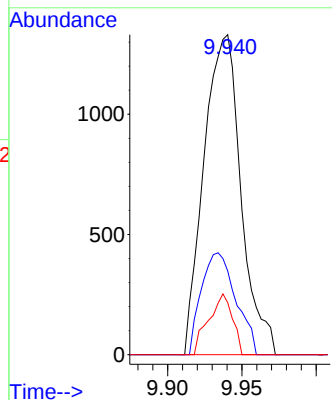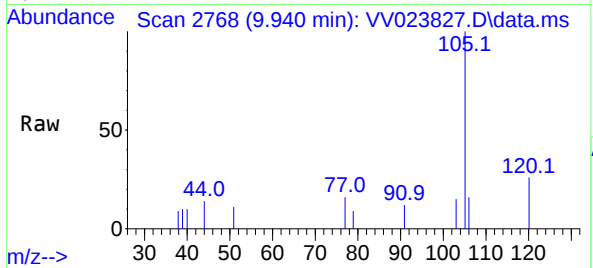

#62
1,3,5-Trimethylbenzene
Concen: 0.136 ug/L
RT: 10.538 min Scan# 2954
Delta R.T. 0.000 min
Lab File: VV023827.D
Acq: 07 Dec 2021 16:51


Tgt Ion:105 Resp: 4852
Ion Ratio Lower Upper
105 100
120 45.9 40.1 60.1

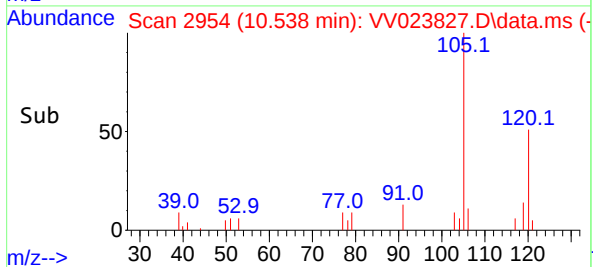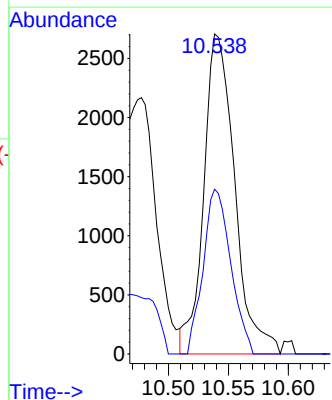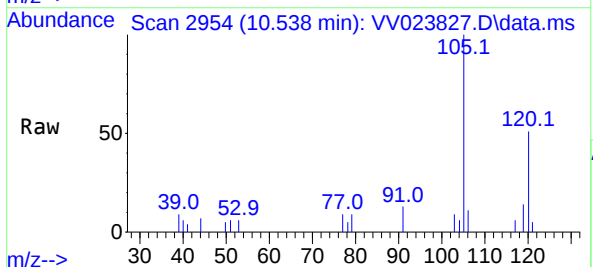

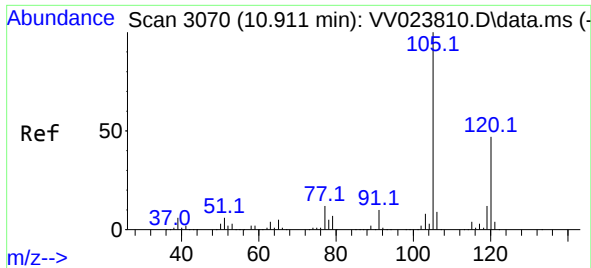

#63
 1,2,4-Trimethylbenzene
 Concen: 0.426 ug/L
 RT: 10.915 min Scan# 3071
 Delta R.T. 0.003 min
 Lab File: VV023827.D
 Acq: 07 Dec 2021 16:51

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G30

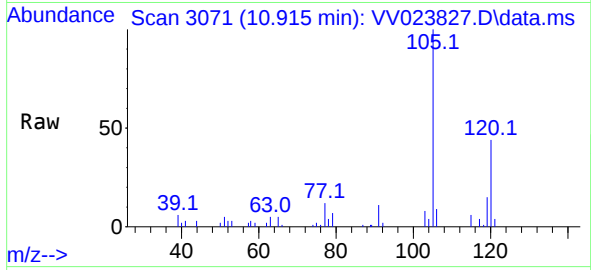

Tgt Ion:	105	Resp:	14986
Ion Ratio	Lower	Upper	
105	100		
120	47.8	36.7	55.1

