

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
 Data File : VV023811.D
 Acq On : 07 Dec 2021 10:25
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK271

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023811.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rVB	101389	101493	18.01%	2.242%
2	1.568	156	164	175	rBV	75650	85496	15.17%	1.889%
3	2.108	319	332	353	rBV	152903	229055	40.64%	5.061%
4	2.507	445	456	473	rVB2	7036	12203	2.17%	0.270%
5	3.899	879	889	920	rBV2	23493	97660	17.33%	2.158%
6	4.346	1011	1028	1053	rVB2	99182	246470	43.73%	5.446%
7	5.043	1228	1245	1275	rBV2	222564	563575	100.00%	12.452%
8	5.613	1407	1422	1452	rBV	170574	352831	62.61%	7.796%
9	5.908	1501	1514	1525	rBV	4323	9690	1.72%	0.214%
10	6.066	1550	1563	1587	rBV	119003	256402	45.50%	5.665%
11	6.982	1838	1848	1868	rBV2	62491	121345	21.53%	2.681%
12	7.313	1939	1951	1969	rBV	281530	488591	86.69%	10.795%
13	7.387	1971	1974	1984	rVB6	5069	8542	1.52%	0.189%
14	7.622	2038	2047	2061	rBV	37163	66796	11.85%	1.476%
15	8.088	2182	2192	2235	rBV	187289	438945	77.89%	9.698%
16	8.850	2417	2429	2459	rBV	261564	431692	76.60%	9.538%
17	10.217	2842	2854	2868	rBV	80762	133149	23.63%	2.942%
18	10.918	3063	3072	3086	rVB5	4180	6354	1.13%	0.140%
19	11.249	3164	3175	3195	rBV	264279	424511	75.32%	9.380%
20	11.622	3279	3291	3310	rBV	274231	428105	75.96%	9.459%
21	15.985	4631	4648	4655	rBV	8108	23024	4.09%	0.509%




Sum of corrected areas: 4525929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023811.D
Acq On : 07 Dec 2021 10:25
Operator : SY/MD
Sample : VV1207WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

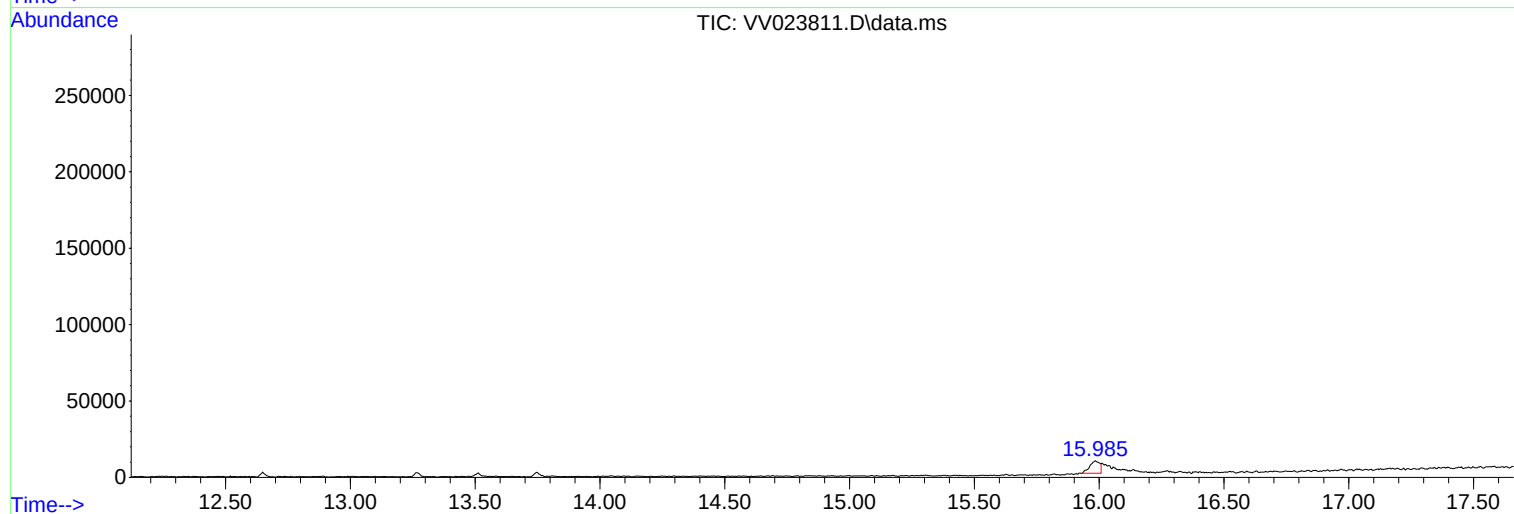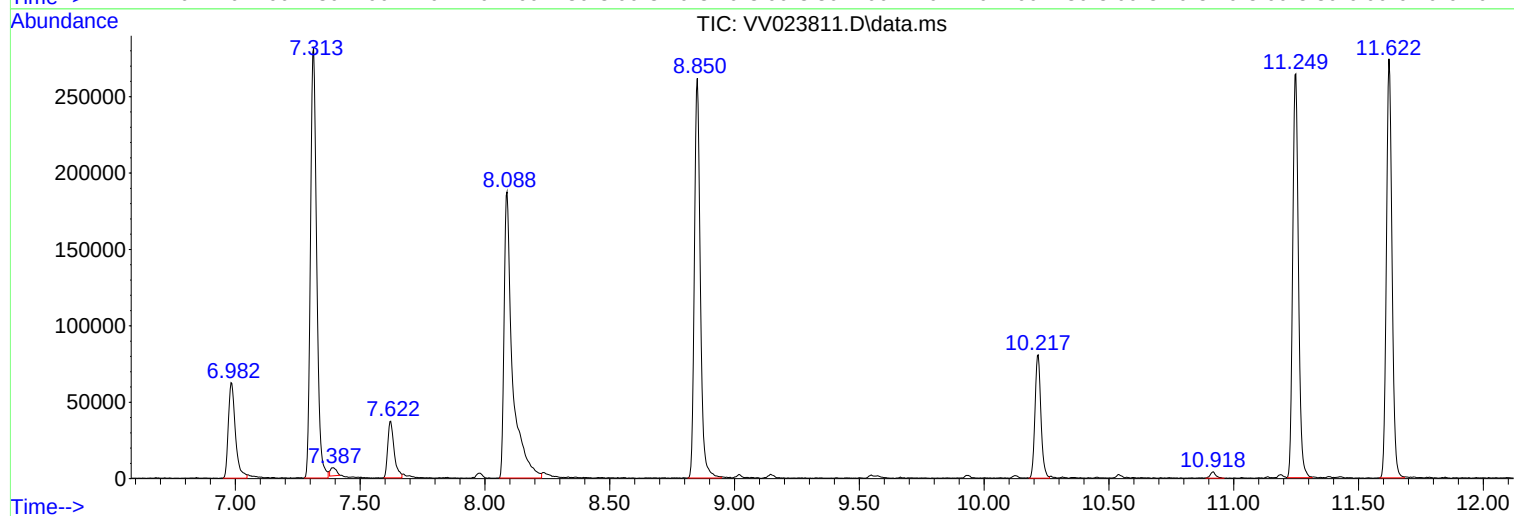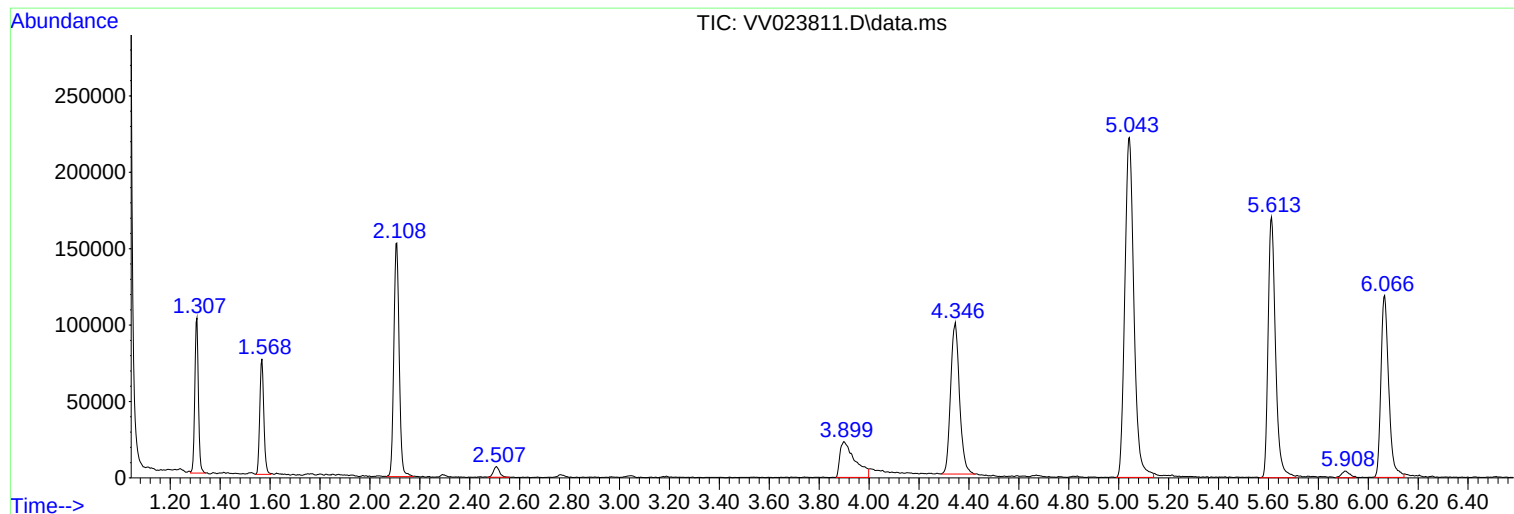

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023811.D
Acq On : 07 Dec 2021 10:25
Operator : SY/MD
Sample : VV1207WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023811.D
Acq On : 07 Dec 2021 10:25
Operator : SY/MD
Sample : VV1207WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK271

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc