

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
 Data File : VV023816.D
 Acq On : 07 Dec 2021 12:32
 Operator : SY/MD
 Sample : M4879-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023816.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	94	rVB	62873	65680	5.62%	1.302%
2	1.568	155	164	175	rBV	54719	61287	5.25%	1.215%
3	2.108	321	332	345	rBV	108746	159250	13.63%	3.156%
4	2.764	526	536	547	rBV3	10910	19380	1.66%	0.384%
5	3.912	879	893	933	rBV2	61223	217135	18.59%	4.304%
6	4.349	1013	1029	1059	rBV	83003	204739	17.53%	4.058%
7	5.050	1230	1247	1272	rBV3	175507	444688	38.07%	8.814%
8	5.619	1410	1424	1458	rBV	147998	306623	26.25%	6.078%
9	5.921	1505	1518	1537	rBV6	23188	48863	4.18%	0.969%
10	6.069	1549	1564	1588	rBV	99239	211067	18.07%	4.184%
11	6.989	1840	1850	1872	rBV3	49784	93174	7.98%	1.847%
12	7.317	1940	1952	1971	rBV	221387	384669	32.93%	7.624%
13	7.625	2039	2048	2072	rBV2	29176	54672	4.68%	1.084%
14	7.976	2134	2157	2177	rBV	699336	1167983	100.00%	23.150%
15	8.088	2182	2192	2218	rBV	207867	368453	31.55%	7.303%
16	8.853	2419	2430	2452	rBV	221888	369769	31.66%	7.329%
17	10.217	2842	2854	2866	rBV2	72023	114124	9.77%	2.262%
18	10.918	3063	3072	3084	rVB3	8547	13123	1.12%	0.260%
19	11.249	3163	3175	3193	rBV	231288	361548	30.95%	7.166%
20	11.535	3253	3264	3280	rBV4	14404	26811	2.30%	0.531%
21	11.625	3280	3292	3309	rVB	222380	352167	30.15%	6.980%




Sum of corrected areas: 5045205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023816.D
Acq On : 07 Dec 2021 12:32
Operator : SY/MD
Sample : M4879-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

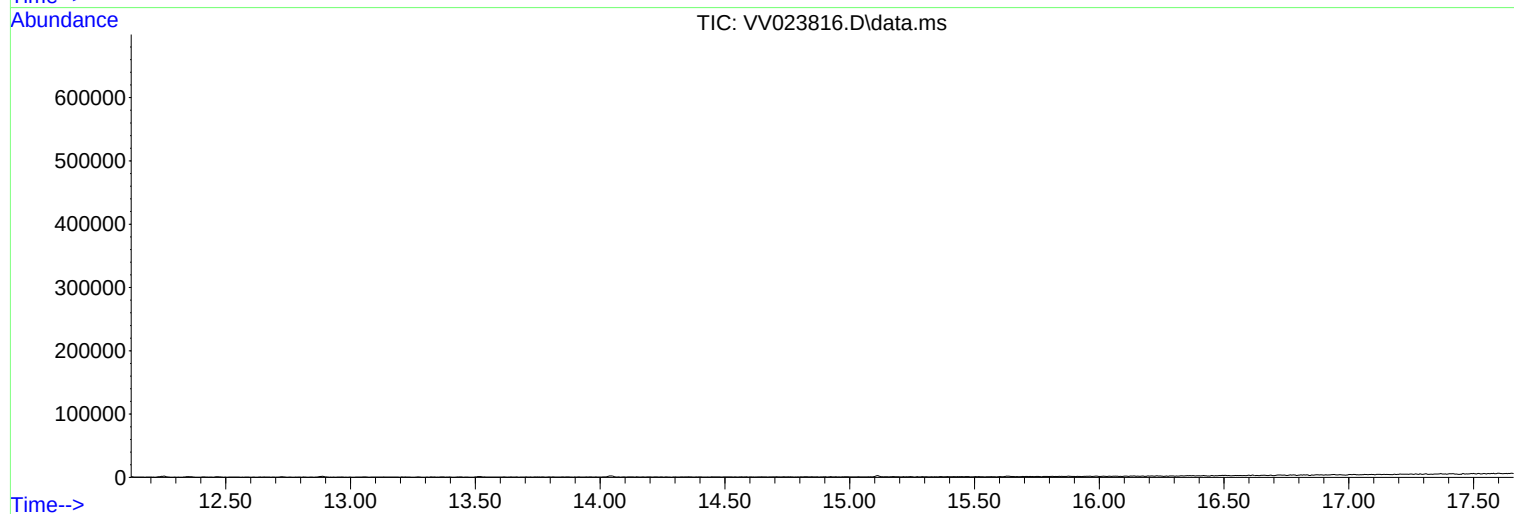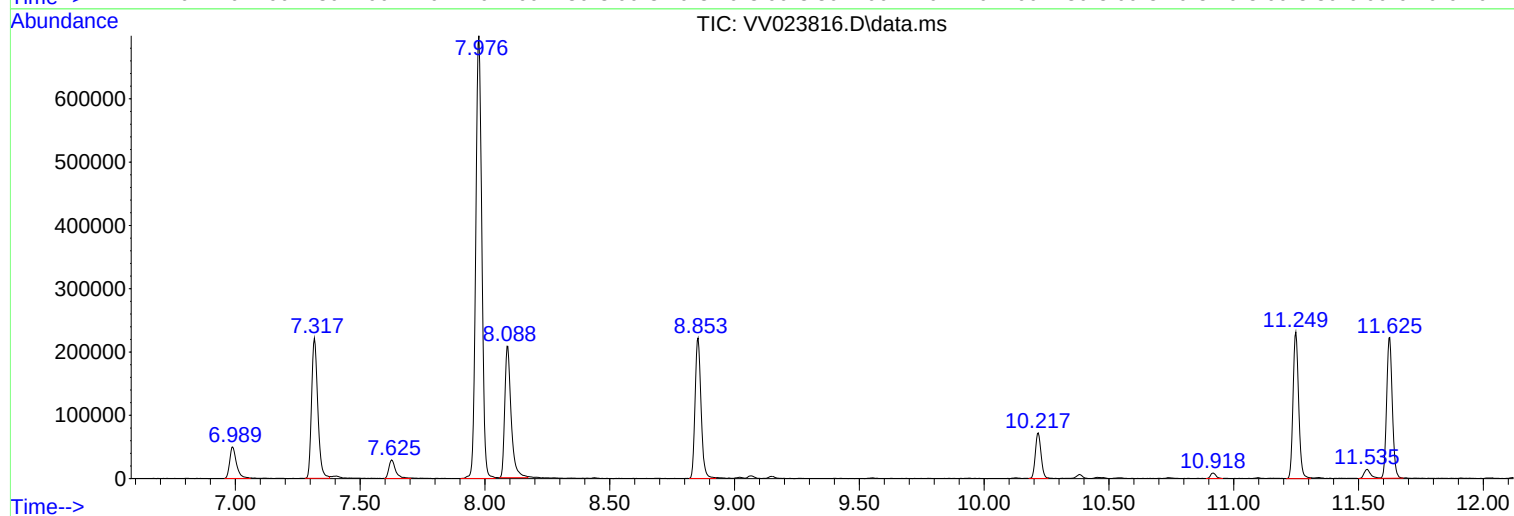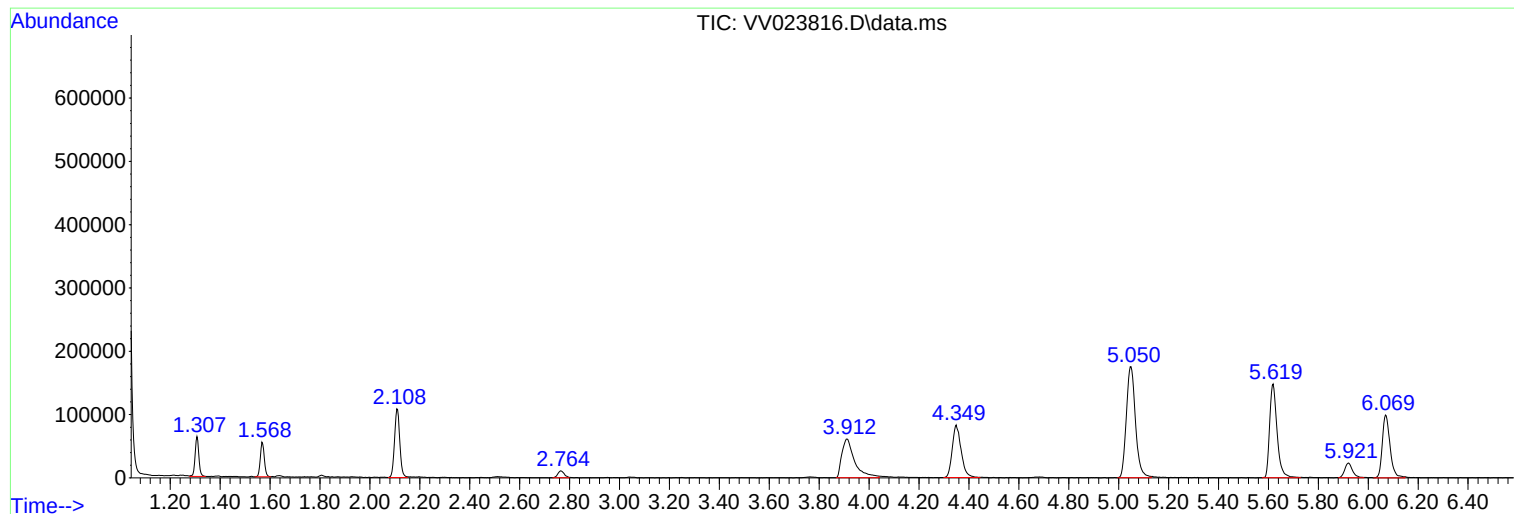

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023816.D
Acq On : 07 Dec 2021 12:32
Operator : SY/MD
Sample : M4879-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023816.D
Acq On : 07 Dec 2021 12:32
Operator : SY/MD
Sample : M4879-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc