

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
 Data File : VV023821.D
 Acq On : 07 Dec 2021 14:31
 Operator : SY/MD
 Sample : M4879-12DL 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0G69DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023821.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	95773	96434	13.08%	1.984%
2	1.568	156	164	175	rVB	72461	80554	10.92%	1.657%
3	2.108	321	332	350	rVB	151946	215545	29.23%	4.435%
4	2.510	446	457	468	rBV3	7169	12148	1.65%	0.250%
5	3.912	881	893	918	rBV2	25539	97116	13.17%	1.998%
6	4.349	1014	1029	1052	rVB	93381	231595	31.41%	4.765%
7	5.047	1227	1246	1270	rBV3	213257	527297	71.51%	10.849%
8	5.619	1412	1424	1444	rBV	141621	288671	39.15%	5.939%
9	5.924	1507	1519	1532	rBV8	5932	12761	1.73%	0.263%
10	6.069	1549	1564	1589	rBV	115887	243275	32.99%	5.005%
11	6.989	1839	1850	1870	rBV	59900	114640	15.55%	2.359%
12	7.317	1940	1952	1972	rBV	265396	465408	63.11%	9.576%
13	7.625	2038	2048	2065	rBV2	35930	66622	9.03%	1.371%
14	7.976	2144	2157	2176	rBV	442555	737410	100.00%	15.172%
15	8.091	2183	2193	2236	rBV	183614	425219	57.66%	8.749%
16	8.853	2418	2430	2452	rBV	219035	360606	48.90%	7.419%
17	10.217	2843	2854	2868	rBV	78147	128126	17.38%	2.636%
18	11.249	3163	3175	3191	rBV	223199	352304	47.78%	7.249%
19	11.625	3279	3292	3311	rBV	253084	404608	54.87%	8.325%




Sum of corrected areas: 4860339

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023821.D
Acq On : 07 Dec 2021 14:31
Operator : SY/MD
Sample : M4879-12DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

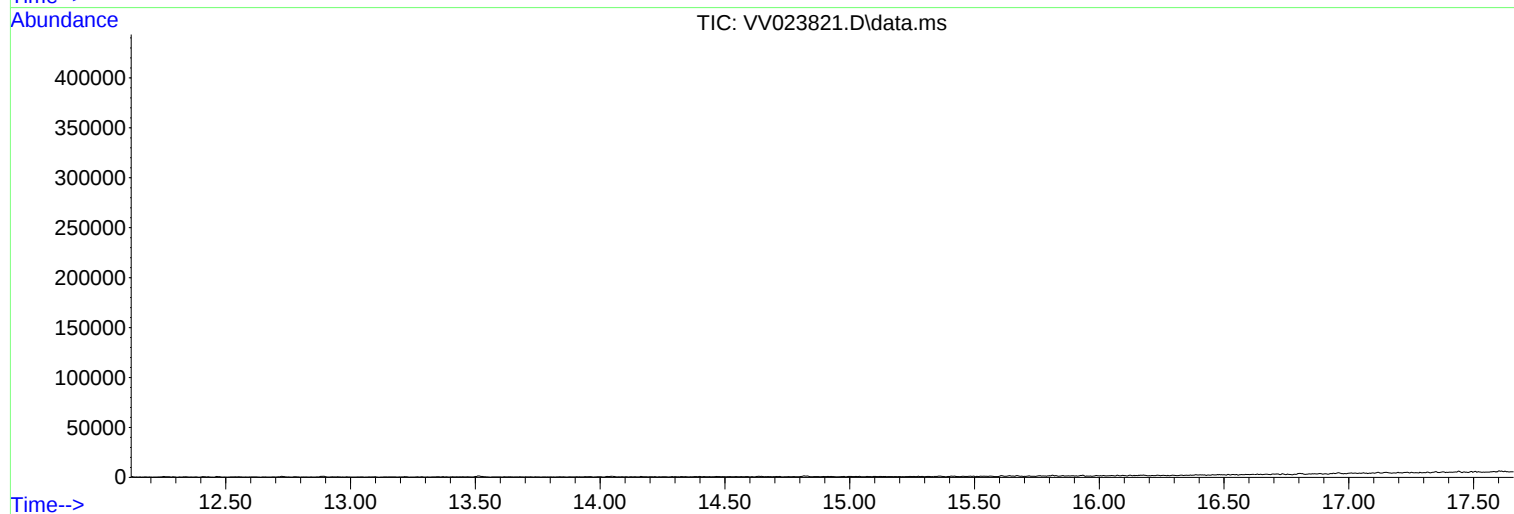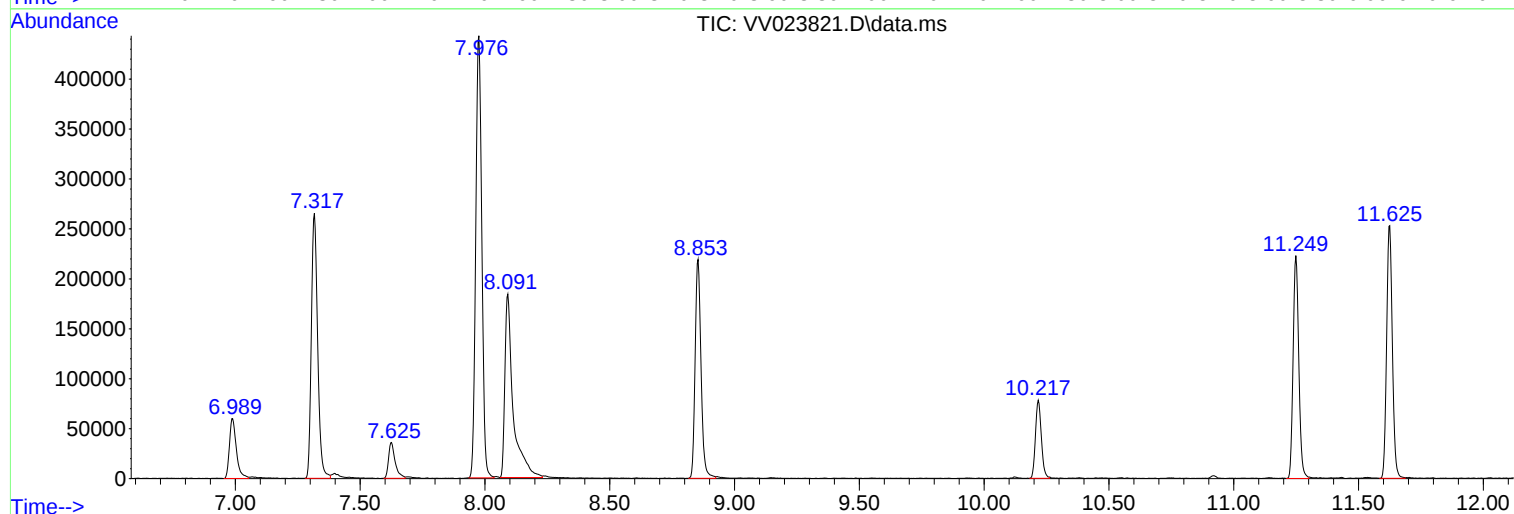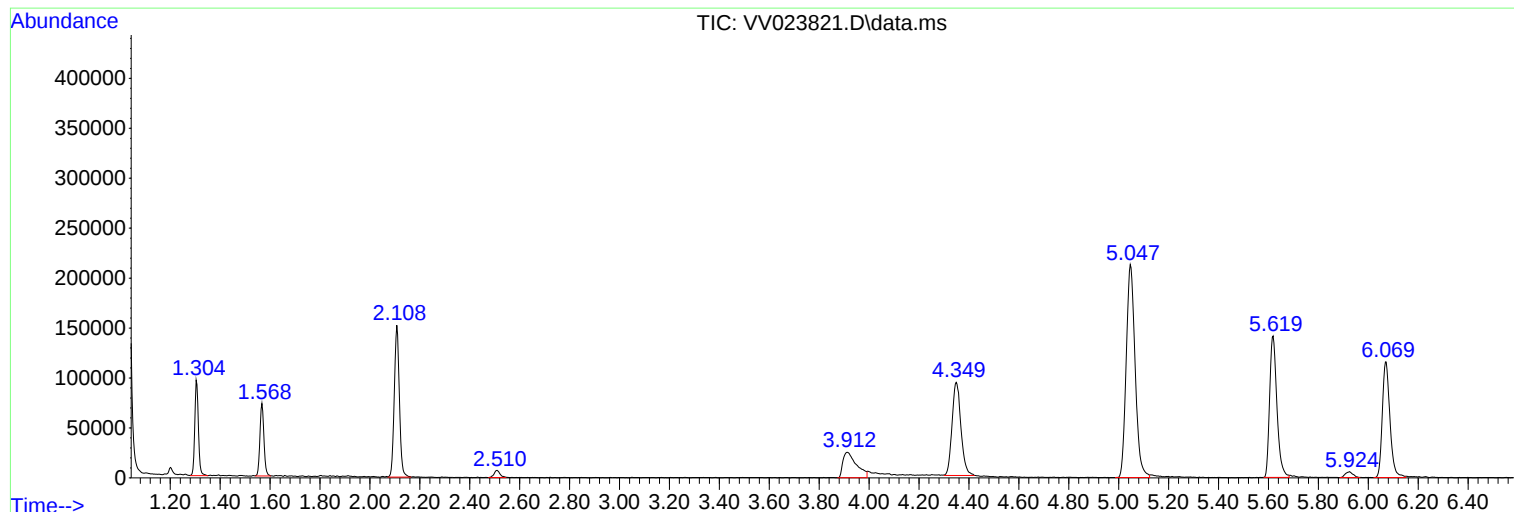

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023821.D
Acq On : 07 Dec 2021 14:31
Operator : SY/MD
Sample : M4879-12DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023821.D
Acq On : 07 Dec 2021 14:31
Operator : SY/MD
Sample : M4879-12DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0G69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc