

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
 Data File : VV023825.D
 Acq On : 07 Dec 2021 16:04
 Operator : SY/MD
 Sample : VIBLK244
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK244

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023825.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rVB	65732	66435	13.75%	1.560%
2	1.568	156	164	174	rBV	58477	66156	13.69%	1.554%
3	2.108	322	332	350	rVB	113758	169423	35.05%	3.979%
4	2.510	446	457	473	rVB2	23362	40610	8.40%	0.954%
5	3.912	878	893	916	rBV2	38508	154572	31.98%	3.630%
6	4.352	1012	1030	1052	rBV	88808	220787	45.68%	5.185%
7	5.050	1230	1247	1270	rBV2	193356	483310	100.00%	11.351%
8	5.619	1412	1424	1449	rBV	175281	355154	73.48%	8.341%
9	5.921	1508	1518	1527	rVB9	2694	5156	1.07%	0.121%
10	6.072	1551	1565	1583	rBV	110055	226285	46.82%	5.314%
11	6.989	1839	1850	1875	rBV	55826	106411	22.02%	2.499%
12	7.317	1940	1952	1970	rBV	239875	417907	86.47%	9.815%
13	7.397	1974	1977	1995	rVB9	4460	8641	1.79%	0.203%
14	7.625	2039	2048	2063	rBV	32318	57532	11.90%	1.351%
15	7.979	2150	2158	2170	rVB4	9773	17122	3.54%	0.402%
16	8.092	2181	2193	2225	rBV	234309	424077	87.74%	9.959%
17	8.423	2285	2296	2308	rBV4	2836	5533	1.14%	0.130%
18	8.854	2419	2430	2449	rBV	260647	423784	87.68%	9.953%
19	9.146	2514	2521	2534	rBV4	3969	6707	1.39%	0.158%
20	10.217	2842	2854	2868	rBV2	80874	128809	26.65%	3.025%
21	10.384	2897	2906	2914	rVB4	3015	4922	1.02%	0.116%
22	10.918	3064	3072	3084	rBV3	7518	11296	2.34%	0.265%
23	11.249	3164	3175	3196	rBV	281072	432877	89.57%	10.166%
24	11.625	3280	3292	3306	rBV	250605	393700	81.46%	9.246%
25	12.886	3673	3684	3693	rVB5	4938	7072	1.46%	0.166%
26	13.503	3868	3876	3889	rVB	9777	15218	3.15%	0.357%
27	14.635	4221	4228	4243	rVB4	5391	8520	1.76%	0.200%


Sum of corrected areas: 4258016

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023825.D
Acq On : 07 Dec 2021 16:04
Operator : SY/MD
Sample : VIBLK244
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

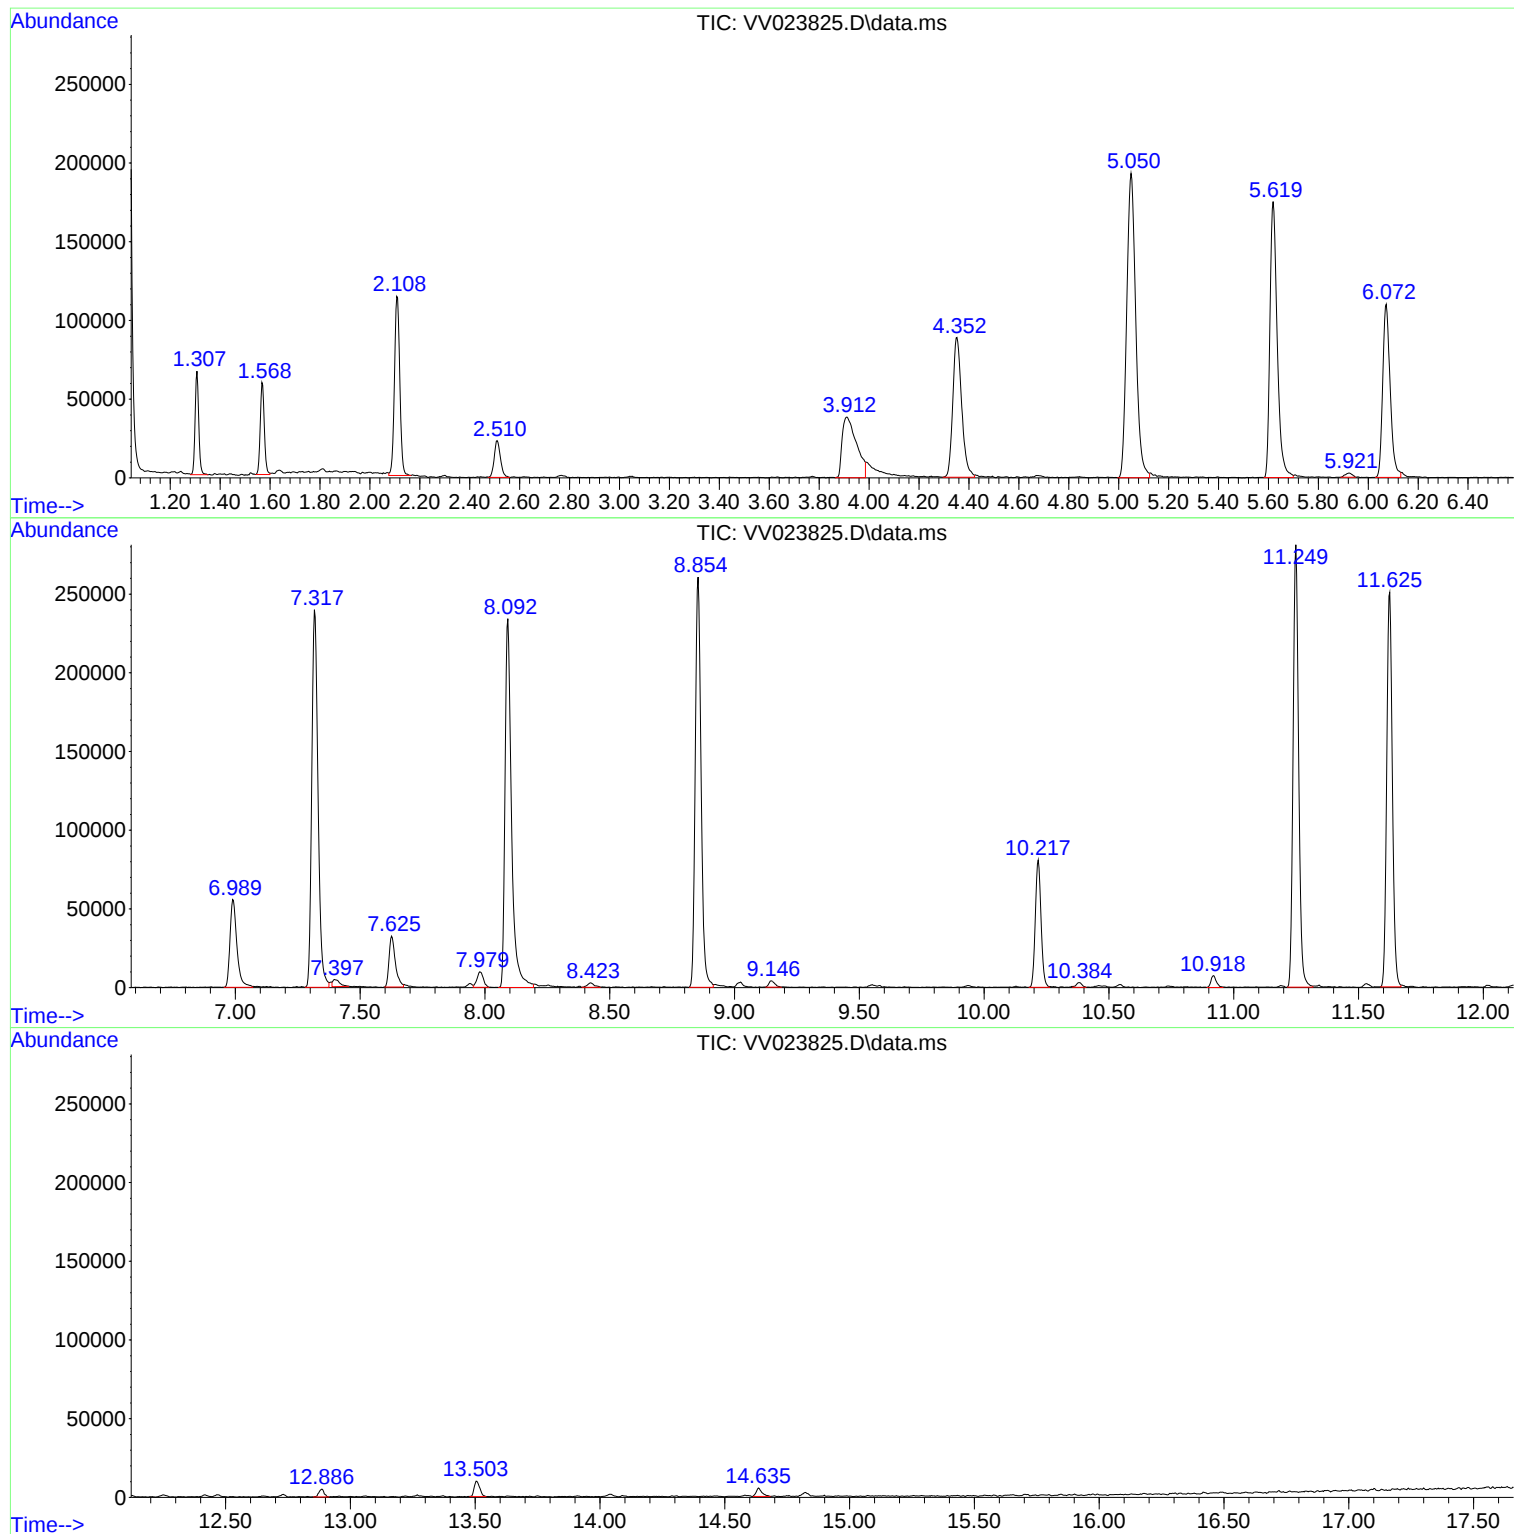

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023825.D
Acq On : 07 Dec 2021 16:04
Operator : SY/MD
Sample : VIBLK244
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023825.D
Acq On : 07 Dec 2021 16:04
Operator : SY/MD
Sample : VIBLK244
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------