


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120721\
Data File : VV023809.D
Acq On : 07 Dec 2021 09:05
Operator : SY/MD
Sample : BFB246
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB246

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 02 02:08:23 2021

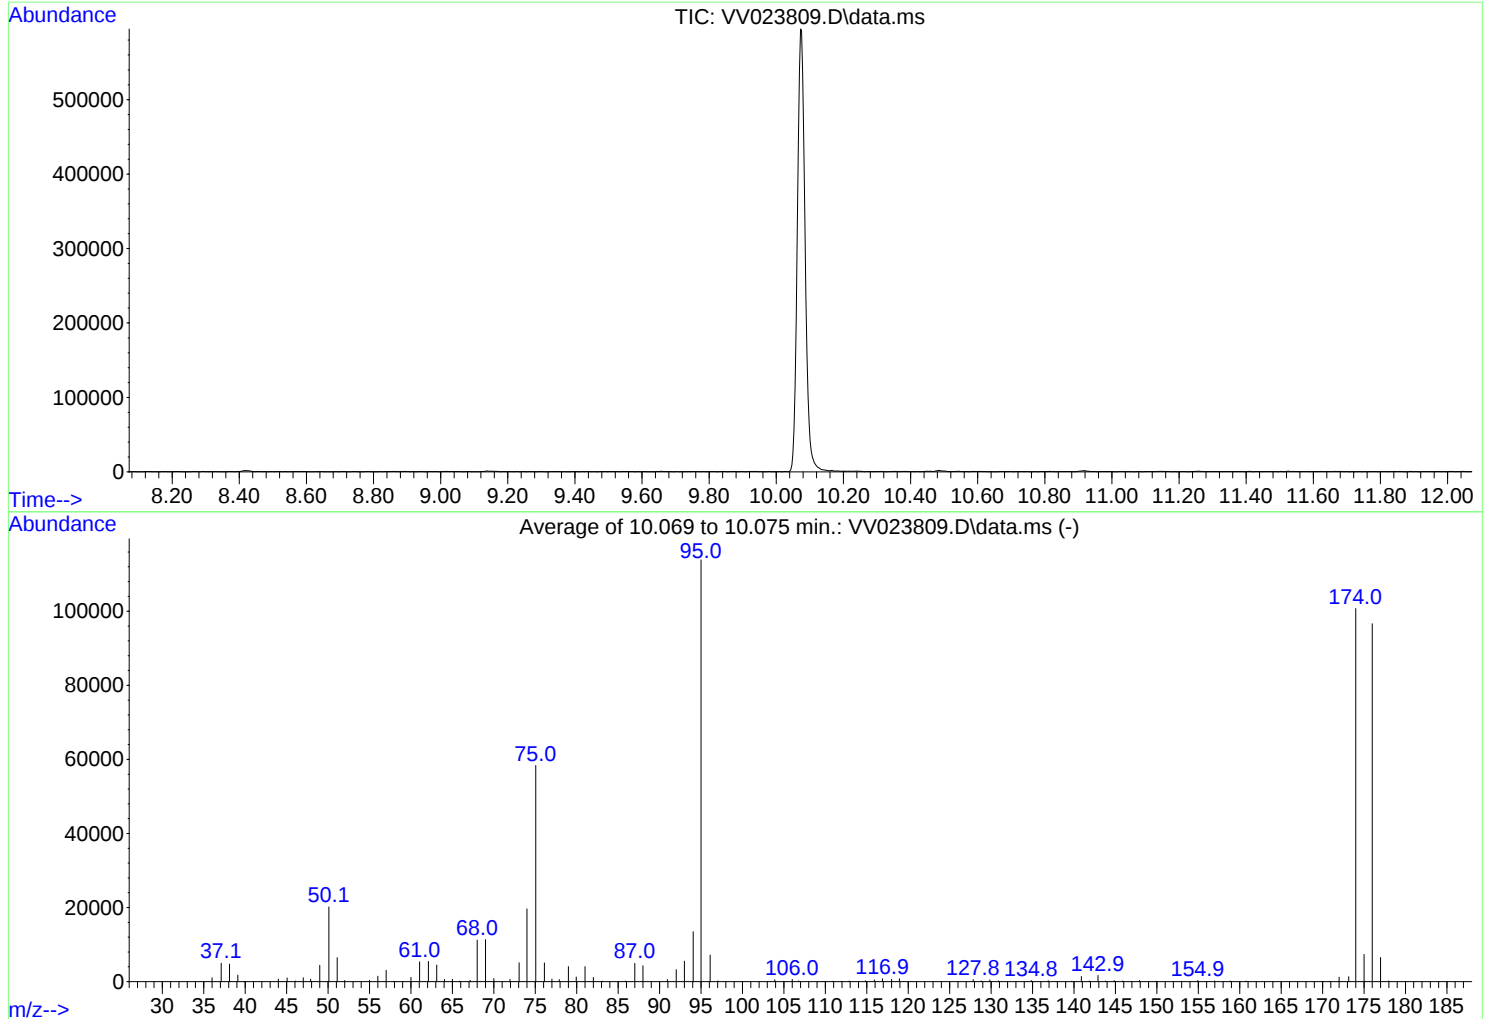

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	20195	PASS
75	95	30	80	51.3	58363	PASS
95	95	100	100	100.0	113877	PASS
96	95	5	9	6.3	7164	PASS
173	174	0.00	2	1.3	1344	PASS
174	95	50	120	88.5	100749	PASS
175	174	5	9	7.3	7334	PASS
176	174	95	105	95.9	96653	PASS
177	176	5	10	6.7	6522	PASS

m/z	Abundance
39.80	183.0
44.00	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	1088.0
37.10	5123.0
38.10	4905.0
39.10	1762.0
39.90	232.0
44.10	945.0
45.00	1009.0
46.10	182.0
47.00	1048.0
47.90	652.0
49.00	4558.0
50.10	20880.0
51.10	6756.0
52.00	345.0
55.00	370.0
56.00	1457.0
57.00	3153.0
57.90	110.0
60.00	1229.0
61.10	5542.0
62.10	5661.0
63.10	4573.0
64.00	665.0
65.00	635.0
65.90	133.0
67.20	369.0
68.00	11687.0
69.00	11724.0
70.00	841.0
72.00	625.0
73.10	5361.0
74.00	20272.0
75.00	60400.0
76.10	5306.0
77.00	679.0
77.90	590.0
79.00	4175.0
79.90	1309.0
81.00	4236.0
82.00	1206.0
83.10	156.0
85.90	177.0
87.00	5145.0
88.00	4393.0
90.90	574.0
92.00	3368.0
93.00	5748.0
94.00	13857.0
95.00	117768.0
96.10	7350.0
97.10	214.0
103.90	563.0
104.90	124.0
106.00	635.0
106.80	229.0
109.70	103.0
110.90	125.0
111.90	110.0
112.80	174.0
114.80	280.0
115.90	495.0
116.90	819.0
118.00	677.0
118.90	774.0
127.80	614.0
128.80	242.0
129.90	527.0
130.90	221.0
134.90	313.0
136.90	272.0
139.80	149.0
140.90	1413.0
141.80	178.0
142.90	1769.0
143.80	175.0
144.90	304.0
145.90	213.0
146.90	120.0
147.90	316.0
149.90	121.0
153.00	132.0
155.00	296.0
157.00	205.0
158.80	179.0
160.70	195.0
170.90	124.0
172.00	1257.0
173.10	1388.0
174.00	103968.0
175.00	7517.0
176.00	100048.0
177.00	6767.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

178.00

249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	967.0
37.10	5108.0
38.10	4805.0
39.10	1767.0
39.90	219.0
44.10	875.0
45.00	983.0
46.00	179.0
47.00	1044.0
47.90	608.0
49.00	4779.0
50.10	20568.0
51.10	6480.0
52.00	327.0
55.00	339.0
56.00	1348.0
57.00	3177.0
57.90	113.0
58.30	110.0
60.00	1117.0
61.00	5616.0
62.10	5520.0
63.10	4581.0
64.10	537.0
65.00	611.0
65.80	123.0
67.10	340.0
68.00	11493.0
69.00	11248.0
70.00	806.0
72.00	647.0
73.00	5270.0
74.00	19960.0
75.10	59832.0
76.10	4998.0
77.00	692.0
77.90	594.0
79.00	4009.0
80.00	1296.0
81.00	4056.0
82.00	1131.0
83.10	170.0
85.90	167.0
87.00	4682.0
88.00	4413.0
91.00	508.0
92.00	3440.0
93.00	5623.0
94.10	14032.0
95.00	116936.0
96.10	7008.0
97.10	247.0
103.90	541.0
105.00	136.0
106.00	640.0
106.80	199.0
110.90	129.0
111.90	121.0
112.90	179.0
114.90	272.0
115.90	487.0
116.90	810.0
118.00	643.0
118.90	846.0
127.90	599.0
128.80	286.0
129.90	505.0
130.90	212.0
134.80	339.0
136.90	306.0
139.80	140.0
140.90	1476.0
141.80	174.0
142.90	1734.0
143.80	130.0
144.80	252.0
145.80	210.0
148.00	332.0
149.90	114.0
153.00	124.0
154.90	283.0
156.90	197.0
158.80	179.0
160.70	200.0
170.80	138.0
172.00	1257.0
173.10	1327.0
174.00	106216.0
175.00	7596.0
176.00	101232.0
177.00	6890.0
178.00	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	1042.0
37.10	4640.0
38.10	4535.0
39.10	1737.0
39.90	166.0
44.00	899.0
45.10	952.0
46.10	164.0
47.00	1053.0
47.90	640.0
49.00	3864.0
50.10	19136.0
51.10	6226.0
52.00	305.0
55.00	324.0
56.00	1598.0
57.00	2831.0
57.90	110.0
60.00	1170.0
61.10	4970.0
62.10	5219.0
63.10	4341.0
64.00	662.0
65.00	648.0
65.90	117.0
67.20	353.0
68.00	10490.0
69.00	11158.0
70.00	873.0
71.90	611.0
73.10	4734.0
74.00	18704.0
75.00	54856.0
76.10	4900.0
77.00	649.0
77.90	475.0
79.00	3999.0
79.90	1179.0
81.00	3879.0
82.00	1100.0
83.10	114.0
85.90	159.0
87.00	5008.0
88.00	4024.0
90.90	568.0
92.00	2907.0
93.00	5164.0
94.00	12583.0
95.00	106928.0
96.10	7133.0
97.00	180.0
103.90	515.0
104.90	114.0
106.00	522.0
106.80	191.0
110.90	109.0
112.80	147.0
114.80	252.0
115.90	469.0
116.90	752.0
118.00	573.0
119.00	684.0
127.80	525.0
128.80	179.0
129.80	456.0
130.90	174.0
134.90	261.0
136.90	221.0
139.70	123.0
140.90	1220.0
141.90	165.0
142.90	1546.0
143.80	179.0
144.80	353.0
146.00	220.0
146.90	139.0
147.80	288.0
149.90	111.0
153.00	120.0
155.00	279.0
157.00	199.0
158.90	133.0
160.80	142.0
172.00	1092.0
173.20	1316.0
174.00	92064.0
175.00	6890.0
176.00	88680.0
177.00	5909.0
178.00	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246