

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029420.D
 Acq On : 07 Dec 2022 16:23
 Operator : SY/MD
 Sample : VV1207MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK294

Quant Time: Dec 08 00:57:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 00:46:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	509087	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	467414	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	238234	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	139524	44.756	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.520%		
7) Chloroethane-d5	1.552	69	112626	47.379	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.760%		
11) 1,1-Dichloroethene-d2	2.098	63	168835	34.723	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.440%		
21) 2-Butanone-d5	3.867	46	201850	106.141	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	106.140%		
24) Chloroform-d	4.336	84	270708	46.145	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.300%		
26) 1,2-Dichloroethane-d4	5.021	65	160872	48.014	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.020%		
32) Benzene-d6	5.040	84	593589	48.061	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.120%		
36) 1,2-Dichloropropane-d6	6.059	67	182955	48.496	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.000%		
41) Toluene-d8	7.307	98	542643	46.631	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.260%		
43) trans-1,3-Dichloroprop...	7.612	79	87911	46.148	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.300%		
47) 2-Hexanone-d5	8.082	63	174714	108.453	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	108.450%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	267270	49.577	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.160%		
66) 1,2-Dichlorobenzene-d4	11.612	152	221469	48.835	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.660%		
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	3224	0.953	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029420.D
Acq On : 07 Dec 2022 16:23
Operator : SY/MD
Sample : VV1207MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK294


Quant Time: Dec 08 00:57:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 08 00:46:44 2022
Response via : Initial Calibration

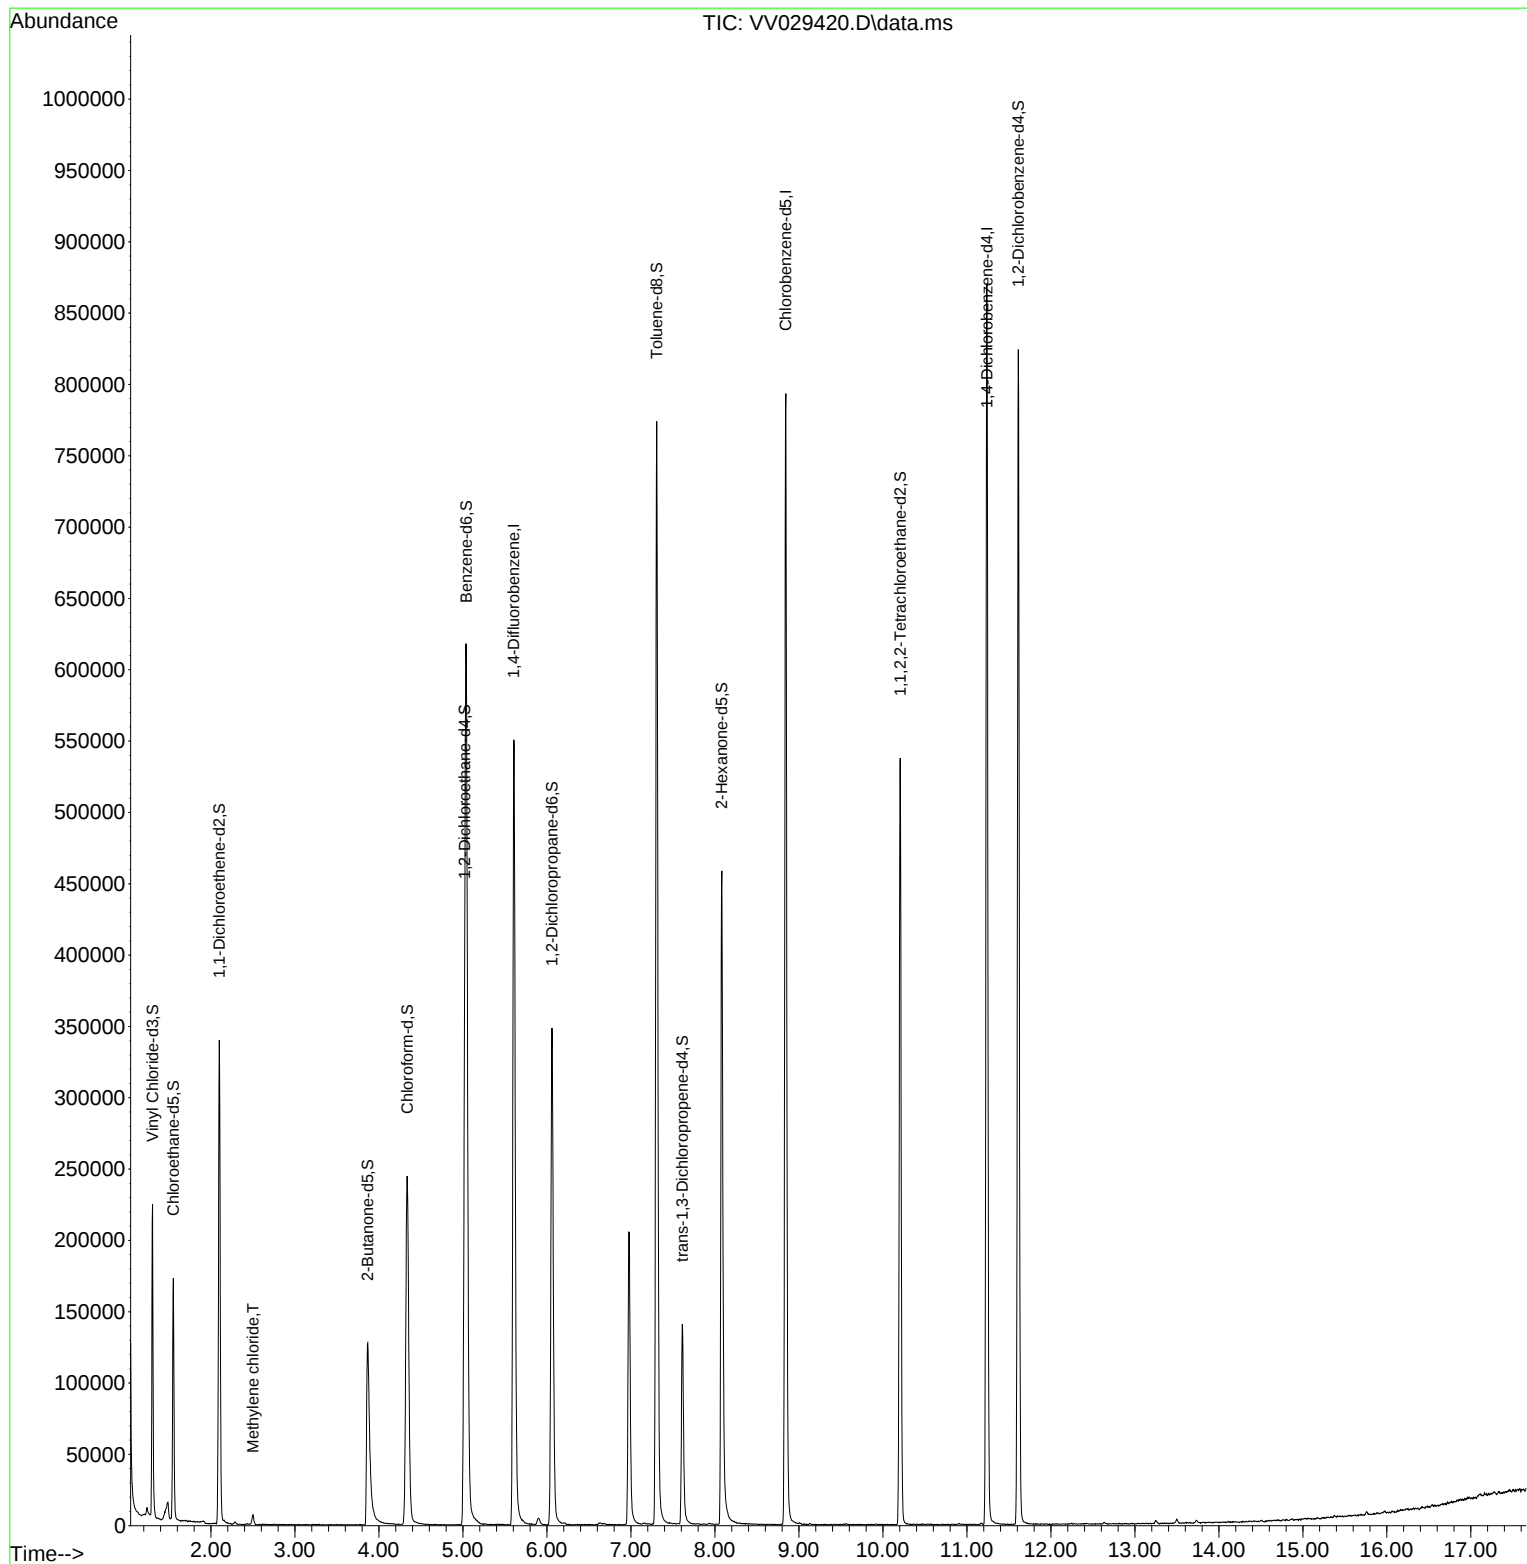

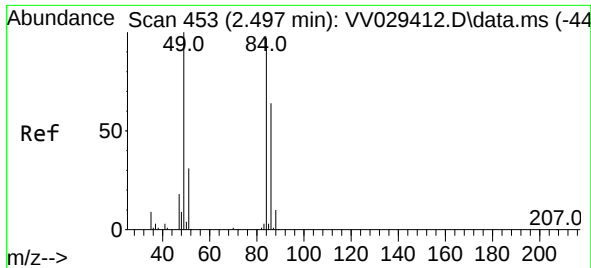

#16
Methylene chloride
Concen: 0.953 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV029420.D
Acq: 07 Dec 2022 16:23

Instrument :
MSVOA_V
ClientSampleId :
VBLK294

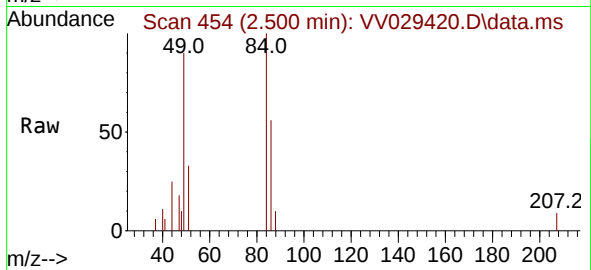

Tgt Ion:	84	Resp:	3224
Ion	Ratio	Lower	Upper
84	100		
86	56.2	46.0	85.4
49	89.9	72.2	134.0

