

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029421.D
 Acq On : 07 Dec 2022 16:47
 Operator : SY/MD
 Sample : VV1207MBL03
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK295

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 12/08/2022
 Supervised By :Mahesh Dadoda 12/08/2022

Quant Time: Dec 08 00:57:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 08 00:46:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	482653	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	437175	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	219572	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	131416	44.464	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	88.920%	
7) Chloroethane-d5	1.561	69	103367	45.865	ug/L	0.01
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.740%	
11) 1,1-Dichloroethene-d2	2.101	63	156540m	33.957	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	67.920%	
21) 2-Butanone-d5	3.867	46	204615	113.488	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	113.490%	
24) Chloroform-d	4.339	84	256610	46.138	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.280%	
26) 1,2-Dichloroethane-d4	5.024	65	157632	49.624	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.240%	
32) Benzene-d6	5.043	84	550839	47.685	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.360%	
36) 1,2-Dichloropropane-d6	6.063	67	174944	49.580	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.160%	
41) Toluene-d8	7.307	98	510638	46.915	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.840%	
43) trans-1,3-Dichloroprop...	7.612	79	83757	47.008	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.020%	
47) 2-Hexanone-d5	8.082	63	170695	113.287	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	113.290%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	249751	49.532	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.060%	
66) 1,2-Dichlorobenzene-d4	11.612	152	204265	48.870	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.740%	
Target Compounds						
16) Methylene chloride	2.500	84	2924	0.912	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029421.D
Acq On : 07 Dec 2022 16:47
Operator : SY/MD
Sample : VV1207MBL03
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
VBLK295

Quant Time: Dec 08 00:57:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 08 00:46:44 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Krupa Patel 12/08/2022
Supervised By :Mahesh Dadoda 12/08/2022

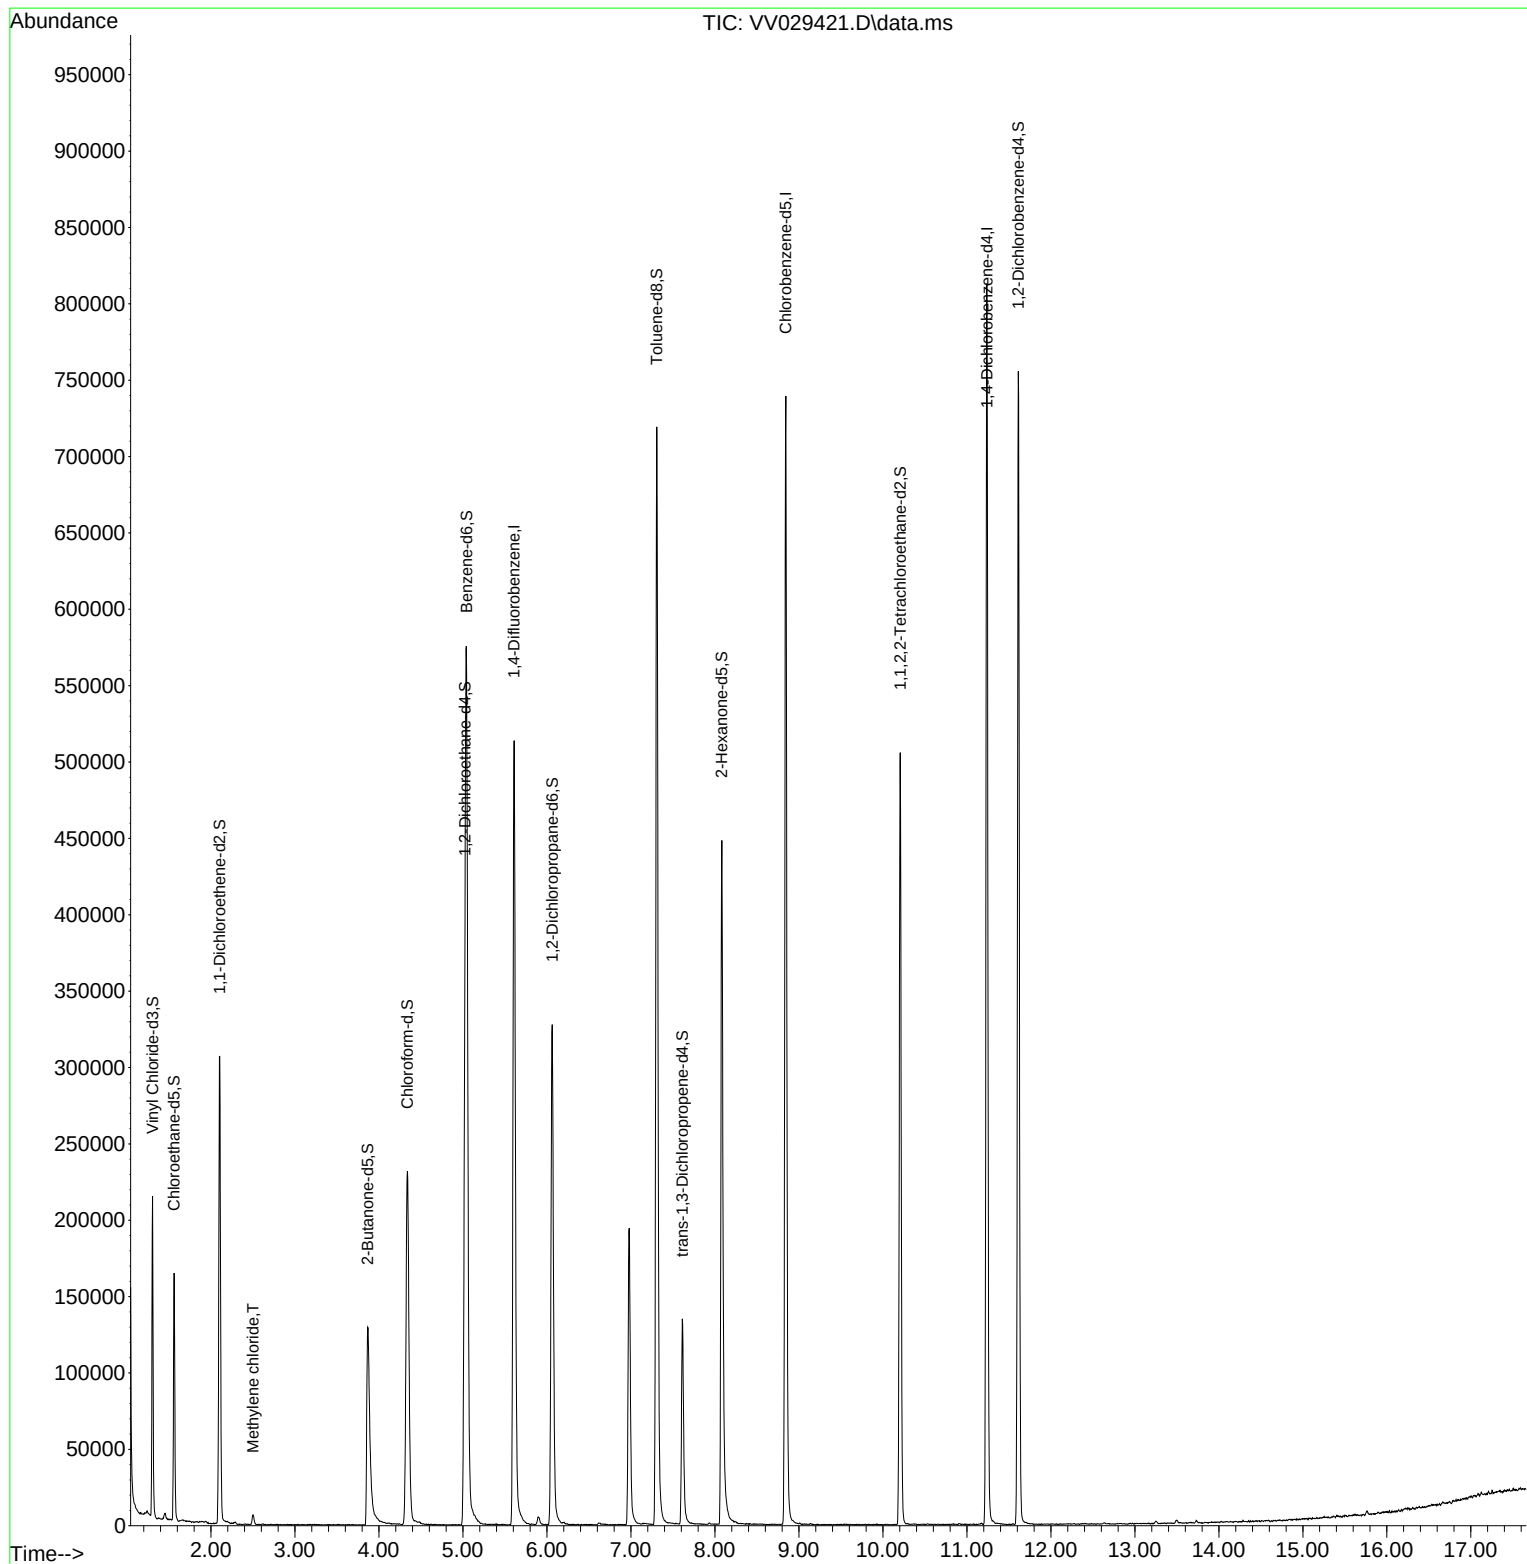

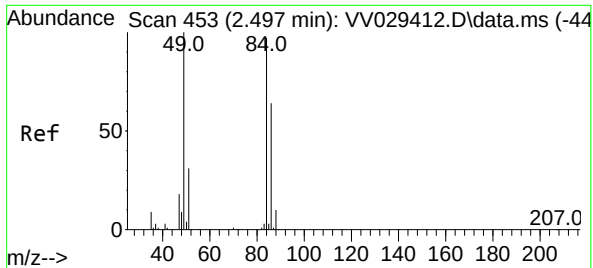

#16
Methylene chloride
Concen: 0.912 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV029421.D
Acq: 07 Dec 2022 16:47

Instrument :
MSVOA_V
ClientSampleId :
VBLK295

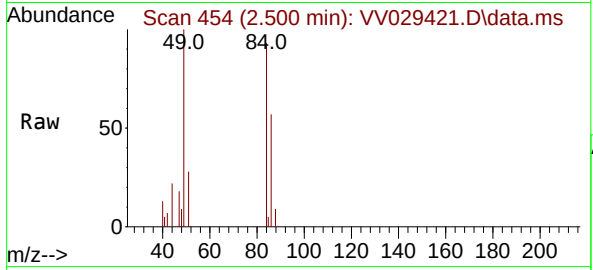

Tgt Ion:	84	Resp:	2924
Ion	Ratio	Lower	Upper
84	100		
86	60.8	46.0	85.4
49	107.5	72.2	134.0

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 12/08/2022
Supervised By :Mahesh Dadoda 12/08/2022

