

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029416.D
 Acq On : 07 Dec 2022 14:45
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK290

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	235682	236448	14.65%	1.825%
2	1.487	122	139	151	rVV6	12092	30578	1.90%	0.236%
3	1.552	151	159	174	rVB	169895	197991	12.27%	1.529%
4	2.027	302	307	311	rVB4	918	930	0.06%	0.007%
5	2.050	311	314	317	rBV4	670	537	0.03%	0.004%
6	2.098	317	329	347	rBV	340594	493298	30.57%	3.808%
7	2.285	379	387	398	rVB	4912	7463	0.46%	0.058%
8	2.426	423	431	439	rBV3	1071	1895	0.12%	0.015%
9	2.500	445	454	465	rVB	7563	12132	0.75%	0.094%
10	2.699	512	516	520	rBV2	291	323	0.02%	0.002%
11	2.757	525	534	546	rVV9	3089	6059	0.38%	0.047%
12	2.921	580	585	587	rVV	374	295	0.02%	0.002%
13	3.014	610	614	620	rVB2	220	255	0.02%	0.002%
14	3.047	620	624	627	rBV3	387	348	0.02%	0.003%
15	3.185	659	667	671	rBV2	622	930	0.06%	0.007%
16	3.265	685	692	697	rVV4	358	417	0.03%	0.003%
17	3.474	754	757	763	rBV2	311	339	0.02%	0.003%
18	3.542	773	778	784	rVB2	418	341	0.02%	0.003%
19	3.584	784	791	796	rBV2	315	427	0.03%	0.003%
20	3.867	869	879	913	rBV	123615	330494	20.48%	2.551%
21	4.246	990	997	1001	rBV5	587	777	0.05%	0.006%
22	4.336	1007	1025	1050	rBV	246450	613091	38.00%	4.733%
23	4.574	1095	1099	1101	rBV3	542	392	0.02%	0.003%
24	4.596	1101	1106	1109	rBV3	634	593	0.04%	0.005%
25	4.658	1118	1125	1130	rBV4	1394	1853	0.11%	0.014%
26	4.735	1144	1149	1151	rBV	331	279	0.02%	0.002%
27	4.815	1170	1174	1178	rBV3	1102	918	0.06%	0.007%
28	4.908	1196	1203	1207	rBV2	381	378	0.02%	0.003%
29	5.037	1225	1243	1288	rBV2	611963	1613479	100.00%	12.456%
30	5.294	1321	1323	1329	rVB	410	335	0.02%	0.003%
31	5.400	1354	1356	1360	rVB4	492	281	0.02%	0.002%
32	5.458	1370	1374	1377	rBV	249	287	0.02%	0.002%
33	5.474	1377	1379	1386	rVB3	476	480	0.03%	0.004%
34	5.510	1386	1390	1395	rVB3	455	408	0.03%	0.003%
35	5.606	1407	1420	1452	rBV	524268	1053517	65.29%	8.133%
36	5.793	1475	1478	1486	rVB4	644	599	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029416.D
 Acq On : 07 Dec 2022 14:45
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK290

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.902	1500	1512	1513	rBV6	5557	7700	0.48%	0.059%
38	6.059	1547	1561	1592	rBV	346053	713133	44.20%	5.505%
39	6.284	1629	1631	1635	rVB3	430	340	0.02%	0.003%
40	6.503	1693	1699	1708	rVB3	656	1172	0.07%	0.009%
41	6.622	1727	1736	1743	rBV5	1326	2635	0.16%	0.020%
42	6.661	1743	1748	1750	rBV4	537	422	0.03%	0.003%
43	6.764	1775	1780	1783	rBV3	364	380	0.02%	0.003%
44	6.818	1793	1797	1802	rVB4	365	390	0.02%	0.003%
45	6.911	1823	1826	1831	rVB3	489	462	0.03%	0.004%
46	6.976	1831	1846	1877	rBV	206480	386427	23.95%	2.983%
47	7.201	1911	1916	1918	rBV5	446	382	0.02%	0.003%
48	7.230	1920	1925	1934	rVB6	2019	2752	0.17%	0.021%
49	7.307	1935	1949	1985	rBV	782377	1376764	85.33%	10.629%
50	7.548	2022	2024	2027	rVB3	535	313	0.02%	0.002%
51	7.612	2030	2044	2072	rBV	144754	252877	15.67%	1.952%
52	7.831	2108	2112	2118	rBV6	1550	1868	0.12%	0.014%
53	7.969	2148	2155	2163	rVB6	2906	4350	0.27%	0.034%
54	8.014	2166	2169	2173	rVB3	385	293	0.02%	0.002%
55	8.082	2179	2190	2226	rBV	447637	792737	49.13%	6.120%
56	8.307	2258	2260	2265	rVB4	587	349	0.02%	0.003%
57	8.407	2287	2291	2293	rBV3	396	292	0.02%	0.002%
58	8.644	2363	2365	2370	rVV3	342	287	0.02%	0.002%
59	8.680	2374	2376	2381	rVB2	483	455	0.03%	0.004%
60	8.767	2400	2403	2406	rBV3	459	302	0.02%	0.002%
61	8.789	2406	2410	2413	rBV3	285	283	0.02%	0.002%
62	8.844	2413	2427	2467	rBV	742855	1234975	76.54%	9.534%
63	9.005	2473	2477	2486	rVB3	3894	4994	0.31%	0.039%
64	9.133	2509	2517	2529	rVV3	3413	5691	0.35%	0.044%
65	9.297	2562	2568	2570	rBV4	469	478	0.03%	0.004%
66	9.542	2635	2644	2645	rBV2	4132	4893	0.30%	0.038%
67	9.722	2696	2700	2702	rBV3	701	608	0.04%	0.005%
68	9.863	2741	2744	2747	rVB2	414	308	0.02%	0.002%
69	9.924	2754	2763	2772	rVV2	3785	5531	0.34%	0.043%
70	10.075	2800	2810	2817	rBV5	1665	2775	0.17%	0.021%
71	10.114	2818	2822	2825	rBV3	288	281	0.02%	0.002%
72	10.207	2835	2851	2876	rBV	537089	838437	51.96%	6.473%
73	10.336	2888	2891	2899	rVB3	394	367	0.02%	0.003%
74	10.448	2923	2926	2933	rVB4	439	420	0.03%	0.003%
75	10.484	2933	2937	2939	rBV2	309	270	0.02%	0.002%
76	10.532	2943	2952	2962	rVV	4177	6446	0.40%	0.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029416.D
 Acq On : 07 Dec 2022 14:45
 Operator : SY/MD
 Sample : VV1207WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK290

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.722	3007	3011	3016	rVB3	333	309	0.02%	0.002%
78	10.841	3045	3048	3053	rBV3	439	485	0.03%	0.004%
79	10.902	3060	3067	3079	rVB2	4617	6755	0.42%	0.052%
80	11.021	3100	3104	3106	rBV	498	326	0.02%	0.003%
81	11.120	3133	3135	3142	rVB3	496	473	0.03%	0.004%
82	11.172	3142	3151	3160	rBV2	5597	8884	0.55%	0.069%
83	11.239	3160	3172	3198	rVV	836494	1280776	79.38%	9.888%
84	11.345	3203	3205	3210	rVB3	701	490	0.03%	0.004%
85	11.529	3259	3262	3267	rVB4	410	396	0.02%	0.003%
86	11.612	3275	3288	3308	rBV	834030	1313444	81.40%	10.140%
87	11.802	3342	3347	3351	rBV3	422	405	0.03%	0.003%
88	11.995	3405	3407	3412	rVB2	477	351	0.02%	0.003%
89	12.021	3412	3415	3419	rVB2	464	336	0.02%	0.003%
90	12.049	3419	3424	3428	rBV4	394	472	0.03%	0.004%
91	12.152	3453	3456	3460	rVB3	447	300	0.02%	0.002%
92	12.210	3469	3474	3476	rBV3	479	407	0.03%	0.003%
93	12.384	3525	3528	3532	rBV4	476	349	0.02%	0.003%
94	12.583	3587	3590	3594	rVB3	562	381	0.02%	0.003%
95	12.635	3595	3606	3616	rBV3	6989	10488	0.65%	0.081%
96	13.156	3765	3768	3772	rBV2	561	385	0.02%	0.003%
97	13.252	3788	3798	3810	rBV3	9814	15620	0.97%	0.121%
98	13.397	3840	3843	3844	rBV2	488	304	0.02%	0.002%
99	13.493	3865	3873	3886	rBV	17299	29131	1.81%	0.225%
100	13.731	3938	3947	3960	rBV3	11597	18972	1.18%	0.146%




Sum of corrected areas: 12953245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029416.D
Acq On : 07 Dec 2022 14:45
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK290

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

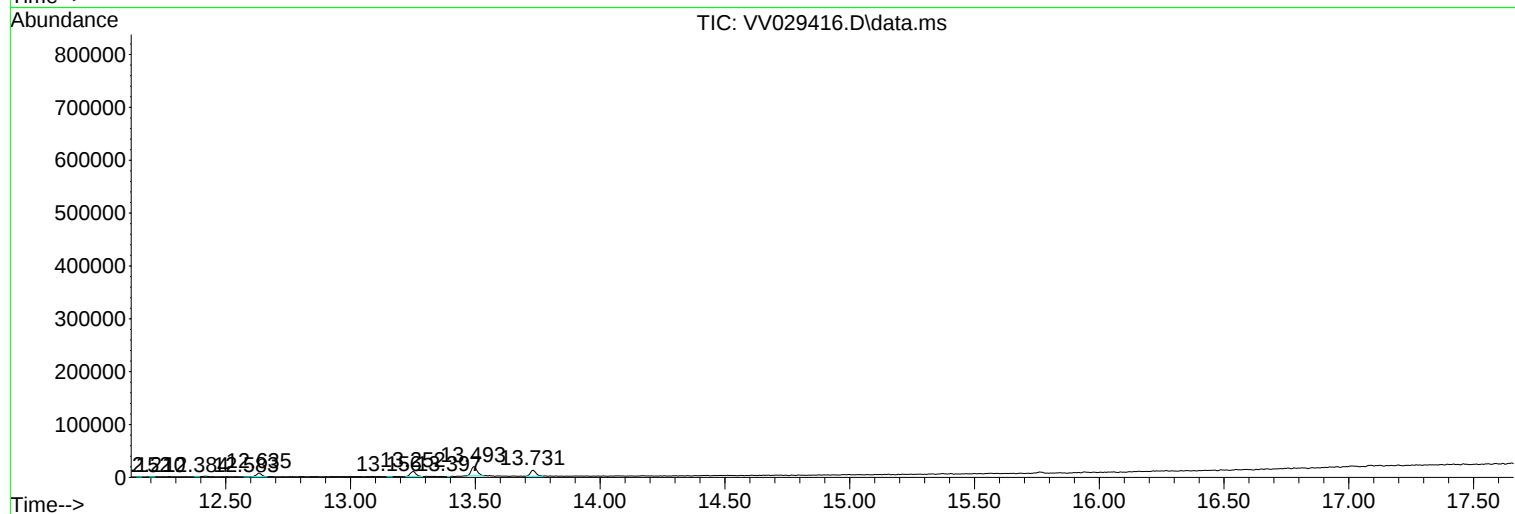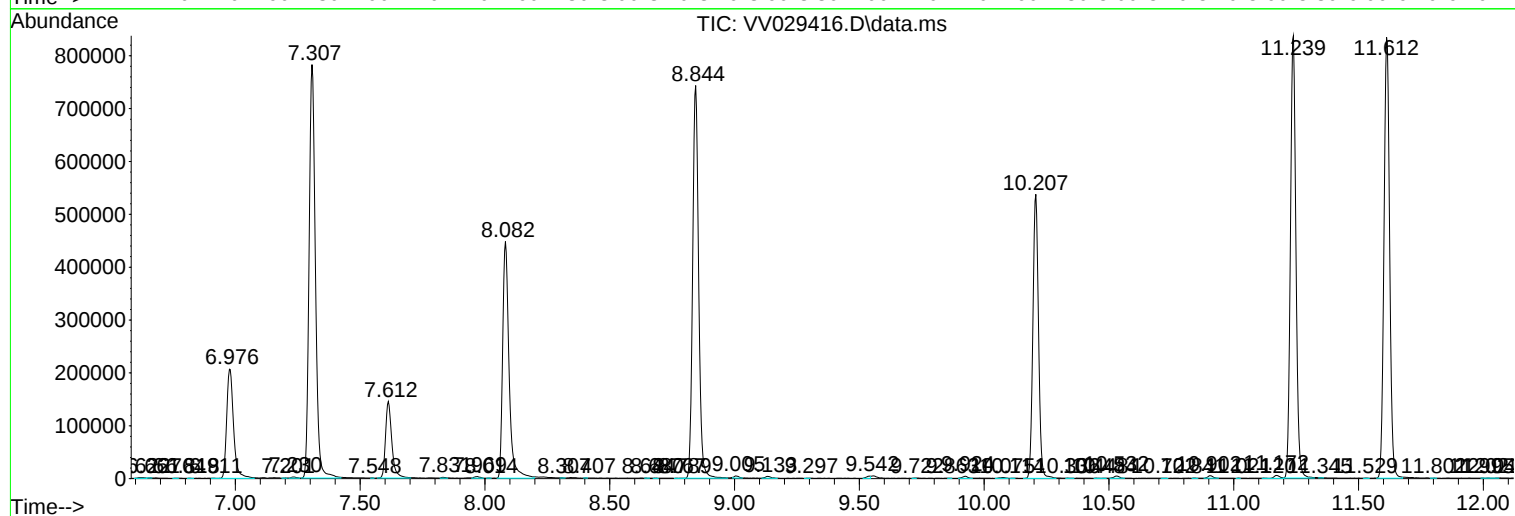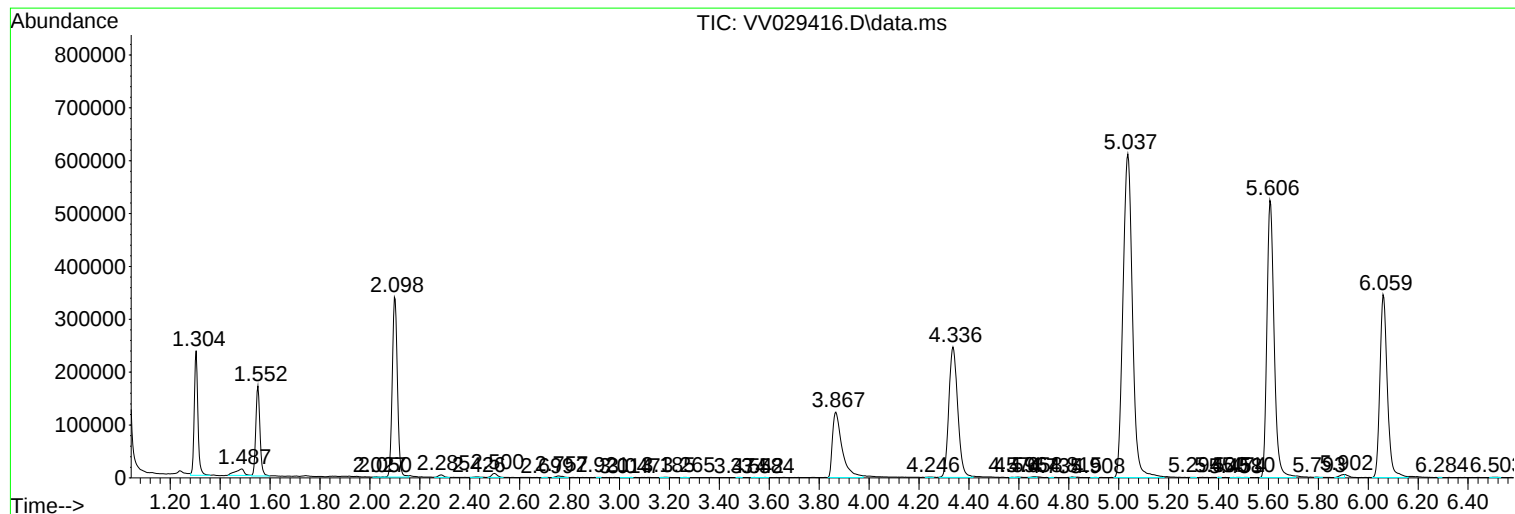

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029416.D
Acq On : 07 Dec 2022 14:45
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK290

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029416.D
Acq On : 07 Dec 2022 14:45
Operator : SY/MD
Sample : VV1207WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK290

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------