

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029417.D
 Acq On : 07 Dec 2022 15:10
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	219403	219614	13.46%	1.698%
2	1.551	151	159	182	rVB	166251	197510	12.10%	1.527%
3	1.902	266	268	272	rBV3	763	620	0.04%	0.005%
4	2.101	318	330	345	rBV	341348	490347	30.05%	3.791%
5	2.285	381	387	397	rVB2	3699	5427	0.33%	0.042%
6	2.500	443	454	467	rVB	8556	14046	0.86%	0.109%
7	2.600	482	485	486	rBV2	515	283	0.02%	0.002%
8	2.670	504	507	510	rBV	454	290	0.02%	0.002%
9	2.757	526	534	545	rVV7	2451	4749	0.29%	0.037%
10	2.973	597	601	608	rBV3	284	329	0.02%	0.003%
11	3.185	660	667	676	rVB2	825	1187	0.07%	0.009%
12	3.281	691	697	700	rBV3	276	268	0.02%	0.002%
13	3.484	757	760	765	rVB3	291	267	0.02%	0.002%
14	3.677	816	820	828	rVB2	199	255	0.02%	0.002%
15	3.728	829	836	840	rBV	331	331	0.02%	0.003%
16	3.867	869	879	922	rBV	131473	358821	21.99%	2.774%
17	4.220	985	989	992	rBV2	458	356	0.02%	0.003%
18	4.336	1007	1025	1054	rBV	258915	631943	38.73%	4.885%
19	4.600	1103	1107	1115	rVB7	1135	1863	0.11%	0.014%
20	4.661	1123	1126	1138	rVB8	1071	1896	0.12%	0.015%
21	4.802	1165	1170	1172	rBV	620	551	0.03%	0.004%
22	4.818	1172	1175	1176	rBV2	442	268	0.02%	0.002%
23	5.037	1225	1243	1280	rBV2	622301	1631811	100.00%	12.615%
24	5.230	1302	1303	1308	rVB2	582	338	0.02%	0.003%
25	5.320	1329	1331	1339	rVB3	393	408	0.03%	0.003%
26	5.355	1339	1342	1347	rBV3	244	280	0.02%	0.002%
27	5.397	1352	1355	1357	rBV	458	256	0.02%	0.002%
28	5.432	1361	1366	1370	rVB3	391	481	0.03%	0.004%
29	5.455	1370	1373	1375	rBV2	352	290	0.02%	0.002%
30	5.497	1384	1386	1391	rVB3	621	498	0.03%	0.004%
31	5.519	1391	1393	1398	rBV2	360	322	0.02%	0.002%
32	5.606	1406	1420	1451	rBV	520308	1058886	64.89%	8.186%
33	5.899	1501	1511	1524	rVB8	5551	12236	0.75%	0.095%
34	6.059	1546	1561	1594	rBV	348894	724636	44.41%	5.602%
35	6.252	1618	1621	1624	rVB3	358	242	0.01%	0.002%
36	6.410	1667	1670	1676	rVB2	221	249	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029417.D
 Acq On : 07 Dec 2022 15:10
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.439	1676	1679	1682	rBV2	410	304	0.02%	0.002%
38	6.506	1690	1700	1702	rBV3	878	1165	0.07%	0.009%
39	6.551	1711	1714	1717	rVB3	417	270	0.02%	0.002%
40	6.574	1717	1721	1725	rVB2	367	286	0.02%	0.002%
41	6.600	1725	1729	1731	rBV3	583	433	0.03%	0.003%
42	6.625	1731	1737	1739	rBV3	1070	1192	0.07%	0.009%
43	6.979	1835	1847	1876	rBV	213015	392932	24.08%	3.038%
44	7.143	1894	1898	1900	rBV3	844	681	0.04%	0.005%
45	7.233	1920	1926	1936	rVB9	1745	2903	0.18%	0.022%
46	7.307	1936	1949	1986	rBV	787301	1385463	84.90%	10.710%
47	7.612	2033	2044	2072	rBV	149452	257852	15.80%	1.993%
48	7.834	2108	2113	2114	rBV4	883	824	0.05%	0.006%
49	7.886	2126	2129	2135	rBV4	394	391	0.02%	0.003%
50	7.918	2136	2139	2140	rBV2	504	269	0.02%	0.002%
51	7.969	2149	2155	2162	rVB4	1905	2786	0.17%	0.022%
52	8.082	2179	2190	2220	rBV	467236	828992	50.80%	6.408%
53	8.345	2266	2272	2280	rVB6	1014	1699	0.10%	0.013%
54	8.407	2289	2291	2296	rVB4	687	466	0.03%	0.004%
55	8.439	2296	2301	2307	rBV5	466	455	0.03%	0.004%
56	8.599	2349	2351	2355	rVB3	503	238	0.01%	0.002%
57	8.683	2374	2377	2380	rVB2	327	242	0.01%	0.002%
58	8.844	2414	2427	2467	rVV	759764	1239947	75.99%	9.585%
59	9.008	2471	2478	2490	rVB2	3618	6235	0.38%	0.048%
60	9.133	2508	2517	2529	rVV3	3252	5135	0.31%	0.040%
61	9.188	2531	2534	2538	rVB3	377	329	0.02%	0.003%
62	9.426	2603	2608	2613	rBV3	324	283	0.02%	0.002%
63	9.490	2624	2628	2631	rVB3	415	365	0.02%	0.003%
64	9.542	2635	2644	2649	rBV3	3762	7059	0.43%	0.055%
65	9.619	2664	2668	2671	rBV	323	322	0.02%	0.002%
66	9.722	2691	2700	2707	rVB5	804	1198	0.07%	0.009%
67	9.796	2720	2723	2726	rBV3	429	320	0.02%	0.002%
68	9.924	2755	2763	2772	rVB2	3600	5556	0.34%	0.043%
69	10.037	2794	2798	2801	rVB	529	364	0.02%	0.003%
70	10.072	2805	2809	2812	rBV2	512	342	0.02%	0.003%
71	10.107	2818	2820	2824	rBV2	444	260	0.02%	0.002%
72	10.207	2838	2851	2867	rBV	552221	865277	53.03%	6.689%
73	10.374	2900	2903	2909	rBV4	730	630	0.04%	0.005%
74	10.461	2926	2930	2935	rBV4	332	363	0.02%	0.003%
75	10.532	2944	2952	2962	rBV	3892	5460	0.33%	0.042%
76	10.802	3032	3036	3038	rBV2	400	311	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
 Data File : VV029417.D
 Acq On : 07 Dec 2022 15:10
 Operator : SY/MD
 Sample : VV1207WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK291

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.844	3046	3049	3054	rVB3	516	350	0.02%	0.003%
78	10.905	3060	3068	3076	rBV3	3929	5412	0.33%	0.042%
79	11.172	3143	3151	3159	rBV5	4177	6414	0.39%	0.050%
80	11.236	3159	3171	3193	rBV	806177	1229819	75.37%	9.507%
81	11.461	3239	3241	3245	rVB2	447	257	0.02%	0.002%
82	11.612	3274	3288	3310	rBV	801800	1260721	77.26%	9.746%
83	11.754	3329	3332	3335	rBV3	470	286	0.02%	0.002%
84	11.821	3349	3353	3356	rBV3	372	290	0.02%	0.002%
85	11.914	3378	3382	3385	rBV2	448	331	0.02%	0.003%
86	11.950	3390	3393	3395	rBV2	458	301	0.02%	0.002%
87	12.130	3445	3449	3455	rVB3	554	535	0.03%	0.004%
88	12.175	3455	3463	3465	rBV3	543	602	0.04%	0.005%
89	12.220	3474	3477	3485	rBV4	560	797	0.05%	0.006%
90	12.281	3490	3496	3499	rBV4	604	434	0.03%	0.003%
91	12.332	3510	3512	3515	rVB2	513	269	0.02%	0.002%
92	12.413	3534	3537	3541	rVV4	580	538	0.03%	0.004%
93	12.458	3547	3551	3554	rBV4	260	261	0.02%	0.002%
94	12.638	3595	3607	3615	rBV5	4549	7137	0.44%	0.055%
95	12.799	3655	3657	3666	rVB4	480	482	0.03%	0.004%
96	12.844	3667	3671	3672	rBV	367	265	0.02%	0.002%
97	12.876	3679	3681	3684	rBV2	357	281	0.02%	0.002%
98	13.249	3790	3797	3808	rVB4	6835	10256	0.63%	0.079%
99	13.496	3866	3874	3892	rVB	10025	17743	1.09%	0.137%
100	13.734	3940	3948	3962	rVB3	6407	10383	0.64%	0.080%




Sum of corrected areas: 12935917

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029417.D
Acq On : 07 Dec 2022 15:10
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

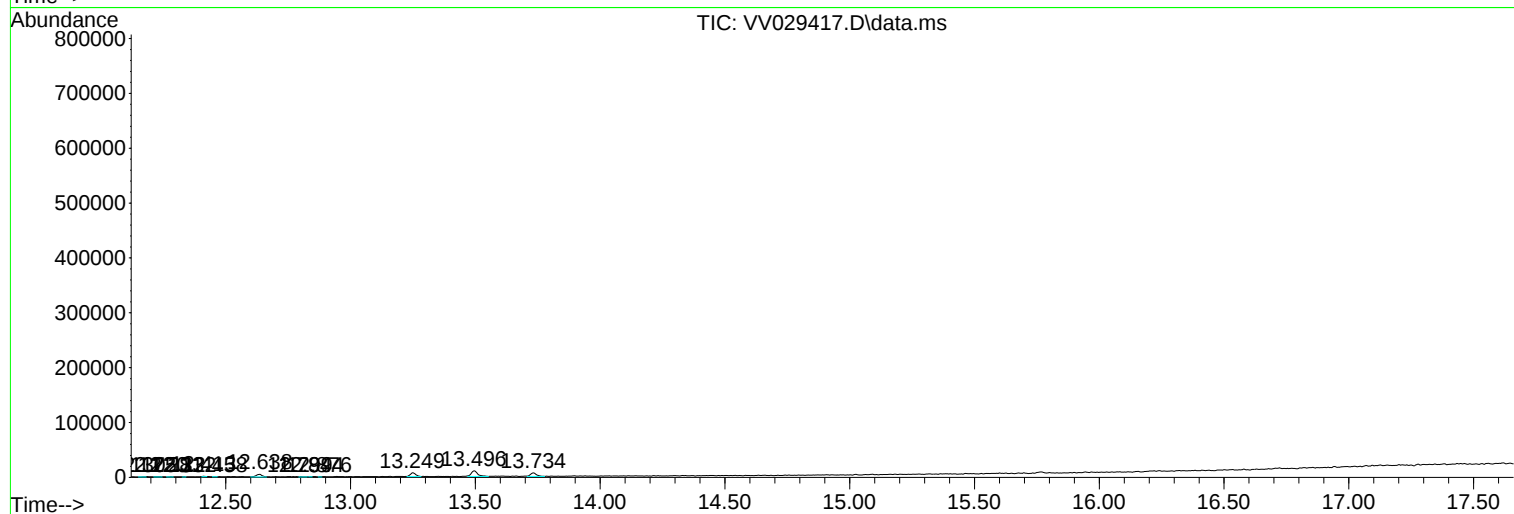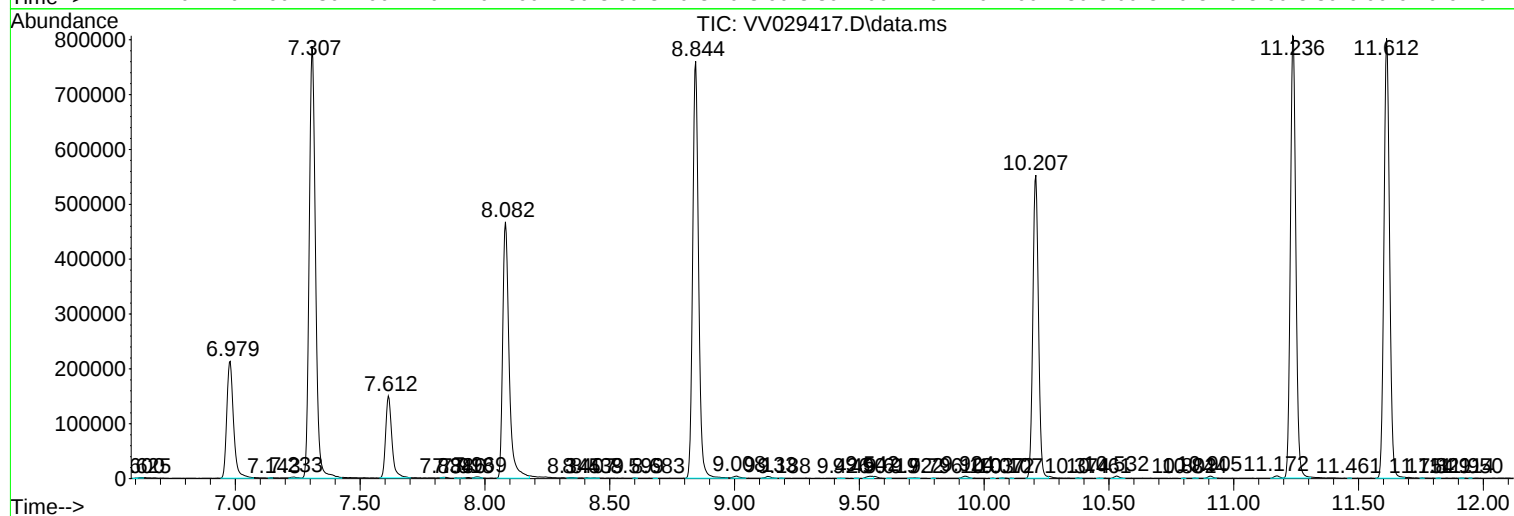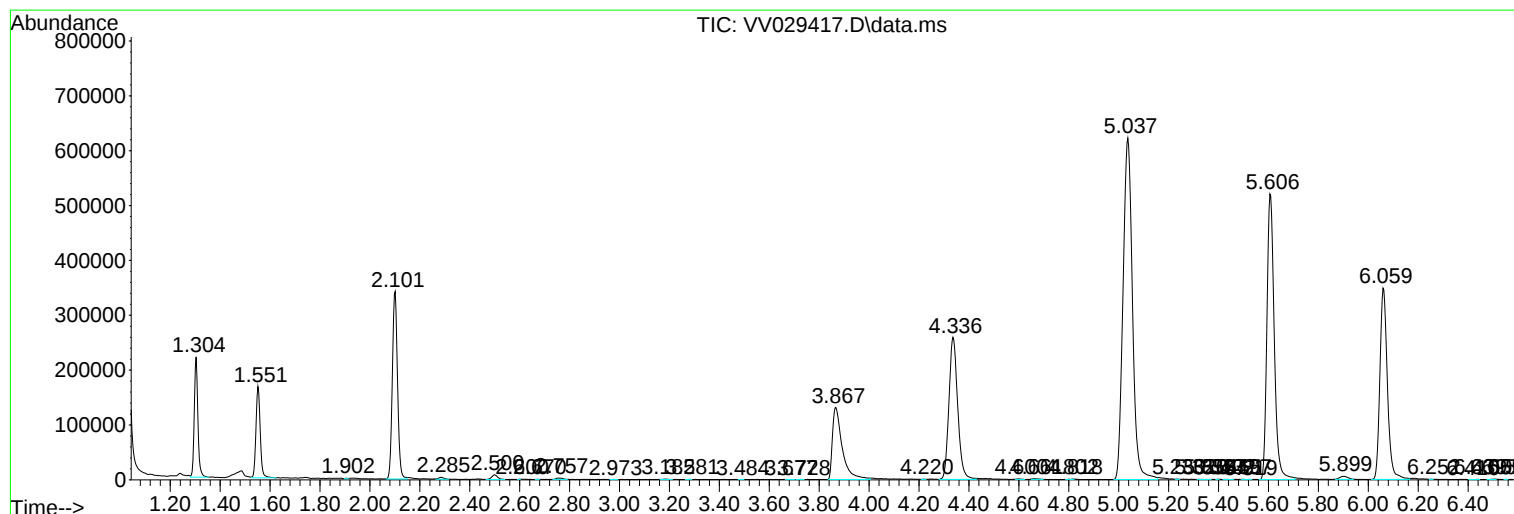

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029417.D
Acq On : 07 Dec 2022 15:10
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120722\
Data File : VV029417.D
Acq On : 07 Dec 2022 15:10
Operator : SY/MD
Sample : VV1207WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK291

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
